

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
 Data File : VV020696.D
 Acq On : 22 Mar 2021 12:47
 Operator : SY/MD
 Sample : VV0322MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

Signal : TIC: VV020696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	78	83	95	rVB	283695	274535	16.27%	2.095%
2	1.571	159	165	173	rVB	198686	214748	12.73%	1.639%
3	2.108	324	332	356	rVB	422790	636054	37.70%	4.853%
4	2.365	410	412	414	rBV3	3641	2226	0.13%	0.017%
5	2.571	474	476	479	rBV4	3102	2029	0.12%	0.015%
6	2.587	479	481	486	rVB5	3851	2502	0.15%	0.019%
7	2.838	556	559	563	rVB5	3818	2911	0.17%	0.022%
8	2.860	563	566	569	rBV4	3721	2980	0.18%	0.023%
9	2.918	579	584	587	rVB6	4003	3464	0.21%	0.026%
10	2.937	589	590	592	rBV2	3460	1692	0.10%	0.013%
11	3.021	612	616	617	rBV4	2793	1869	0.11%	0.014%
12	3.089	636	637	640	rBV3	3074	1618	0.10%	0.012%
13	3.134	648	651	652	rBV3	4087	2334	0.14%	0.018%
14	3.355	717	720	724	rBV6	2652	2534	0.15%	0.019%
15	3.429	741	743	746	rVV4	3671	2476	0.15%	0.019%
16	3.465	750	754	755	rVV4	3589	2019	0.12%	0.015%
17	3.484	757	760	761	rVV3	3084	1885	0.11%	0.014%
18	3.506	765	767	769	rBV3	3564	1805	0.11%	0.014%
19	3.597	793	795	797	rBV3	3288	2043	0.12%	0.016%
20	3.854	872	875	877	rBV3	3102	2339	0.14%	0.018%
21	3.896	878	888	913	rBV2	112161	336844	19.96%	2.570%
22	4.352	1018	1030	1050	rVB	292130	679758	40.29%	5.187%
23	4.783	1161	1164	1167	rBV4	3842	3031	0.18%	0.023%
24	4.825	1175	1177	1183	rVB7	2774	2248	0.13%	0.017%
25	4.934	1208	1211	1213	rBV4	3088	2186	0.13%	0.017%
26	5.050	1232	1247	1269	rBV2	671038	1687273	100.00%	12.874%
27	5.465	1374	1376	1378	rBV3	3282	2186	0.13%	0.017%
28	5.619	1412	1424	1446	rBV	506326	1019518	60.42%	7.779%
29	5.912	1513	1515	1518	rBV4	4585	2095	0.12%	0.016%
30	6.072	1554	1565	1584	rBV2	377773	747303	44.29%	5.702%
31	6.407	1667	1669	1673	rBV5	4424	3759	0.22%	0.029%
32	6.651	1742	1745	1747	rBV4	3777	2795	0.17%	0.021%
33	6.989	1841	1850	1870	rBV	203144	363986	21.57%	2.777%
34	7.133	1893	1895	1897	rBV3	2957	1581	0.09%	0.012%
35	7.320	1941	1953	1970	rBV	771957	1325936	78.58%	10.117%
36	7.625	2040	2048	2065	rBV2	142933	241534	14.32%	1.843%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
 Data File : VV020696.D
 Acq On : 22 Mar 2021 12:47
 Operator : SY/MD
 Sample : VV0322MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

37	7.989	2152	2161	2167	rVB2	5744	9208	0.55%	0.070%
38	8.092	2184	2193	2215	rBV	453488	780846	46.28%	5.958%
39	8.371	2276	2280	2284	rBV7	4868	3960	0.23%	0.030%
40	8.535	2326	2331	2334	rBV6	3890	3005	0.18%	0.023%

41	8.648	2363	2366	2367	rBV3	5288	3300	0.20%	0.025%
42	8.731	2389	2392	2394	rBV4	3881	2468	0.15%	0.019%
43	8.767	2401	2403	2406	rBV4	3224	2464	0.15%	0.019%
44	8.857	2418	2431	2451	rBV	803469	1303812	77.27%	9.948%
45	9.249	2549	2553	2554	rBV4	2798	1866	0.11%	0.014%

46	9.487	2624	2627	2632	rBV6	3269	3879	0.23%	0.030%
47	9.635	2671	2673	2677	rBV5	3234	2704	0.16%	0.021%
48	9.725	2699	2701	2704	rBV4	2616	2190	0.13%	0.017%
49	9.763	2711	2713	2715	rBV3	2985	1861	0.11%	0.014%
50	9.799	2720	2724	2725	rBV4	2896	2183	0.13%	0.017%

51	9.825	2730	2732	2735	rVB4	3670	1882	0.11%	0.014%
52	9.844	2735	2738	2741	rBV5	2794	2314	0.14%	0.018%
53	10.005	2785	2788	2791	rVB4	2666	1855	0.11%	0.014%
54	10.143	2827	2831	2835	rBV6	3978	3821	0.23%	0.029%
55	10.220	2844	2855	2872	rBV	535102	832942	49.37%	6.356%

56	10.358	2894	2898	2899	rBV4	3064	1645	0.10%	0.013%
57	10.387	2905	2907	2913	rVB7	4645	4097	0.24%	0.031%
58	10.432	2918	2921	2924	rBV4	3873	2439	0.14%	0.019%
59	10.545	2953	2956	2958	rBV4	3020	1830	0.11%	0.014%
60	10.651	2985	2989	2991	rBV5	3091	1868	0.11%	0.014%

61	10.825	3038	3043	3047	rVB7	4085	3768	0.22%	0.029%
62	10.921	3069	3073	3075	rBV5	5411	4237	0.25%	0.032%
63	11.014	3098	3102	3105	rBV5	2269	1800	0.11%	0.014%
64	11.088	3121	3125	3128	rBV5	4323	3659	0.22%	0.028%
65	11.255	3164	3177	3194	rBV	784152	1219097	72.25%	9.302%

66	11.583	3277	3279	3282	rBV4	3280	1806	0.11%	0.014%
67	11.628	3282	3293	3309	rVV	779734	1214280	71.97%	9.265%
68	11.706	3315	3317	3322	rVB6	4296	3150	0.19%	0.024%
69	12.030	3412	3418	3422	rBV9	4365	5618	0.33%	0.043%
70	12.210	3472	3474	3476	rBV3	2999	1906	0.11%	0.015%

71	12.300	3496	3502	3507	rBV10	3950	5138	0.30%	0.039%
72	12.558	3579	3582	3585	rBV4	3189	2383	0.14%	0.018%
73	12.728	3632	3635	3637	rBV4	4221	1979	0.12%	0.015%
74	12.853	3672	3674	3679	rVB6	2741	1839	0.11%	0.014%
75	13.043	3730	3733	3739	rVV8	2776	2570	0.15%	0.020%

76	13.156	3765	3768	3770	rBV4	3649	2470	0.15%	0.019%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
 Data File : VV020696.D
 Acq On : 22 Mar 2021 12:47
 Operator : SY/MD
 Sample : VV0322MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Title : VOC Analysis

77	13.217	3784	3787	3789	rBV3	2177	1858	0.11%	0.014%
78	13.226	3789	3790	3794	rVB4	4037	1602	0.09%	0.012%
79	13.265	3794	3802	3804	rBV9	7657	8780	0.52%	0.067%
80	13.471	3863	3866	3871	rBV7	4525	4337	0.26%	0.033%
81	13.570	3893	3897	3899	rBV5	2235	1595	0.09%	0.012%
82	13.583	3899	3901	3905	rBV5	2692	2083	0.12%	0.016%
83	13.673	3925	3929	3934	rVB8	4859	5889	0.35%	0.045%
84	13.696	3934	3936	3939	rBV4	5093	2815	0.17%	0.021%
85	13.725	3943	3945	3947	rBV3	2983	1814	0.11%	0.014%
86	13.905	3998	4001	4003	rBV4	4098	2430	0.14%	0.019%
87	13.963	4016	4019	4022	rBV5	1813	1826	0.11%	0.014%
88	14.011	4030	4034	4036	rBV4	4072	2791	0.17%	0.021%
89	14.049	4044	4046	4052	rVB7	2720	1677	0.10%	0.013%
90	14.117	4063	4067	4069	rBV4	3407	2361	0.14%	0.018%
91	14.181	4085	4087	4089	rBV3	3364	1800	0.11%	0.014%
92	14.300	4120	4124	4128	rBV7	2884	2879	0.17%	0.022%
93	14.413	4156	4159	4161	rBV4	3186	1844	0.11%	0.014%
94	14.503	4183	4187	4188	rBV4	3519	2175	0.13%	0.017%
95	14.603	4215	4218	4221	rBV5	3665	2347	0.14%	0.018%
96	14.680	4239	4242	4246	rBV5	5000	4458	0.26%	0.034%
97	15.345	4447	4449	4452	rBV4	2755	1739	0.10%	0.013%
98	15.400	4463	4466	4468	rBV4	3368	1776	0.11%	0.014%
99	15.554	4511	4514	4516	rBV4	3867	2359	0.14%	0.018%
100	15.882	4612	4616	4617	rBV4	3224	2357	0.14%	0.018%




Sum of corrected areas: 13105827

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
Data File : VV020696.D
Acq On : 22 Mar 2021 12:47
Operator : SY/MD
Sample : VV0322MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

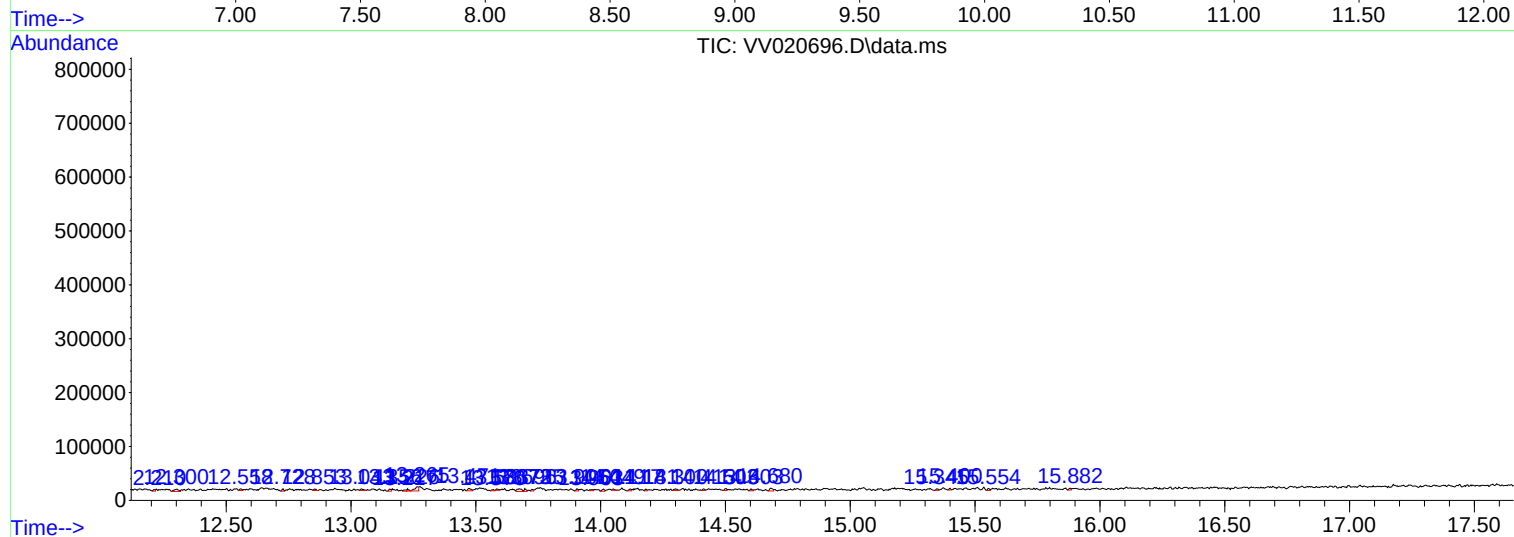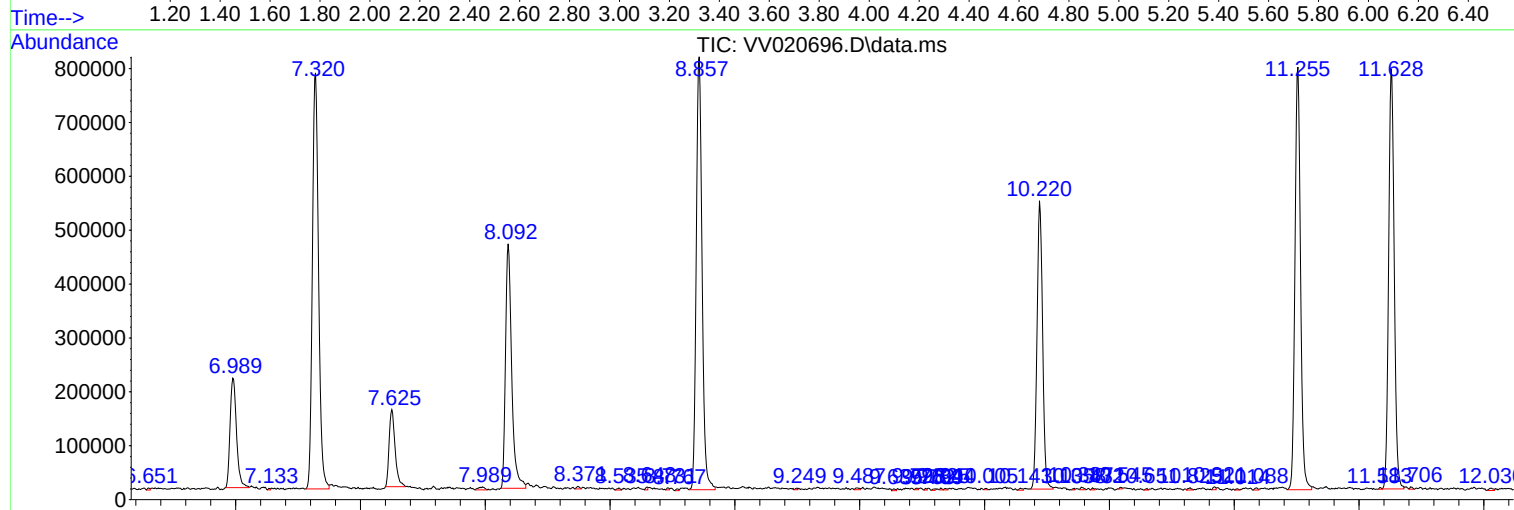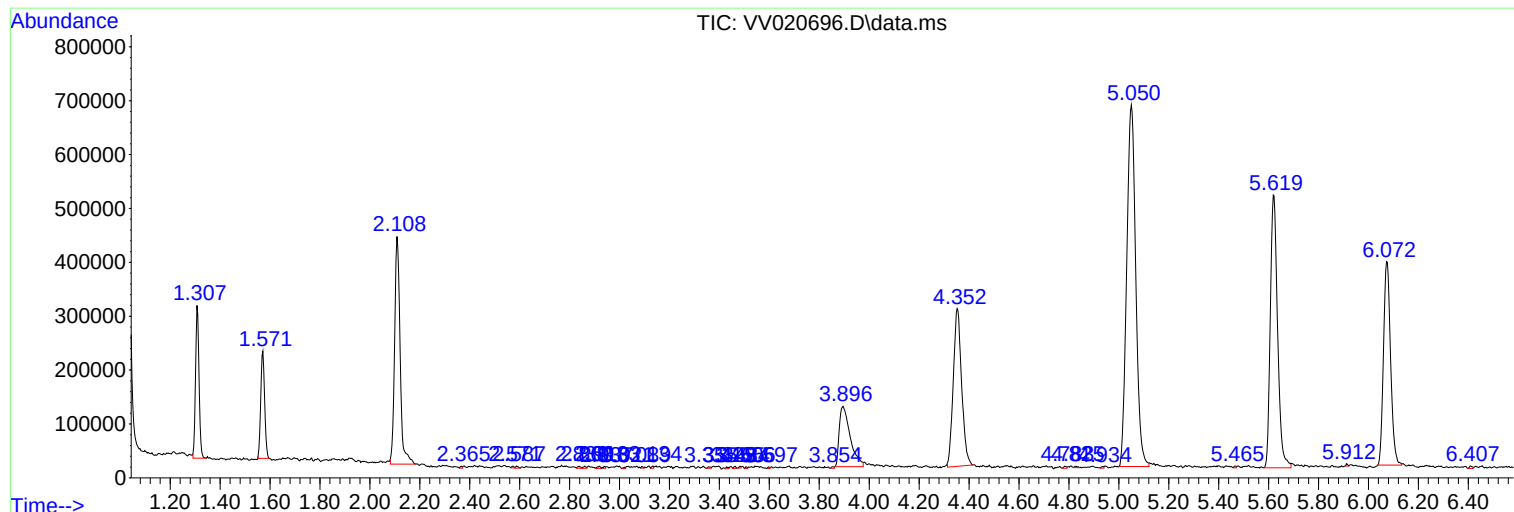

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
Data File : VV020696.D
Acq On : 22 Mar 2021 12:47
Operator : SY/MD
Sample : VV0322MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
Data File : VV020696.D
Acq On : 22 Mar 2021 12:47
Operator : SY/MD
Sample : VV0322MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc