

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
 Data File : VV020697.D
 Acq On : 22 Mar 2021 13:13
 Operator : SY/MD
 Sample : M1685-22ME
 Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4H0ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

Signal : TIC: VV020697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	78	83	101	rVB	228736	281010	9.89%	1.754%
2	2.085	317	325	336	rVB	430690	611583	21.53%	3.816%
3	2.584	477	480	482	rBV4	2360	1938	0.07%	0.012%
4	2.619	487	491	493	rBV5	3414	2827	0.10%	0.018%
5	2.715	519	521	523	rBV3	2269	1458	0.05%	0.009%
6	2.744	527	530	532	rBV4	8513	6258	0.22%	0.039%
7	2.857	562	565	566	rBV3	3215	1501	0.05%	0.009%
8	2.870	566	569	571	rBV3	2507	1758	0.06%	0.011%
9	3.130	648	650	654	rVV5	2872	1920	0.07%	0.012%
10	3.362	720	722	726	rVB4	4114	2620	0.09%	0.016%
11	3.394	728	732	734	rBV5	2485	1771	0.06%	0.011%
12	3.407	734	736	740	rBV4	2502	1676	0.06%	0.010%
13	3.442	743	747	750	rBV5	2213	2191	0.08%	0.014%
14	3.564	783	785	789	rVB5	3623	1837	0.06%	0.011%
15	3.709	826	830	832	rBV4	3923	3156	0.11%	0.020%
16	3.786	852	854	857	rBV3	2597	1562	0.05%	0.010%
17	3.905	876	891	922	rBV2	1116183	2840050	100.00%	17.723%
18	4.346	1015	1028	1047	rBV	269148	672966	23.70%	4.200%
19	4.587	1099	1103	1104	rBV4	3983	2940	0.10%	0.018%
20	4.731	1145	1148	1153	rBV7	3069	3622	0.13%	0.023%
21	4.879	1190	1194	1200	rVB8	4418	4791	0.17%	0.030%
22	4.911	1200	1204	1206	rBV4	2642	2211	0.08%	0.014%
23	4.953	1214	1217	1219	rVB4	3456	1698	0.06%	0.011%
24	5.043	1230	1245	1271	rBV2	718787	1744765	61.43%	10.888%
25	5.464	1370	1376	1378	rBV7	3890	3560	0.13%	0.022%
26	5.493	1383	1385	1386	rBV2	3501	1586	0.06%	0.010%
27	5.616	1412	1423	1442	rBV	536960	1077962	37.96%	6.727%
28	6.069	1553	1564	1584	rBV	377232	773991	27.25%	4.830%
29	6.204	1602	1606	1607	rBV4	3106	2443	0.09%	0.015%
30	6.548	1709	1713	1718	rVB8	4132	4403	0.16%	0.027%
31	6.574	1718	1721	1723	rBV4	2504	2120	0.07%	0.013%
32	6.638	1738	1741	1742	rBV3	4119	2187	0.08%	0.014%
33	6.648	1742	1744	1746	rVV3	2935	1473	0.05%	0.009%
34	6.989	1840	1850	1873	rBV2	196450	394824	13.90%	2.464%
35	7.275	1936	1939	1940	rBV3	3014	1804	0.06%	0.011%
36	7.316	1940	1952	1974	rVV	792238	1411943	49.72%	8.811%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
 Data File : VV020697.D
 Acq On : 22 Mar 2021 13:13
 Operator : SY/MD
 Sample : M1685-22ME
 Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4H0ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Title : VOC Analysis

37	7.625	2038	2048	2072	rBV2	134096	278441	9.80%	1.738%
38	7.760	2087	2090	2091	rBV3	3549	1483	0.05%	0.009%
39	7.863	2119	2122	2124	rBV4	2800	1982	0.07%	0.012%
40	8.130	2187	2205	2227	rBV2	212722	743219	26.17%	4.638%
41	8.580	2341	2345	2349	rBV6	4183	4554	0.16%	0.028%
42	8.644	2363	2365	2368	rBV4	2934	2001	0.07%	0.012%
43	8.751	2395	2398	2401	rBV5	3746	2800	0.10%	0.017%
44	8.857	2420	2431	2454	rBV	786973	1439752	50.69%	8.985%
45	9.021	2480	2482	2484	rBV3	2348	1348	0.05%	0.008%
46	9.214	2535	2542	2544	rBV8	4979	6057	0.21%	0.038%
47	9.291	2564	2566	2569	rVV3	2964	1571	0.06%	0.010%
48	9.329	2576	2578	2581	rBV4	3208	1851	0.07%	0.012%
49	9.416	2603	2605	2606	rBV2	3834	1850	0.07%	0.012%
50	9.538	2640	2643	2646	rBV5	2872	1908	0.07%	0.012%
51	9.632	2670	2672	2675	rVB4	4455	2364	0.08%	0.015%
52	9.673	2681	2685	2689	rBV6	3757	3083	0.11%	0.019%
53	9.718	2697	2699	2702	rBV3	2201	1702	0.06%	0.011%
54	9.741	2702	2706	2707	rBV4	3657	2269	0.08%	0.014%
55	9.828	2729	2733	2734	rBV4	6203	4198	0.15%	0.026%
56	10.053	2798	2803	2805	rBV5	4984	4255	0.15%	0.027%
57	10.230	2847	2858	2871	rBV	476639	824121	29.02%	5.143%
58	10.493	2936	2940	2943	rBV5	3161	2673	0.09%	0.017%
59	10.651	2987	2989	2991	rBV3	3604	1598	0.06%	0.010%
60	10.670	2991	2995	2996	rBV4	3515	2412	0.08%	0.015%
61	10.722	3007	3011	3016	rBV9	4296	3620	0.13%	0.023%
62	10.786	3029	3031	3034	rVB4	3084	1333	0.05%	0.008%
63	10.863	3048	3055	3058	rBV7	4406	4899	0.17%	0.031%
64	10.908	3064	3069	3070	rBV5	4873	3273	0.12%	0.020%
65	10.927	3070	3075	3077	rVV5	3963	4266	0.15%	0.027%
66	10.988	3091	3094	3097	rBV5	5262	3592	0.13%	0.022%
67	11.004	3097	3099	3106	rVV7	3301	2911	0.10%	0.018%
68	11.143	3139	3142	3145	rBV4	3464	3082	0.11%	0.019%
69	11.159	3145	3147	3150	rBV4	3105	2426	0.09%	0.015%
70	11.258	3167	3178	3193	rBV	903057	1396876	49.18%	8.717%
71	11.467	3240	3243	3245	rBV3	3239	2358	0.08%	0.015%
72	11.635	3283	3295	3310	rBV	823715	1317241	46.38%	8.220%
73	12.011	3408	3412	3413	rBV4	1894	1377	0.05%	0.009%
74	12.040	3419	3421	3423	rBV3	4430	2192	0.08%	0.014%
75	12.120	3444	3446	3449	rVB4	4021	2231	0.08%	0.014%
76	12.226	3473	3479	3483	rBV8	3348	3597	0.13%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
 Data File : VV020697.D
 Acq On : 22 Mar 2021 13:13
 Operator : SY/MD
 Sample : M1685-22ME
 Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4H0ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

77	12.303	3501	3503	3506	rBV4	2449	1514	0.05%	0.009%
78	12.329	3508	3511	3512	rBV3	2232	1364	0.05%	0.009%
79	13.033	3727	3730	3733	rBV5	3745	3192	0.11%	0.020%
80	13.249	3793	3797	3800	rBV5	4891	3902	0.14%	0.024%
81	13.384	3837	3839	3844	rBV6	2972	2420	0.09%	0.015%
82	13.458	3858	3862	3865	rVB5	4552	3045	0.11%	0.019%
83	13.474	3865	3867	3870	rBV4	2009	1405	0.05%	0.009%
84	13.512	3877	3879	3882	rVB4	2389	1478	0.05%	0.009%
85	13.590	3901	3903	3904	rBV2	3409	1400	0.05%	0.009%
86	13.635	3914	3917	3919	rBV4	4403	2639	0.09%	0.016%
87	13.866	3987	3989	3992	rBV4	3383	1960	0.07%	0.012%
88	13.882	3992	3994	3996	rBV3	2917	1457	0.05%	0.009%
89	13.924	4003	4007	4010	rBV6	2881	2381	0.08%	0.015%
90	13.998	4025	4030	4032	rBV5	4655	3983	0.14%	0.025%
91	14.191	4088	4090	4092	rBV3	3371	2120	0.07%	0.013%
92	14.265	4111	4113	4115	rVV2	3067	1409	0.05%	0.009%
93	14.580	4209	4211	4213	rBV3	3661	2150	0.08%	0.013%
94	14.692	4244	4246	4252	rBV7	4130	3211	0.11%	0.020%
95	14.737	4257	4260	4263	rBV5	3411	2582	0.09%	0.016%
96	15.081	4364	4367	4369	rBV4	4830	2639	0.09%	0.016%
97	15.496	4494	4496	4500	rBV5	2784	2136	0.08%	0.013%
98	15.721	4564	4566	4567	rBV2	3551	1936	0.07%	0.012%
99	15.985	4645	4648	4650	rBV4	3807	2566	0.09%	0.016%
100	16.229	4722	4724	4727	rBV4	3904	2676	0.09%	0.017%




Sum of corrected areas: 16024736

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
Data File : VV020697.D
Acq On : 22 Mar 2021 13:13
Operator : SY/MD
Sample : M1685-22ME
Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4H0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

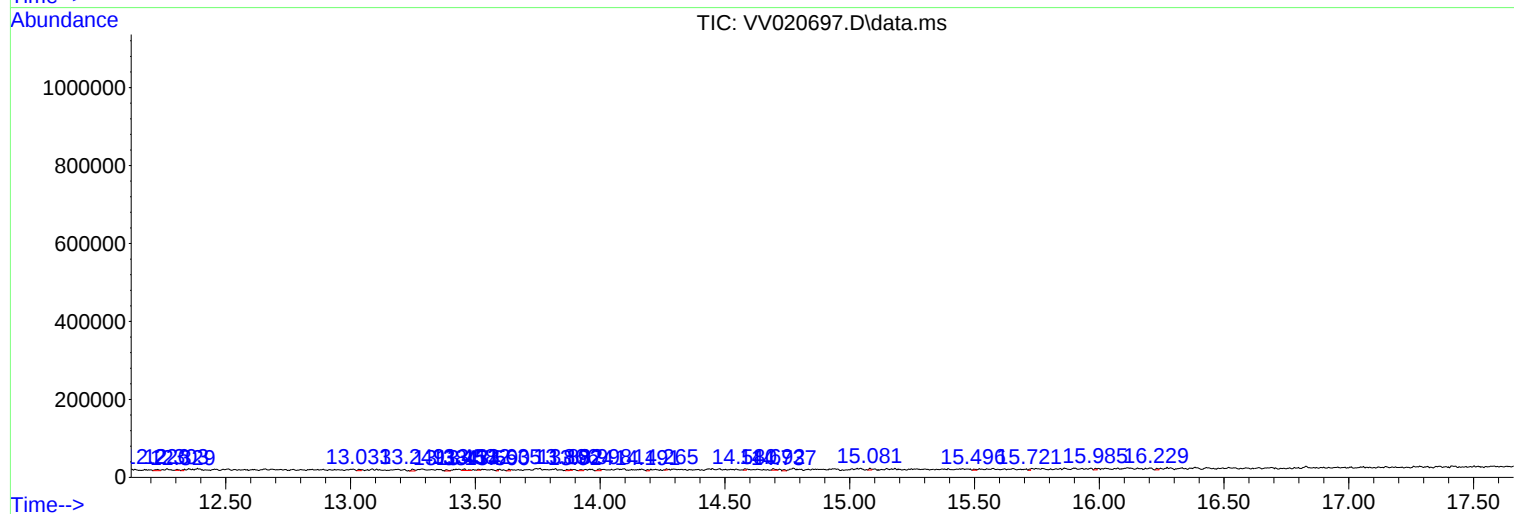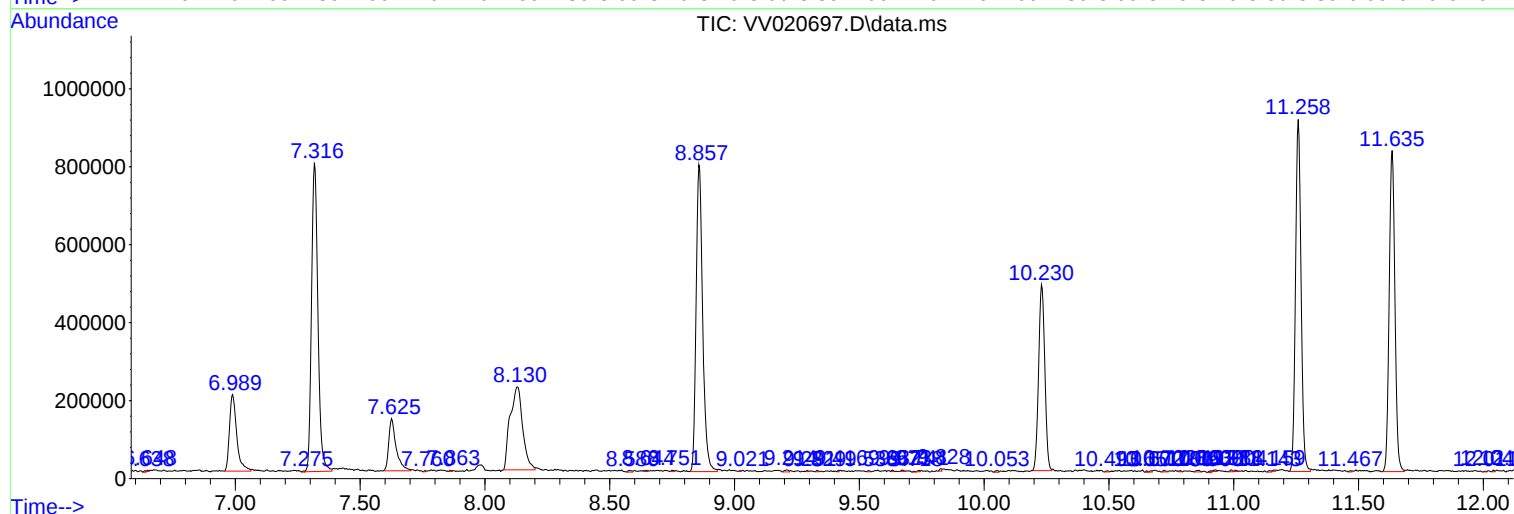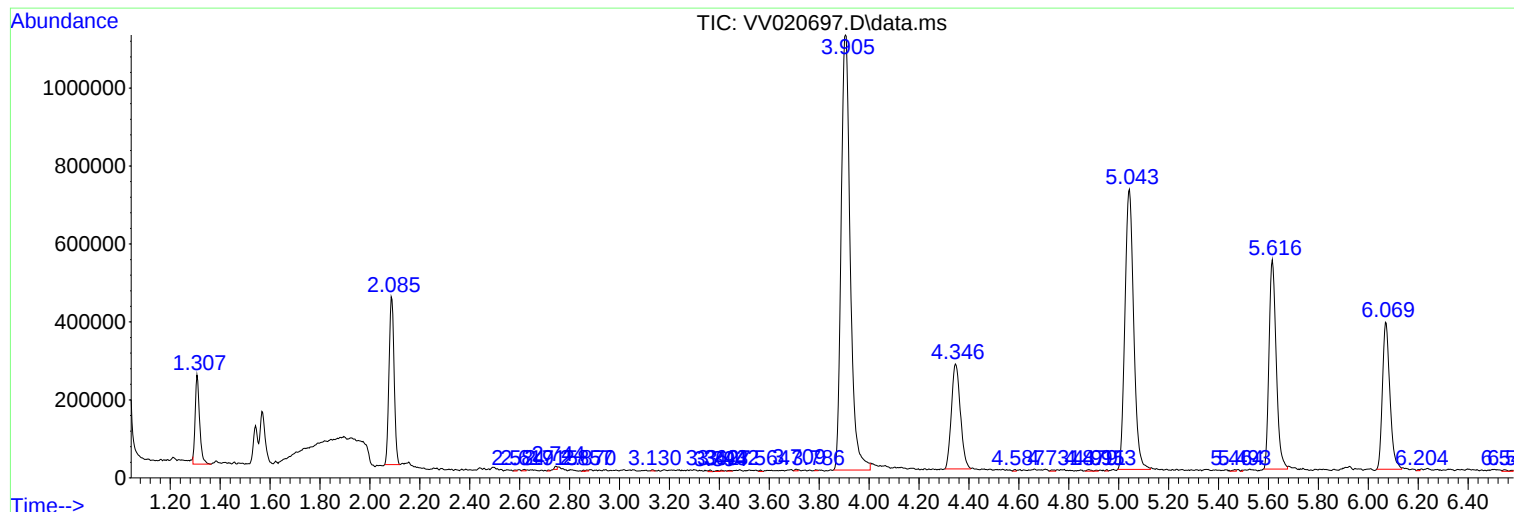

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
Data File : VV020697.D
Acq On : 22 Mar 2021 13:13
Operator : SY/MD
Sample : M1685-22ME
Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4H0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032221\
Data File : VV020697.D
Acq On : 22 Mar 2021 13:13
Operator : SY/MD
Sample : M1685-22ME
Misc : 5.76g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4H0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
