




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030291.D
Acq On : 22 Mar 2023 14:21
Operator : SY/MD
Sample : VV0322WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK317

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:49:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 23 01:48:30 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/23/2023
Supervised By :Mahesh Dadoda 03/23/2023

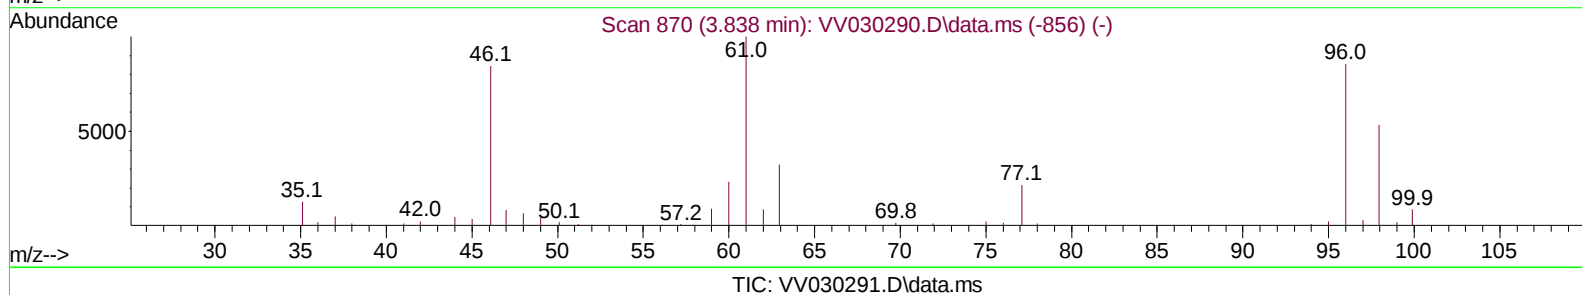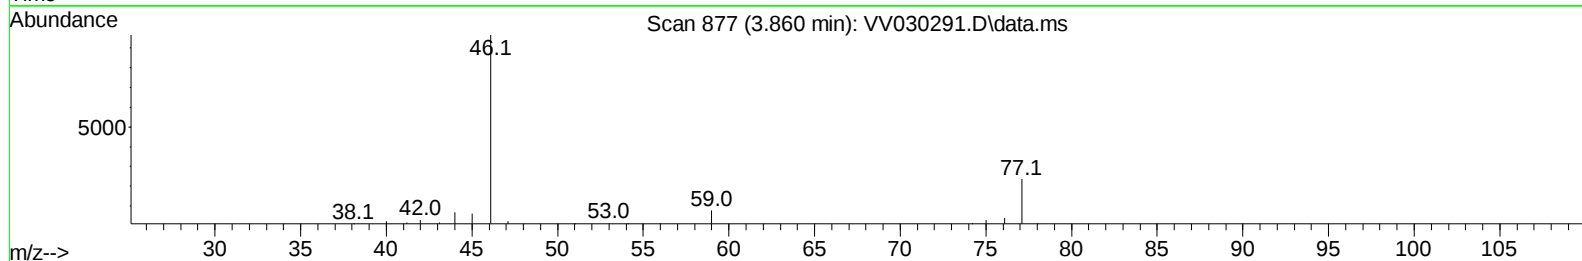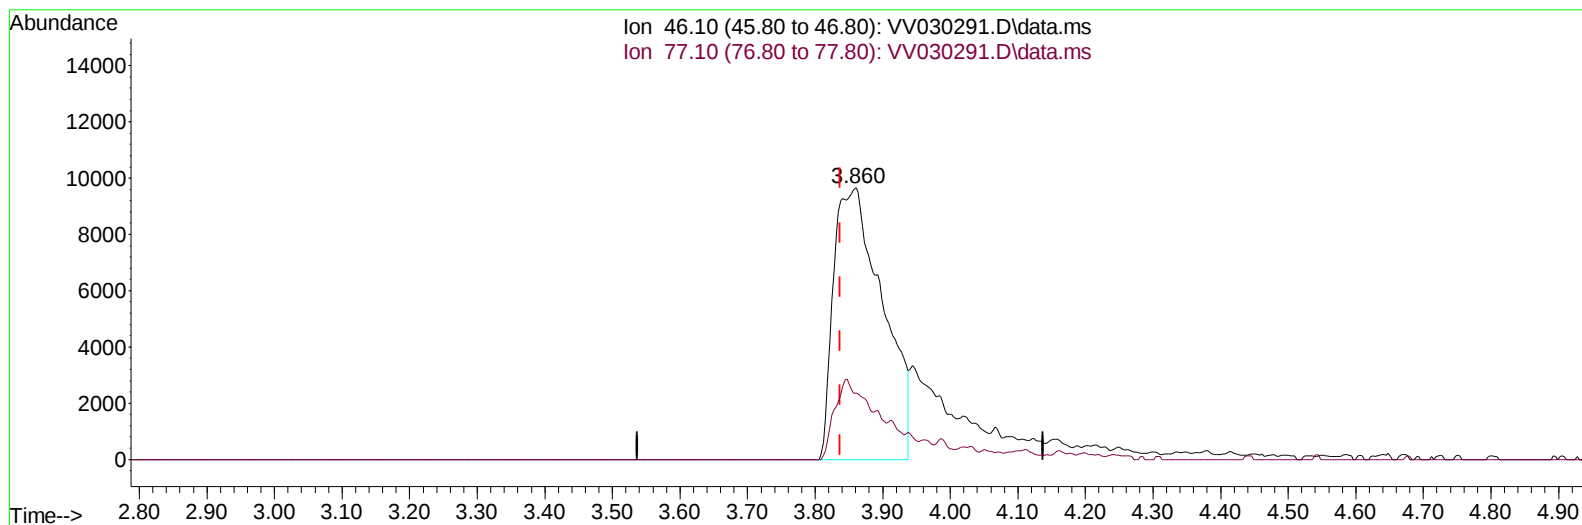

(20) 2-Butanone-d5 (S)

3.860min (+ 0.023) 34.89 ug/L

response 48519

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	18.44#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
 Data File : VV030291.D
 Acq On : 22 Mar 2023 14:21
 Operator : SY/MD
 Sample : VV0322WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK317

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:49:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 23 01:48:30 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/23/2023
 Supervised By :Mahesh Dadoda 03/23/2023

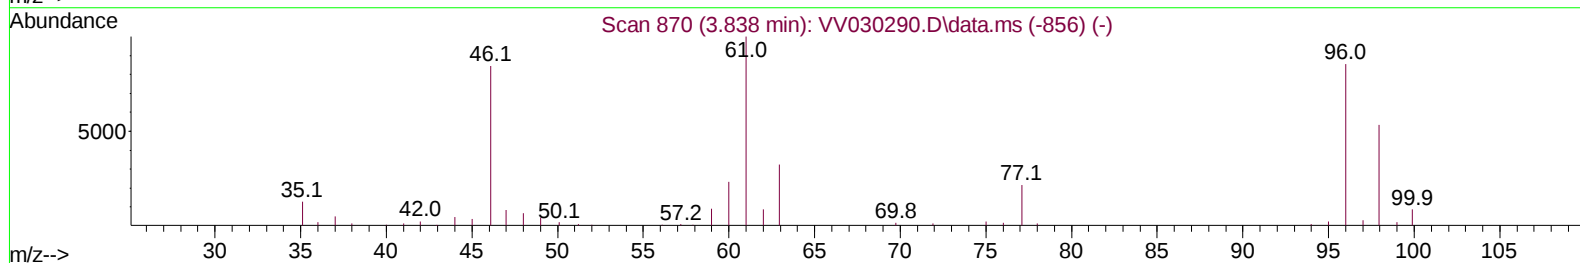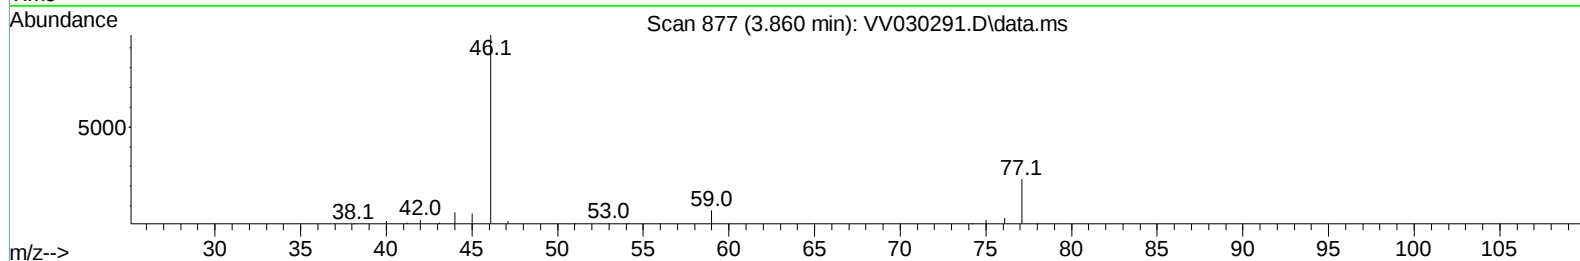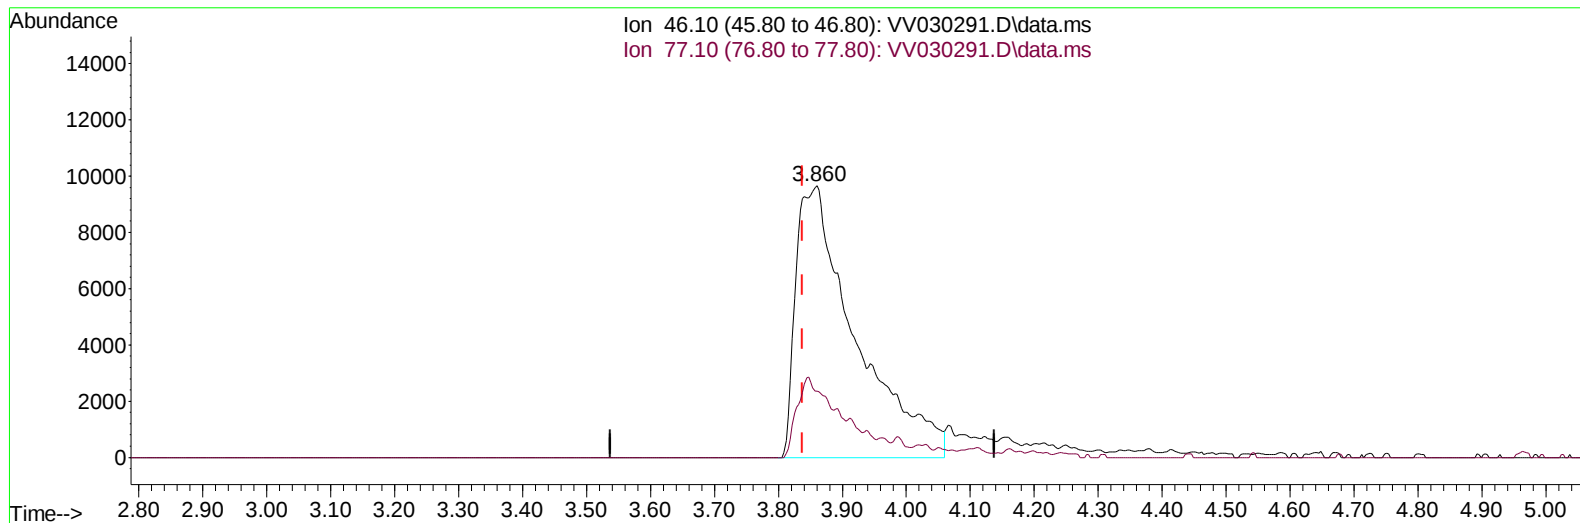

TIC: VV030291.D\data.ms

(20) 2-Butanone-d5 (S)

3.860min (+ 0.023) 44.88 ug/L m

response 62412

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	14.34
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
 Data File : VV030291.D
 Acq On : 22 Mar 2023 14:21
 Operator : SY/MD
 Sample : VV0322WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK317

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:49:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 23 01:48:30 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/23/2023
 Supervised By :Mahesh Dadoda 03/23/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		116571	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117		111656	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		56936	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		36331	4.817	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.400%	
7) Chloroethane-d5	1.536	69		34416	4.861	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.200%	
11) 1,1-Dichloroethene-d2	2.063	63		62717	4.044	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.800%	
20) 2-Butanone-d5	3.860	46		62412m	44.880	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.760%	
24) Chloroform-d	4.262	84		74273	4.820	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%	
26) 1,2-Dichloroethane-d4	4.953	65		38868	6.179	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.600%	
32) Benzene-d6	4.970	84		133060	4.429	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%	
36) 1,2-Dichloropropane-d6	5.998	67		36957	4.089	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	81.800%	
41) Toluene-d8	7.252	98		121429	4.264	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.564	79		14375	4.649	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.000%	
46) 2-Hexanone-d5	8.040	63		54591	42.671	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.340%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		26504	4.122	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.400%	
66) 1,2-Dichlorobenzene-d4	11.571	152		48478	5.032	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.600%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030291.D
Acq On : 22 Mar 2023 14:21
Operator : SY/MD
Sample : VV0322WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK317

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:49:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 23 01:48:30 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/23/2023
Supervised By :Mahesh Dadoda 03/23/2023

