




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
 Data File : VV030293.D
 Acq On : 22 Mar 2023 15:08
 Operator : SY/MD
 Sample : 02003-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBM8

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:49:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 23 01:48:30 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/23/2023
 Supervised By :Mahesh Dadoda 03/23/2023

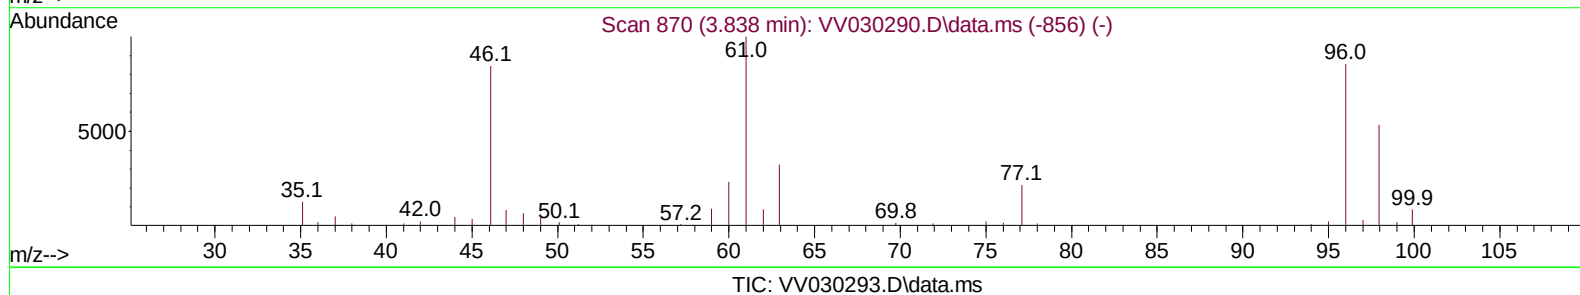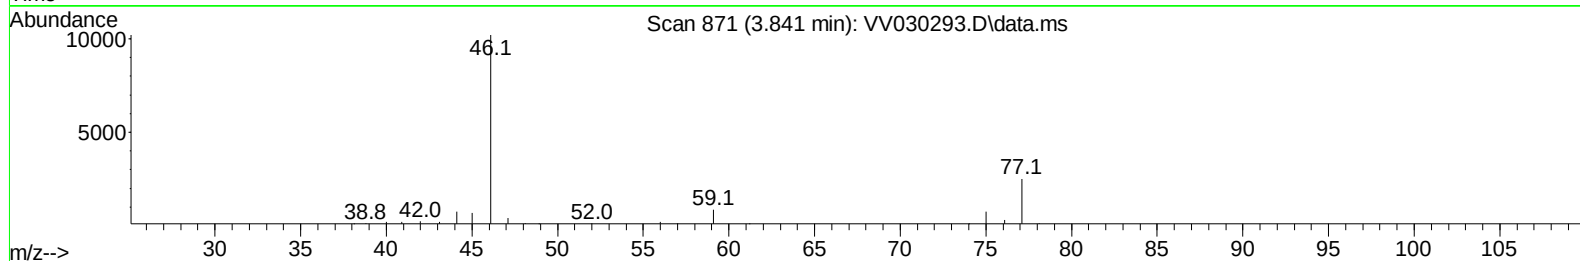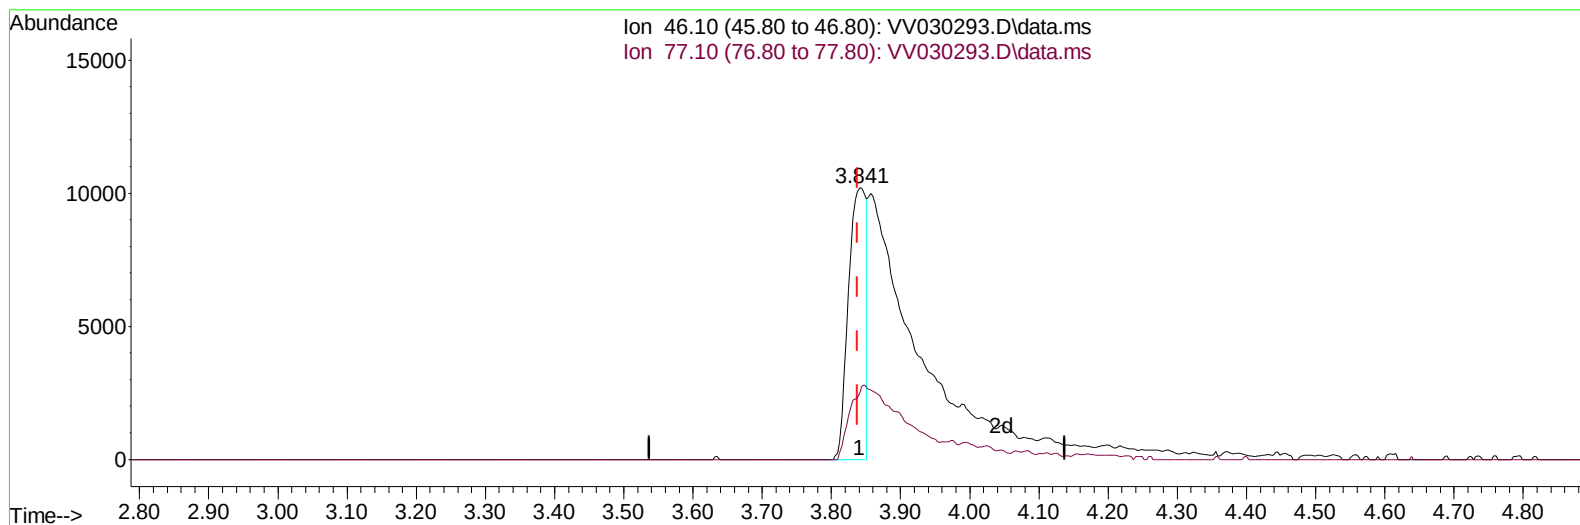

(20) 2-Butanone-d5 (S)

3.841min (+ 0.003) 12.63 ug/L

response 18109

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	80.82#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
 Data File : VV030293.D
 Acq On : 22 Mar 2023 15:08
 Operator : SY/MD
 Sample : 02003-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BM8

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:49:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 23 01:48:30 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/23/2023
 Supervised By :Mahesh Dadoda 03/23/2023

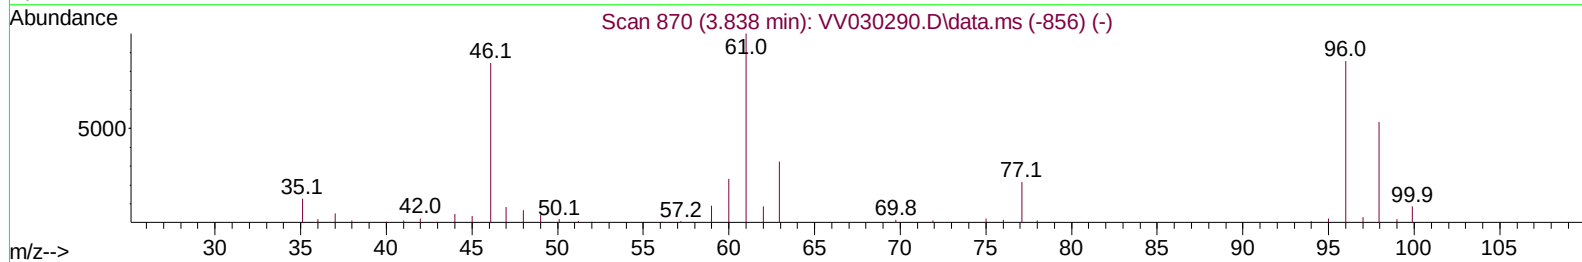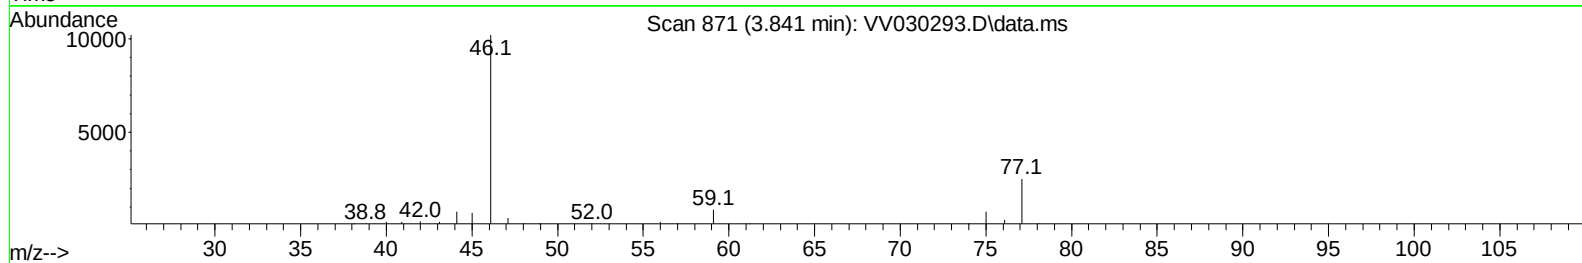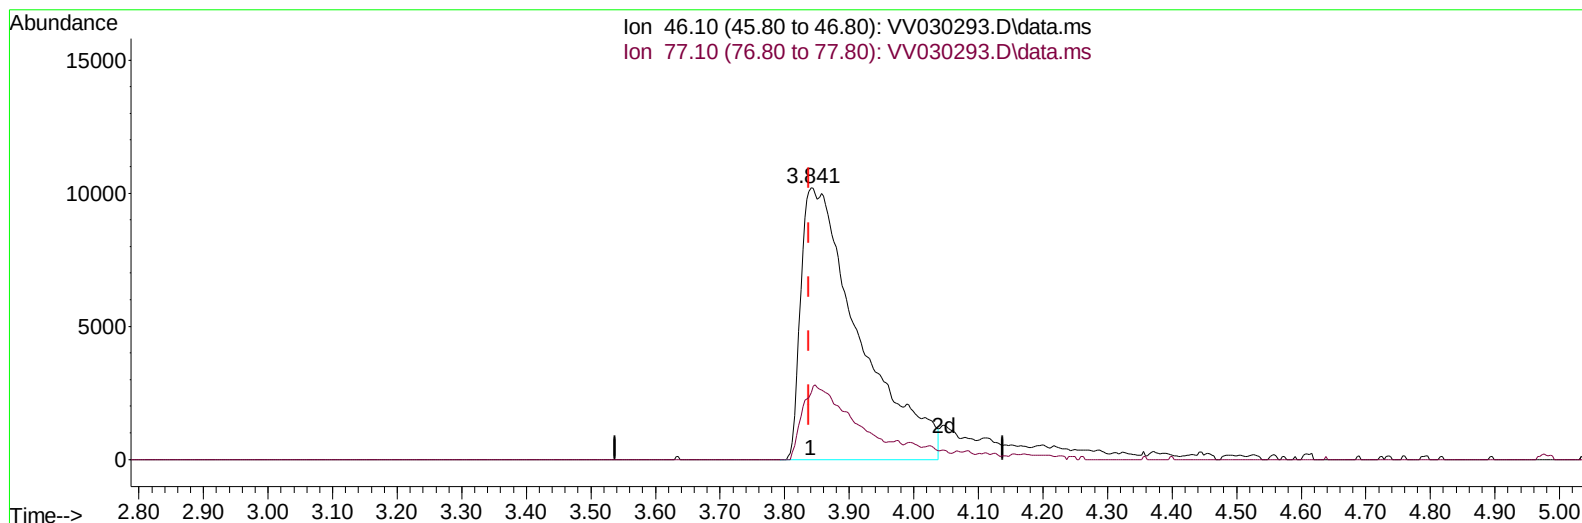

TIC: VV030293.D\data.ms

(20) 2-Butanone-d5 (S)

3.841min (+ 0.003) 44.54 ug/L m

response 63879

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	22.91#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
 Data File : VV030293.D
 Acq On : 22 Mar 2023 15:08
 Operator : SY/MD
 Sample : 02003-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBM8

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:49:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 23 01:48:30 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/23/2023
 Supervised By :Mahesh Dadoda 03/23/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		120227	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117		116530	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		60613	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		34764	4.469	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.400%	
7) Chloroethane-d5	1.536	69		34170	4.679	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.600%	
11) 1,1-Dichloroethene-d2	2.063	63		60487	3.782	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.600%	
20) 2-Butanone-d5	3.841	46		63879m	44.538	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.080%	
24) Chloroform-d	4.265	84		73264	4.610	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.200%	
26) 1,2-Dichloroethane-d4	4.957	65		38845	5.988	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.800%	
32) Benzene-d6	4.970	84		132626	4.230	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%	
36) 1,2-Dichloropropane-d6	6.002	67		35811	3.796	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.000%	
41) Toluene-d8	7.252	98		119328	4.015	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.200%	
43) trans-1,3-Dichloroprop...	7.561	79		15520	4.809	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.200%	
46) 2-Hexanone-d5	8.040	63		54264	40.641	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.280%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		26676	3.975	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.600%	
66) 1,2-Dichlorobenzene-d4	11.571	152		48368	4.716	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.400%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030293.D
Acq On : 22 Mar 2023 15:08
Operator : SY/MD
Sample : 02003-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBM8

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:49:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 23 01:48:30 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/23/2023
Supervised By :Mahesh Dadoda 03/23/2023

