

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
 Data File : VV030293.D
 Acq On : 22 Mar 2023 15:08
 Operator : SY/MD
 Sample : 02003-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BM8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	62	rBV4	2968	4568	1.20%	0.141%
2	1.282	68	75	86	rBV	53757	56018	14.74%	1.726%
3	1.536	146	154	169	rVB	56685	66883	17.60%	2.060%
4	2.063	307	318	330	rBV	114362	167365	44.03%	5.156%
5	3.844	860	872	906	rBV2	18550	100038	26.32%	3.082%
6	4.262	986	1002	1030	rBV	67713	172325	45.33%	5.309%
7	4.970	1203	1222	1250	rBV2	148242	380118	100.00%	11.710%
8	5.545	1388	1401	1422	rBV	135252	278487	73.26%	8.579%
9	5.998	1527	1542	1561	rBV2	84444	178685	47.01%	5.505%
10	6.924	1819	1830	1845	rBV	39953	74442	19.58%	2.293%
11	7.082	1870	1879	1890	rVB5	3711	7214	1.90%	0.222%
12	7.252	1919	1932	1953	rBV	172596	314248	82.67%	9.681%
13	7.564	2017	2029	2052	rBV2	23983	46518	12.24%	1.433%
14	7.886	2119	2129	2132	rBV2	2712	4243	1.12%	0.131%
15	7.915	2134	2138	2147	rVB5	4168	5895	1.55%	0.182%
16	8.040	2163	2177	2214	rBV	137800	300413	79.03%	9.255%
17	8.793	2399	2411	2434	rBV	207186	348540	91.69%	10.738%
18	10.162	2827	2837	2849	rBV	60672	98831	26.00%	3.045%
19	10.333	2879	2890	2899	rVB2	7558	12618	3.32%	0.389%
20	11.194	3147	3158	3179	rBV	220580	339159	89.22%	10.449%
21	11.571	3263	3275	3298	rVB	181764	289388	76.13%	8.915%




Sum of corrected areas: 3245996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030293.D
Acq On : 22 Mar 2023 15:08
Operator : SY/MD
Sample : 02003-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

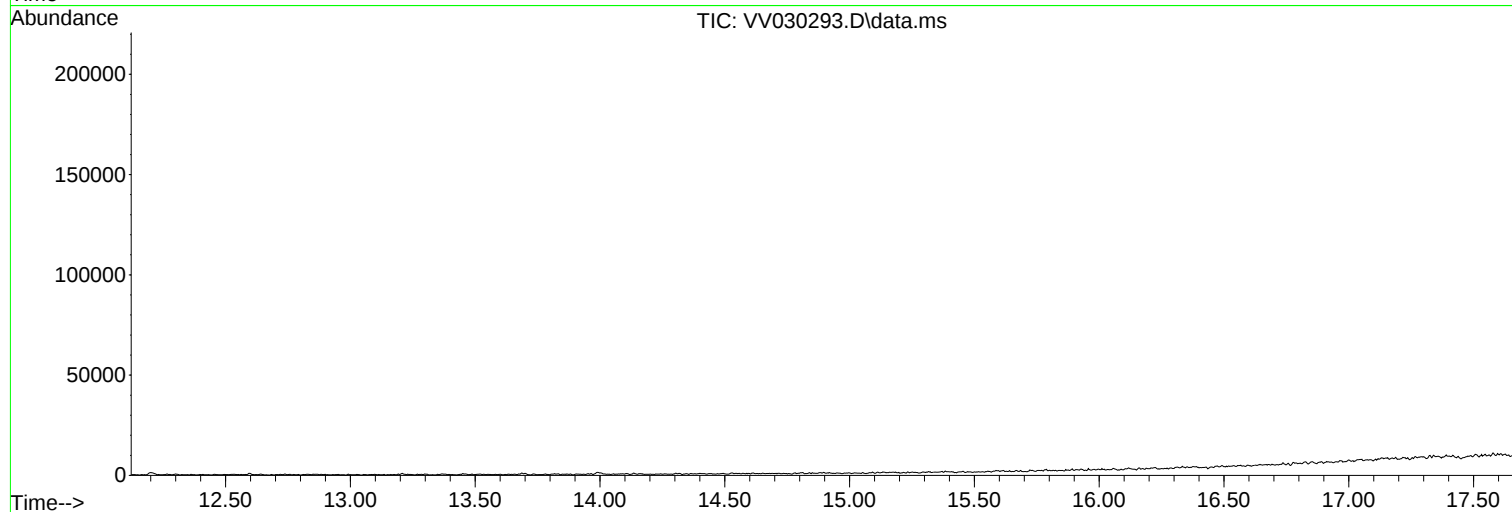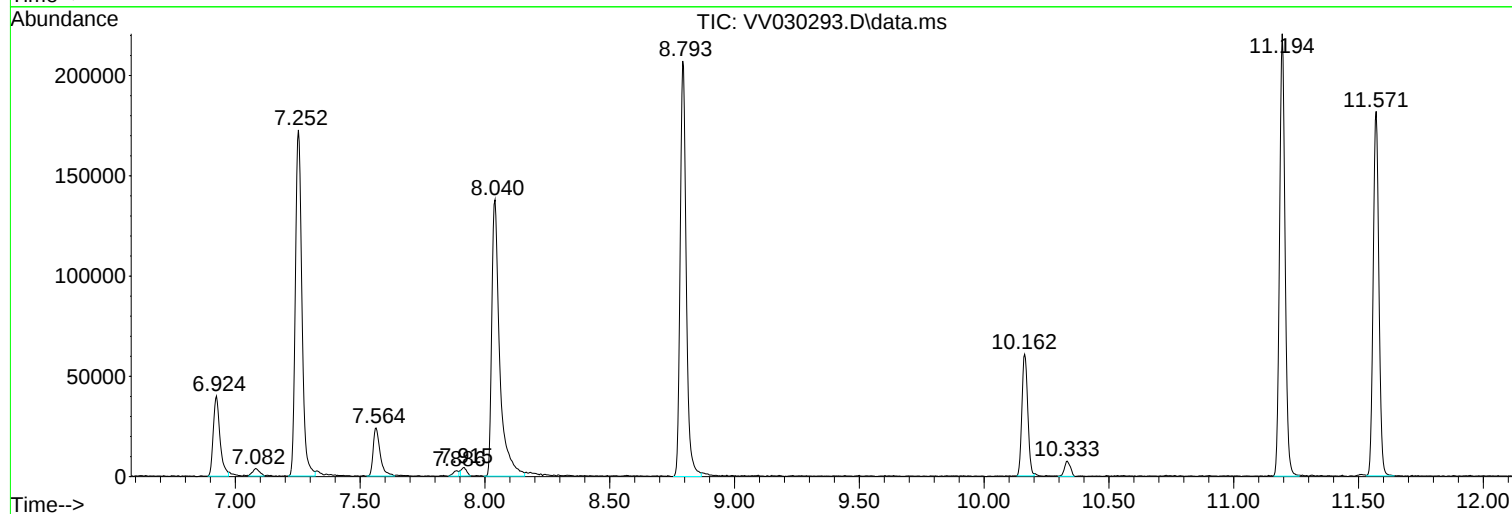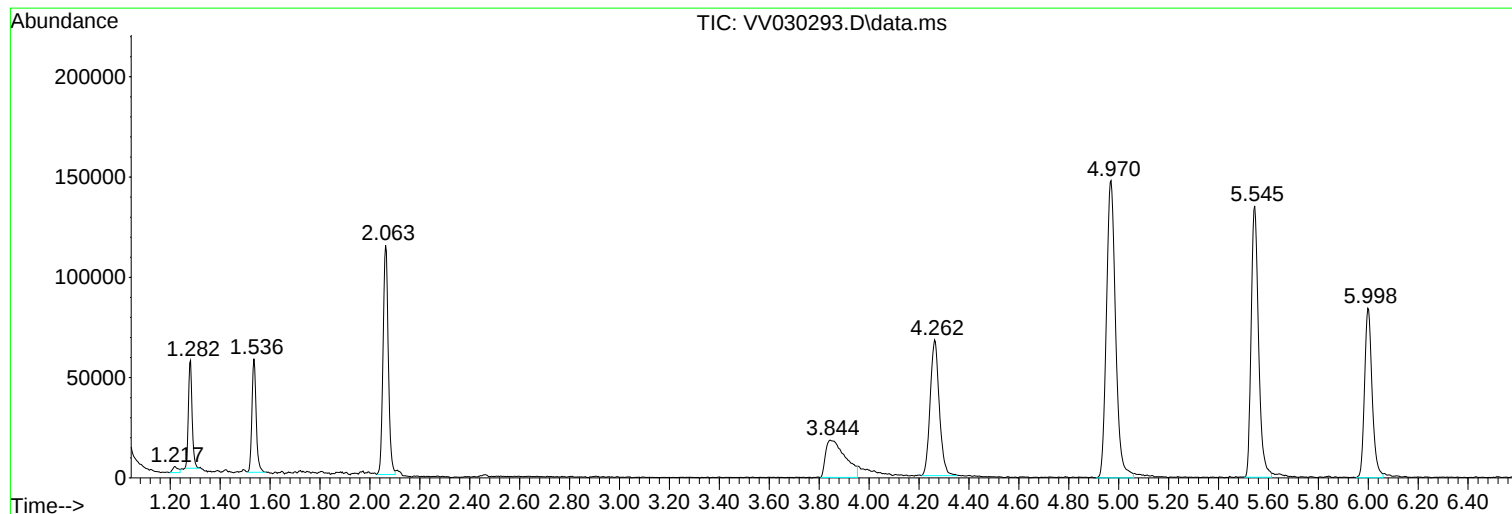

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030293.D
Acq On : 22 Mar 2023 15:08
Operator : SY/MD
Sample : 02003-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030293.D
Acq On : 22 Mar 2023 15:08
Operator : SY/MD
Sample : 02003-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------