

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
 Data File : VV030294.D
 Acq On : 22 Mar 2023 15:33
 Operator : SY/MD
 Sample : 02003-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBM6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	62	rBV4	3313	4772	1.31%	0.149%
2	1.282	68	75	95	rVB	52244	60364	16.62%	1.880%
3	1.539	146	155	167	rVB	49746	61733	17.00%	1.923%
4	2.066	307	319	334	rBV	105183	154422	42.52%	4.809%
5	3.818	850	864	894	rBV	32045	110833	30.52%	3.452%
6	4.259	983	1001	1022	rBV2	68941	170239	46.87%	5.302%
7	4.966	1205	1221	1249	rBV2	140544	363196	100.00%	11.311%
8	5.545	1388	1401	1423	rBV2	129682	269128	74.10%	8.382%
9	5.998	1526	1542	1562	rBV3	81223	172457	47.48%	5.371%
10	6.921	1819	1829	1846	rBV2	36417	71235	19.61%	2.219%
11	7.252	1919	1932	1960	rBV	171078	305619	84.15%	9.518%
12	7.561	2019	2028	2053	rBV2	24173	45626	12.56%	1.421%
13	7.883	2117	2128	2147	rBV2	13023	30480	8.39%	0.949%
14	8.034	2165	2175	2201	rBV	148387	283005	77.92%	8.814%
15	8.793	2399	2411	2438	rBV	195970	331900	91.38%	10.337%
16	10.162	2826	2837	2853	rVB2	57873	93298	25.69%	2.906%
17	10.336	2879	2891	2909	rBV	38787	63575	17.50%	1.980%
18	11.194	3146	3158	3179	rBV	205501	327131	90.07%	10.188%
19	11.571	3264	3275	3296	rVB	177351	277503	76.41%	8.643%
20	12.204	3462	3472	3482	rVB3	9494	14361	3.95%	0.447%




Sum of corrected areas: 3210877

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030294.D
Acq On : 22 Mar 2023 15:33
Operator : SY/MD
Sample : 02003-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

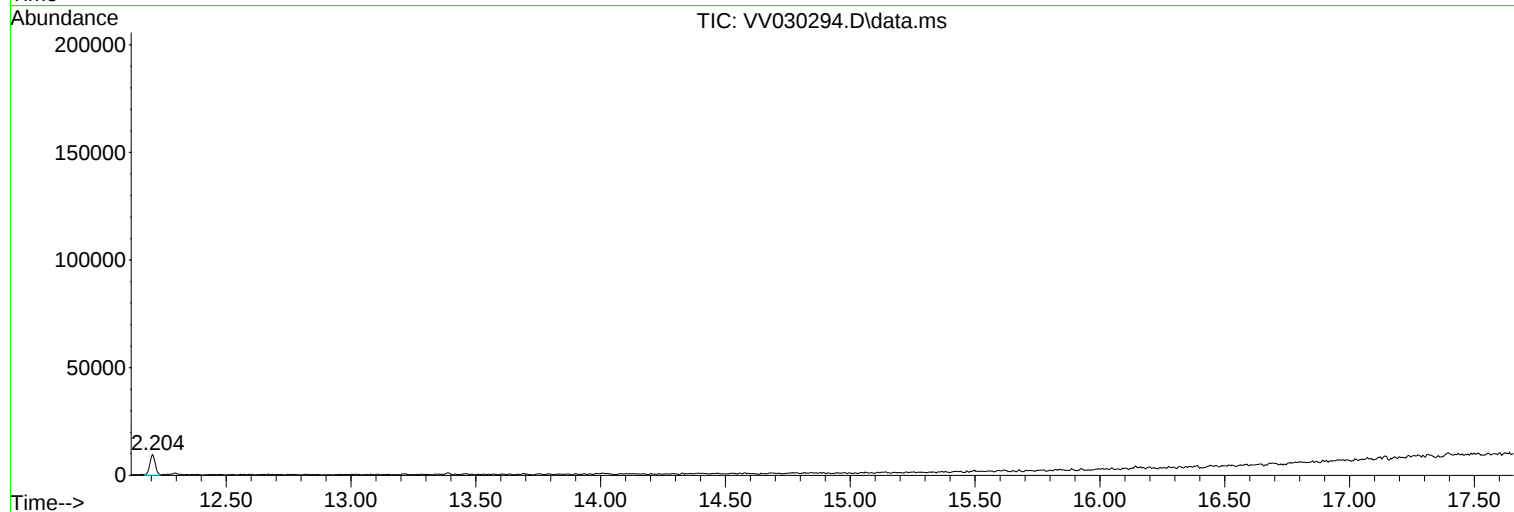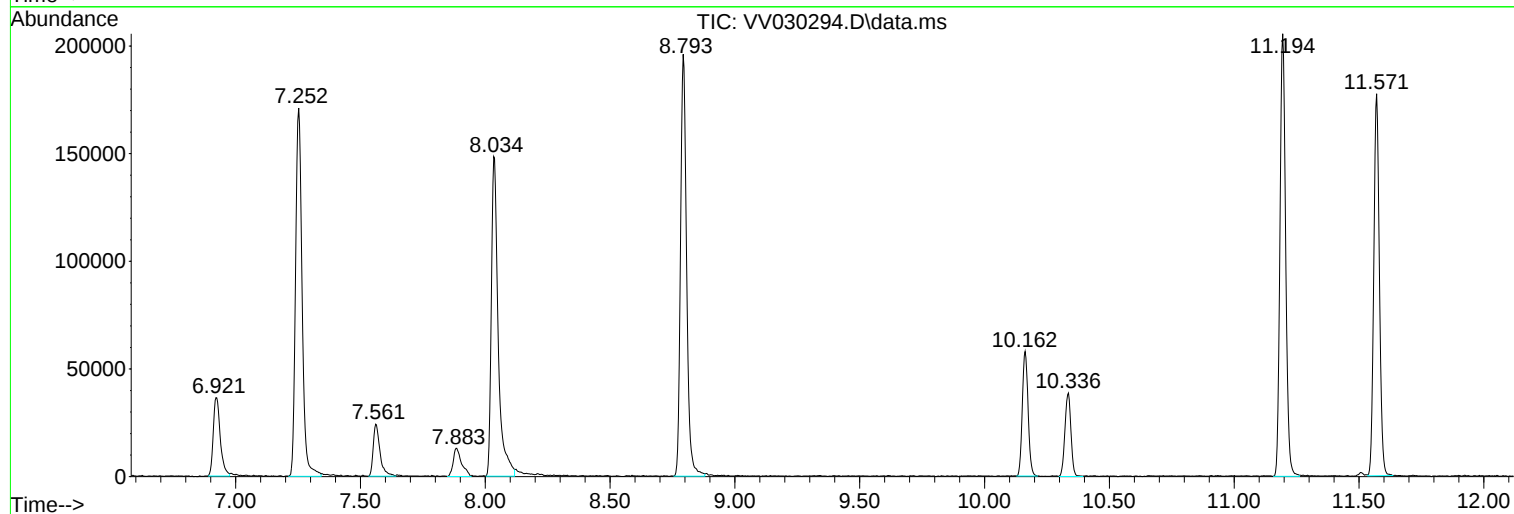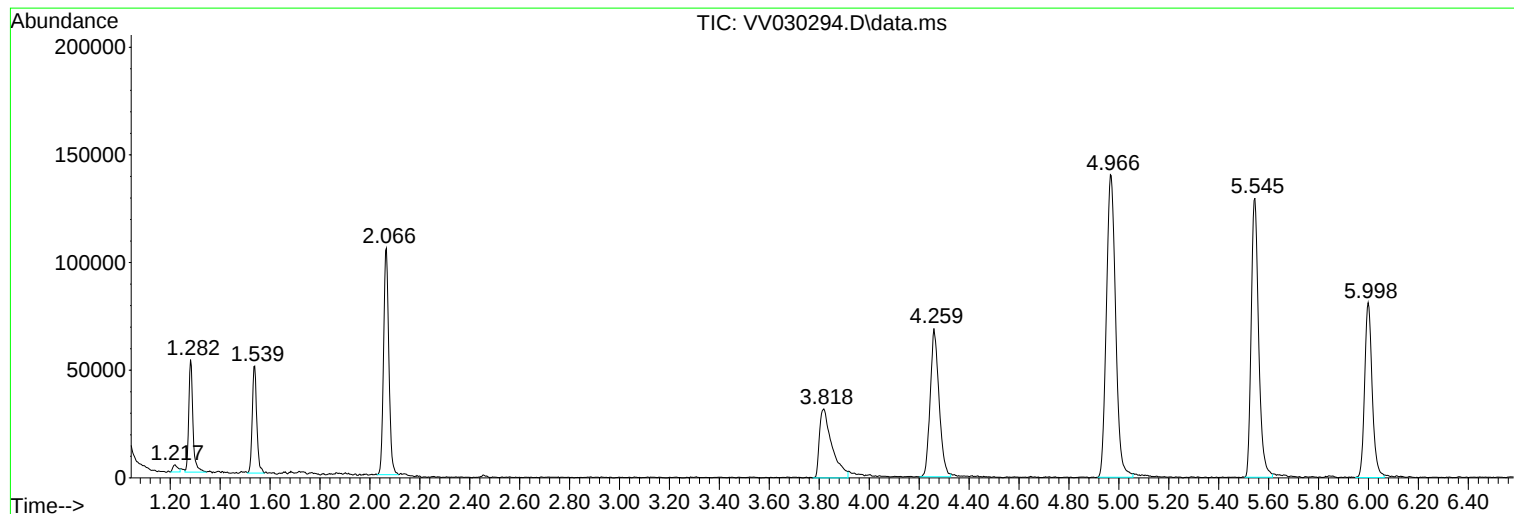

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030294.D
Acq On : 22 Mar 2023 15:33
Operator : SY/MD
Sample : 02003-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030294.D
Acq On : 22 Mar 2023 15:33
Operator : SY/MD
Sample : 02003-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------