

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
 Data File : VV030295.D
 Acq On : 22 Mar 2023 16:19
 Operator : SY/MD
 Sample : 02003-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BM7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	86	rVV	55318	61410	15.83%	1.843%
2	1.536	147	154	170	rVB	58774	70526	18.18%	2.117%
3	2.063	307	318	335	rBV	118118	172199	44.39%	5.168%
4	2.458	432	441	451	rVB6	3508	6285	1.62%	0.189%
5	3.838	856	870	906	rBV2	24216	115037	29.65%	3.453%
6	4.262	984	1002	1026	rBV	69684	182857	47.14%	5.488%
7	4.970	1205	1222	1251	rBV2	150832	387941	100.00%	11.644%
8	5.545	1388	1401	1429	rBV	133539	281642	72.60%	8.453%
9	5.998	1528	1542	1566	rBV2	88619	186695	48.12%	5.604%
10	6.924	1819	1830	1845	rBV2	39669	75451	19.45%	2.265%
11	7.252	1920	1932	1957	rBV	180177	325249	83.84%	9.762%
12	7.561	2018	2028	2045	rBV	24969	46340	11.95%	1.391%
13	7.889	2114	2130	2135	rBV3	4077	7892	2.03%	0.237%
14	8.037	2165	2176	2211	rBV	154575	309822	79.86%	9.299%
15	8.793	2398	2411	2432	rBV	203963	342850	88.38%	10.291%
16	10.162	2826	2837	2854	rBV	66078	102159	26.33%	3.066%
17	10.336	2881	2891	2901	rBV2	8522	13614	3.51%	0.409%
18	11.194	3147	3158	3180	rBV	219671	341982	88.15%	10.264%
19	11.571	3261	3275	3292	rBV	185379	297116	76.59%	8.918%
20	12.204	3464	3472	3481	rBV5	2917	4644	1.20%	0.139%




Sum of corrected areas: 3331711

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030295.D
Acq On : 22 Mar 2023 16:19
Operator : SY/MD
Sample : 02003-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

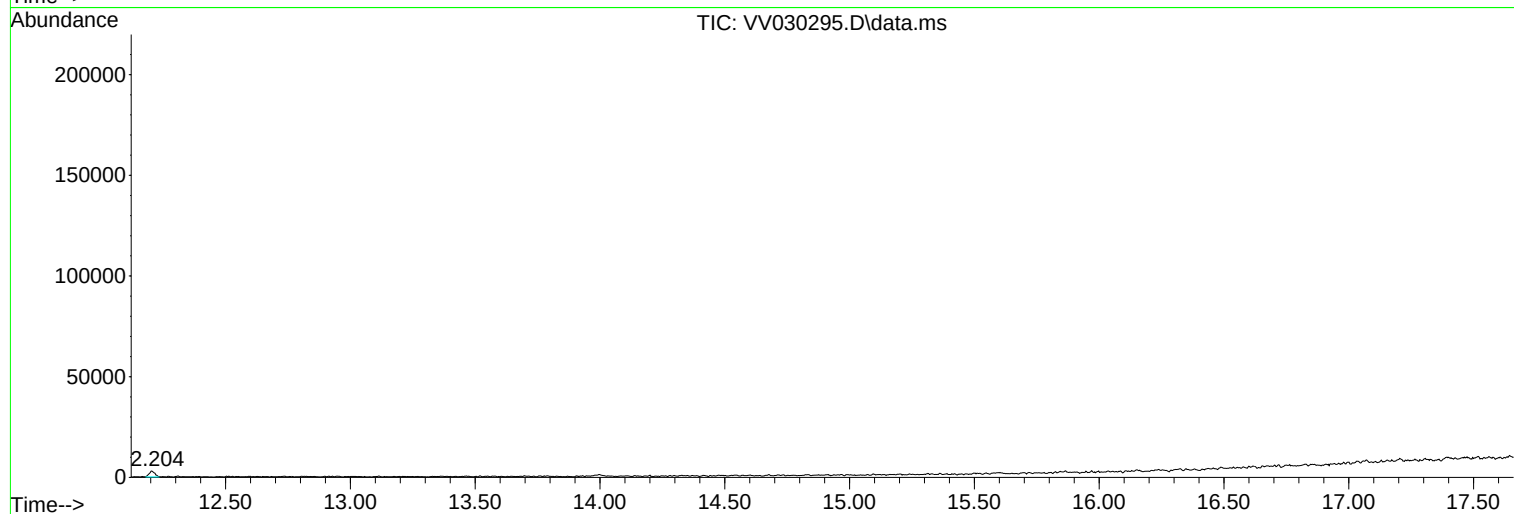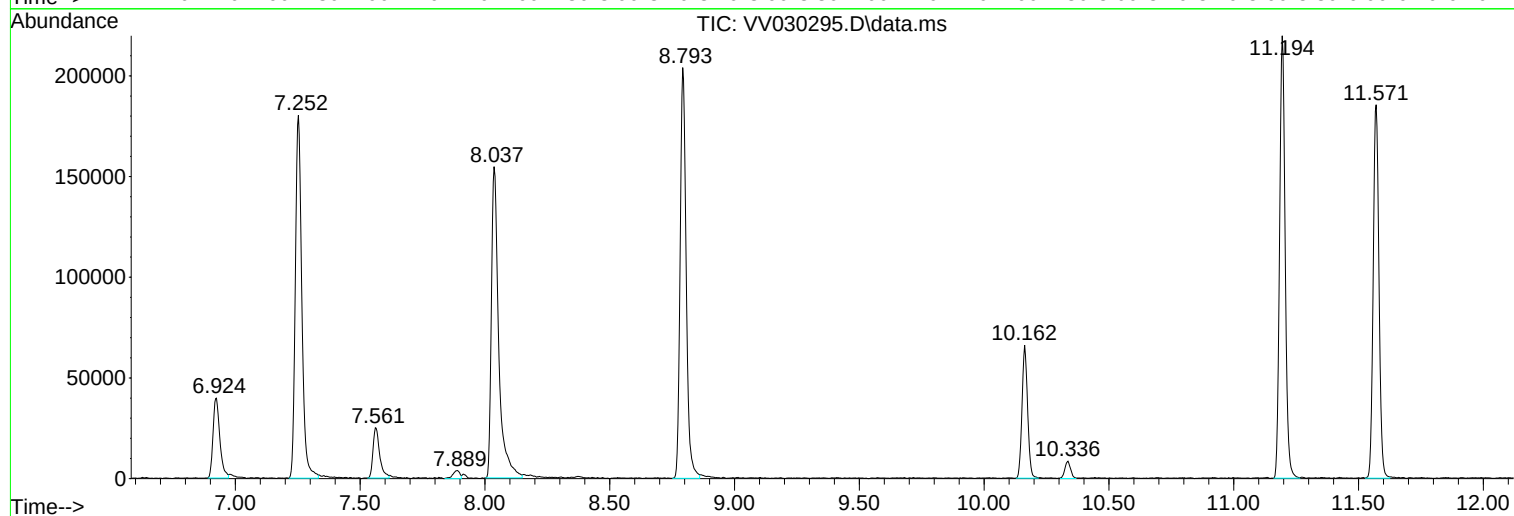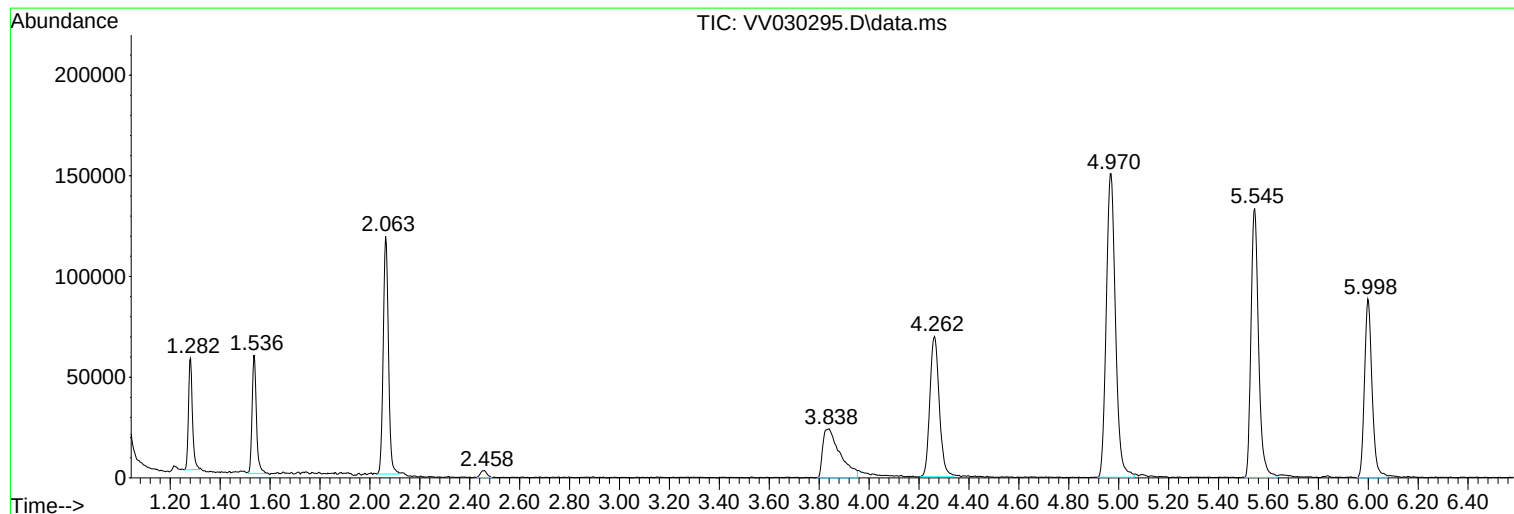

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030295.D
Acq On : 22 Mar 2023 16:19
Operator : SY/MD
Sample : 02003-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032223\
Data File : VV030295.D
Acq On : 22 Mar 2023 16:19
Operator : SY/MD
Sample : 02003-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc