

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034804.D
 Acq On : 22 Mar 2024 09:21
 Operator : SY/MD
 Sample : VV0322WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK252

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034804.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	96	rVB	167305	171497	15.95%	2.118%
2	1.536	146	154	170	rVB	134508	156797	14.58%	1.936%
3	2.060	305	317	337	rBV	271618	399890	37.18%	4.938%
4	2.452	431	439	450	rBV4	2926	4966	0.46%	0.061%
5	2.593	480	483	486	rBV	193	116	0.01%	0.001%
6	2.648	496	500	505	rBV2	213	205	0.02%	0.003%
7	2.674	505	508	514	rVB2	260	287	0.03%	0.004%
8	2.699	514	516	519	rBV2	379	220	0.02%	0.003%
9	2.812	546	551	554	rBV2	212	216	0.02%	0.003%
10	2.892	572	576	583	rBV2	340	550	0.05%	0.007%
11	2.986	603	605	608	rBV2	168	127	0.01%	0.002%
12	3.040	618	622	627	rVB2	273	287	0.03%	0.004%
13	3.063	628	629	631	rBV	227	102	0.01%	0.001%
14	3.089	635	637	639	rBV	281	151	0.01%	0.002%
15	3.108	639	643	645	rBV2	176	147	0.01%	0.002%
16	3.137	650	652	656	rBV	171	141	0.01%	0.002%
17	3.207	671	674	676	rBV	140	107	0.01%	0.001%
18	3.220	676	678	681	rVV	221	133	0.01%	0.002%
19	3.262	689	691	694	rVB	288	104	0.01%	0.001%
20	3.304	699	704	710	rBV2	235	302	0.03%	0.004%
21	3.420	738	740	742	rBB	259	139	0.01%	0.002%
22	3.442	743	747	748	rBV	273	181	0.02%	0.002%
23	3.490	756	762	764	rBV2	317	335	0.03%	0.004%
24	3.587	787	792	797	rBB2	276	363	0.03%	0.004%
25	3.616	798	801	802	rBV	265	149	0.01%	0.002%
26	3.642	806	809	813	rBV	173	200	0.02%	0.002%
27	3.667	813	817	820	rBV2	240	248	0.02%	0.003%
28	3.716	829	832	835	rBV2	208	157	0.01%	0.002%
29	3.796	848	857	905	rBV	60893	197896	18.40%	2.444%
30	4.246	981	997	1024	rBV	172835	442871	41.18%	5.468%
31	4.516	1078	1081	1083	rBV2	357	292	0.03%	0.004%
32	4.571	1096	1098	1100	rBV	323	189	0.02%	0.002%
33	4.773	1159	1161	1166	rVB2	284	158	0.01%	0.002%
34	4.799	1166	1169	1172	rVB	216	165	0.02%	0.002%
35	4.953	1201	1217	1260	rBV2	400622	1075427	100.00%	13.279%
36	5.391	1350	1353	1356	rBV2	328	182	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034804.D
Acq On : 22 Mar 2024 09:21
Operator : SY/MD
Sample : VV0322WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis

37	5.529	1383	1396	1428	rBV	280817	582480	54.16%	7.192%
38	5.828	1480	1489	1508	rBV3	10547	21632	2.01%	0.267%
39	5.982	1525	1537	1568	rBV	223256	464686	43.21%	5.738%
40	6.133	1580	1584	1585	rBV3	803	620	0.06%	0.008%
41	6.204	1603	1606	1609	rBV	328	172	0.02%	0.002%
42	6.259	1620	1623	1625	rBV2	202	161	0.01%	0.002%
43	6.326	1641	1644	1648	rVV2	159	170	0.02%	0.002%
44	6.365	1653	1656	1658	rBV2	253	165	0.02%	0.002%
45	6.400	1664	1667	1671	rBB	141	148	0.01%	0.002%
46	6.526	1704	1706	1711	rVB2	213	149	0.01%	0.002%
47	6.590	1723	1726	1731	rVV2	218	229	0.02%	0.003%
48	6.841	1801	1804	1806	rBV2	147	123	0.01%	0.002%
49	6.908	1815	1825	1849	rBV	125140	241635	22.47%	2.984%
50	7.172	1905	1907	1911	rBV3	420	354	0.03%	0.004%
51	7.239	1917	1928	1960	rBV	491963	870447	80.94%	10.748%
52	7.551	2016	2025	2048	rBV	89516	162904	15.15%	2.011%
53	7.767	2089	2092	2094	rBV2	410	290	0.03%	0.004%
54	7.918	2136	2139	2148	rBV3	446	663	0.06%	0.008%
55	7.966	2150	2154	2160	rBV2	197	291	0.03%	0.004%
56	8.024	2163	2172	2207	rBV	201171	433056	40.27%	5.347%
57	8.609	2352	2354	2357	rVB2	184	105	0.01%	0.001%
58	8.738	2391	2394	2397	rBV2	216	202	0.02%	0.002%
59	8.783	2397	2408	2432	rBV	429463	709594	65.98%	8.762%
60	9.027	2481	2484	2486	rBV	254	171	0.02%	0.002%
61	9.088	2501	2503	2509	rVB3	503	364	0.03%	0.004%
62	9.133	2515	2517	2518	rBV	305	143	0.01%	0.002%
63	9.191	2527	2535	2541	rBV2	346	600	0.06%	0.007%
64	9.326	2572	2577	2580	rBV2	289	349	0.03%	0.004%
65	9.352	2580	2585	2589	rVV2	266	331	0.03%	0.004%
66	9.490	2619	2628	2632	rBV3	1083	1335	0.12%	0.016%
67	9.600	2659	2662	2664	rBV2	168	115	0.01%	0.001%
68	9.616	2664	2667	2671	rBV	180	131	0.01%	0.002%
69	9.751	2706	2709	2713	rBV2	177	204	0.02%	0.003%
70	9.818	2727	2730	2732	rBV	204	162	0.02%	0.002%
71	10.018	2788	2792	2794	rBV2	177	140	0.01%	0.002%
72	10.079	2808	2811	2812	rBV	169	121	0.01%	0.001%
73	10.149	2819	2833	2856	rBV	307531	482547	44.87%	5.958%
74	10.320	2880	2886	2889	rBV2	499	641	0.06%	0.008%
75	10.435	2920	2922	2926	rBV	185	151	0.01%	0.002%
76	10.484	2930	2937	2943	rBV2	1165	1761	0.16%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034804.D
 Acq On : 22 Mar 2024 09:21
 Operator : SY/MD
 Sample : VV0322WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK252

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.554	2952	2959	2960	rBV	362	275	0.03%	0.003%
78	10.628	2976	2982	2987	rBV2	275	408	0.04%	0.005%
79	10.709	3004	3007	3009	rBV2	241	177	0.02%	0.002%
80	10.792	3030	3033	3037	rBV2	154	145	0.01%	0.002%
81	10.812	3037	3039	3041	rBV2	173	106	0.01%	0.001%
82	10.998	3093	3097	3098	rBV	186	115	0.01%	0.001%
83	11.037	3105	3109	3113	rBV2	205	203	0.02%	0.003%
84	11.127	3130	3137	3144	rBV4	2497	3670	0.34%	0.045%
85	11.181	3144	3154	3180	rVV	447189	720236	66.97%	8.893%
86	11.455	3236	3239	3242	rBV	235	174	0.02%	0.002%
87	11.474	3242	3245	3247	rBV	208	168	0.02%	0.002%
88	11.558	3259	3271	3295	rBV	523935	821832	76.42%	10.148%
89	12.175	3459	3463	3464	rBV2	354	227	0.02%	0.003%
90	12.358	3516	3520	3521	rBV	199	138	0.01%	0.002%
91	12.371	3521	3524	3530	rVB4	658	787	0.07%	0.010%
92	12.484	3556	3559	3560	rBV	226	130	0.01%	0.002%
93	12.587	3585	3591	3610	rVB5	3719	5931	0.55%	0.073%
94	13.162	3767	3770	3772	rBV2	362	196	0.02%	0.002%
95	13.204	3774	3783	3795	rBV3	9973	15497	1.44%	0.191%
96	13.442	3848	3857	3871	rBV	43350	71447	6.64%	0.882%
97	13.683	3923	3932	3946	rVB2	13550	21342	1.98%	0.264%
98	13.795	3964	3967	3972	rVB2	415	364	0.03%	0.004%
99	14.284	4117	4119	4122	rBV2	338	99	0.01%	0.001%
100	14.352	4138	4140	4142	rBV2	552	217	0.02%	0.003%




Sum of corrected areas: 8098723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034804.D
Acq On : 22 Mar 2024 09:21
Operator : SY/MD
Sample : VV0322WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

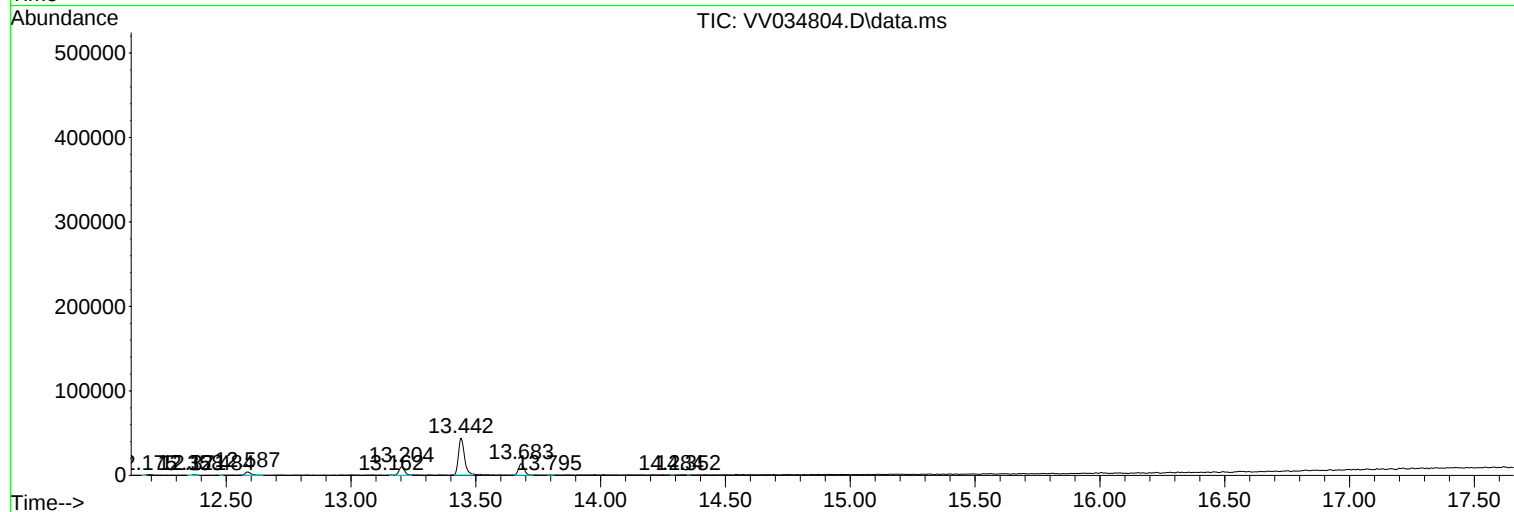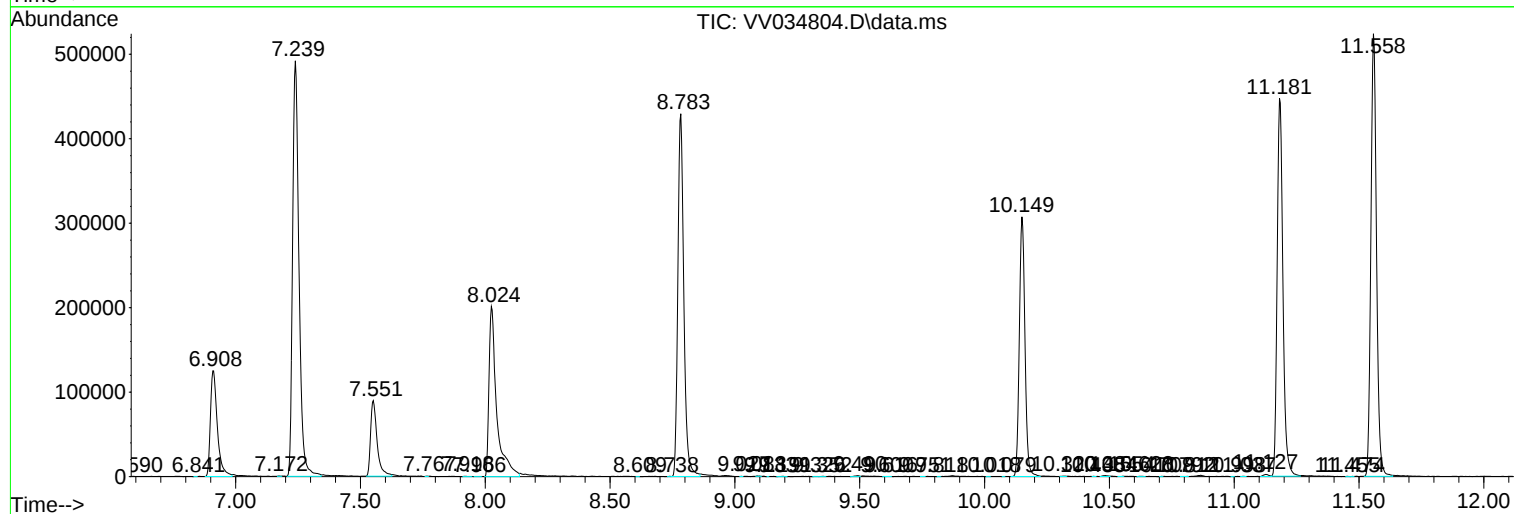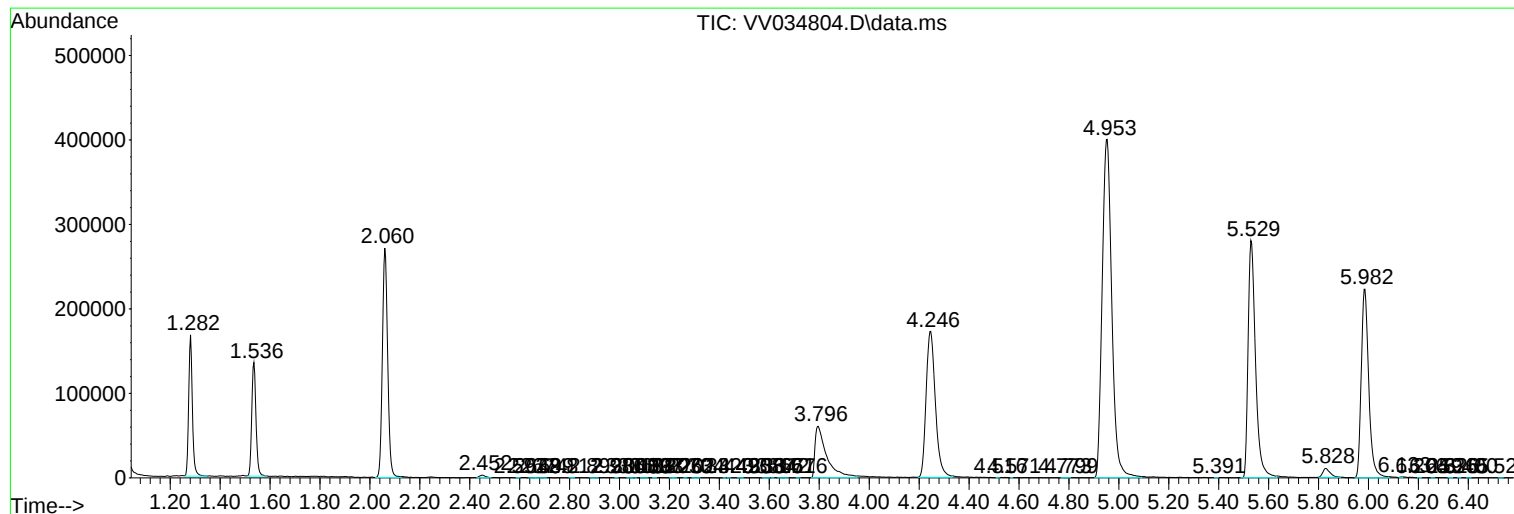

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034804.D
Acq On : 22 Mar 2024 09:21
Operator : SY/MD
Sample : VV0322WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034804.D
Acq On : 22 Mar 2024 09:21
Operator : SY/MD
Sample : VV0322WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------