

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034807.D
 Acq On : 22 Mar 2024 10:33
 Operator : SY/MD
 Sample : P1822-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0778

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	43	47	50	rBV3	1918	1816	0.12%	0.017%
2	1.281	68	75	90	rBV	228090	238309	15.82%	2.263%
3	1.532	146	153	167	rVB	174012	196163	13.02%	1.863%
4	1.982	291	293	296	rVB2	442	221	0.01%	0.002%
5	2.002	296	299	303	rVB3	711	462	0.03%	0.004%
6	2.060	307	317	332	rBV	293233	430520	28.57%	4.088%
7	2.288	386	388	395	rVB2	259	179	0.01%	0.002%
8	2.445	432	437	450	rBV4	1354	2487	0.17%	0.024%
9	2.561	470	473	477	rVV2	461	410	0.03%	0.004%
10	2.600	481	485	489	rVB3	303	188	0.01%	0.002%
11	2.751	528	532	538	rBV2	147	185	0.01%	0.002%
12	2.818	550	553	558	rBV2	235	195	0.01%	0.002%
13	2.905	578	580	586	rVB2	245	218	0.01%	0.002%
14	2.937	586	590	594	rVB3	435	305	0.02%	0.003%
15	3.053	622	626	632	rVB2	174	204	0.01%	0.002%
16	3.111	641	644	647	rVV	281	197	0.01%	0.002%
17	3.201	663	672	676	rBV2	258	346	0.02%	0.003%
18	3.342	711	716	718	rBV	189	178	0.01%	0.002%
19	3.375	723	726	729	rVB	303	204	0.01%	0.002%
20	3.397	729	733	736	rBV2	309	237	0.02%	0.002%
21	3.529	768	774	777	rVB2	264	268	0.02%	0.003%
22	3.551	777	781	786	rBV2	217	248	0.02%	0.002%
23	3.593	791	794	797	rVB2	259	181	0.01%	0.002%
24	3.641	807	809	816	rVB2	235	312	0.02%	0.003%
25	3.677	816	820	826	rBV2	276	392	0.03%	0.004%
26	3.793	847	856	902	rBV	89488	284049	18.85%	2.697%
27	4.246	982	997	1033	rBV2	240844	663828	44.05%	6.303%
28	4.477	1066	1069	1073	rVB4	399	332	0.02%	0.003%
29	4.635	1112	1118	1126	rVB4	338	488	0.03%	0.005%
30	4.712	1138	1142	1146	rBV2	436	365	0.02%	0.003%
31	4.776	1159	1162	1170	rVB3	263	371	0.02%	0.004%
32	4.873	1188	1192	1195	rBV2	326	300	0.02%	0.003%
33	4.953	1201	1217	1261	rBV2	564345	1506834	100.00%	14.308%
34	5.452	1369	1372	1375	rBV2	324	294	0.02%	0.003%
35	5.532	1386	1397	1432	rBV	378668	785904	52.16%	7.462%
36	5.754	1463	1466	1470	rVB3	474	341	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034807.D
 Acq On : 22 Mar 2024 10:33
 Operator : SY/MD
 Sample : P1822-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0778

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.831	1477	1490	1510	rBV4	16557	38076	2.53%	0.362%
38	5.924	1518	1519	1524	rVB3	425	191	0.01%	0.002%
39	5.985	1525	1538	1573	rBV	290139	613431	40.71%	5.825%
40	6.374	1655	1659	1661	rBV3	315	215	0.01%	0.002%
41	6.439	1670	1679	1693	rBV4	4385	9826	0.65%	0.093%
42	6.654	1741	1746	1748	rBV	252	239	0.02%	0.002%
43	6.731	1759	1770	1771	rBV2	258	321	0.02%	0.003%
44	6.789	1783	1788	1792	rVB2	198	218	0.01%	0.002%
45	6.911	1813	1826	1853	rBV	176096	334930	22.23%	3.180%
46	7.133	1890	1895	1897	rVB2	386	340	0.02%	0.003%
47	7.149	1897	1900	1902	rBV2	330	226	0.01%	0.002%
48	7.191	1910	1913	1917	rBV4	466	300	0.02%	0.003%
49	7.243	1917	1929	1965	rBV	633970	1134708	75.30%	10.775%
50	7.551	2016	2025	2062	rBV	119811	223350	14.82%	2.121%
51	7.754	2086	2088	2093	rVB3	459	334	0.02%	0.003%
52	7.876	2116	2126	2139	rVB3	5158	9844	0.65%	0.093%
53	7.989	2158	2161	2163	rBV2	427	287	0.02%	0.003%
54	8.024	2163	2172	2214	rBV	306992	661336	43.89%	6.280%
55	8.413	2289	2293	2295	rBV2	352	191	0.01%	0.002%
56	8.564	2337	2340	2351	rVB4	350	472	0.03%	0.004%
57	8.625	2356	2359	2363	rVB2	433	368	0.02%	0.003%
58	8.680	2374	2376	2381	rVB2	297	180	0.01%	0.002%
59	8.783	2397	2408	2439	rBV	566350	927157	61.53%	8.804%
60	9.082	2500	2501	2505	rVV3	355	208	0.01%	0.002%
61	9.143	2517	2520	2524	rBV	368	251	0.02%	0.002%
62	9.204	2536	2539	2541	rBV	299	178	0.01%	0.002%
63	9.484	2623	2626	2632	rVV2	483	417	0.03%	0.004%
64	9.558	2644	2649	2651	rVV3	342	222	0.01%	0.002%
65	9.625	2668	2670	2673	rBV2	308	203	0.01%	0.002%
66	9.689	2688	2690	2695	rVB2	316	209	0.01%	0.002%
67	10.149	2822	2833	2860	rVV	408202	649131	43.08%	6.164%
68	10.323	2877	2887	2899	rVB	7558	12416	0.82%	0.118%
69	10.474	2931	2934	2939	rBV2	370	296	0.02%	0.003%
70	10.860	3050	3054	3056	rBV	546	414	0.03%	0.004%
71	10.937	3075	3078	3081	rVB2	297	196	0.01%	0.002%
72	10.956	3081	3084	3089	rBV3	390	359	0.02%	0.003%
73	11.127	3134	3137	3138	rBV	599	373	0.02%	0.004%
74	11.185	3144	3155	3181	rBV	501022	806611	53.53%	7.659%
75	11.361	3207	3210	3215	rVB3	394	319	0.02%	0.003%
76	11.448	3233	3237	3240	rBV3	294	205	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034807.D
 Acq On : 22 Mar 2024 10:33
 Operator : SY/MD
 Sample : P1822-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0778

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.558	3259	3271	3294	rBV	601630	966583	64.15%	9.178%
78	11.699	3313	3315	3321	rVV3	483	363	0.02%	0.003%
79	11.734	3324	3326	3333	rVB3	467	428	0.03%	0.004%
80	11.850	3358	3362	3368	rBV2	329	286	0.02%	0.003%
81	12.191	3462	3468	3477	rVB2	1621	2485	0.16%	0.024%
82	12.323	3507	3509	3513	rBV2	282	202	0.01%	0.002%
83	12.593	3591	3593	3598	rVB3	560	504	0.03%	0.005%
84	12.660	3609	3614	3617	rBV2	378	307	0.02%	0.003%
85	12.898	3686	3688	3692	rVB2	306	196	0.01%	0.002%
86	13.210	3778	3785	3794	rVB7	1335	1933	0.13%	0.018%
87	13.303	3812	3814	3818	rVB2	392	241	0.02%	0.002%
88	13.451	3853	3860	3877	rVV2	3088	6428	0.43%	0.061%
89	13.593	3901	3904	3909	rBV4	358	268	0.02%	0.003%
90	13.648	3917	3921	3927	rBV2	373	422	0.03%	0.004%
91	13.689	3927	3934	3943	rBV4	1423	1967	0.13%	0.019%
92	13.770	3956	3959	3963	rBV3	274	238	0.02%	0.002%
93	13.808	3970	3971	3977	rBV3	323	280	0.02%	0.003%
94	13.959	4014	4018	4020	rBV2	271	207	0.01%	0.002%
95	14.040	4040	4043	4048	rBV3	369	408	0.03%	0.004%
96	14.374	4144	4147	4152	rBV4	423	378	0.03%	0.004%
97	14.448	4167	4170	4172	rBV3	416	313	0.02%	0.003%
98	14.699	4246	4248	4253	rVV3	324	217	0.01%	0.002%
99	14.773	4268	4271	4272	rBV	403	218	0.01%	0.002%
100	15.168	4392	4394	4397	rBV2	665	456	0.03%	0.004%




Sum of corrected areas: 10531407

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034807.D
Acq On : 22 Mar 2024 10:33
Operator : SY/MD
Sample : P1822-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0778

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

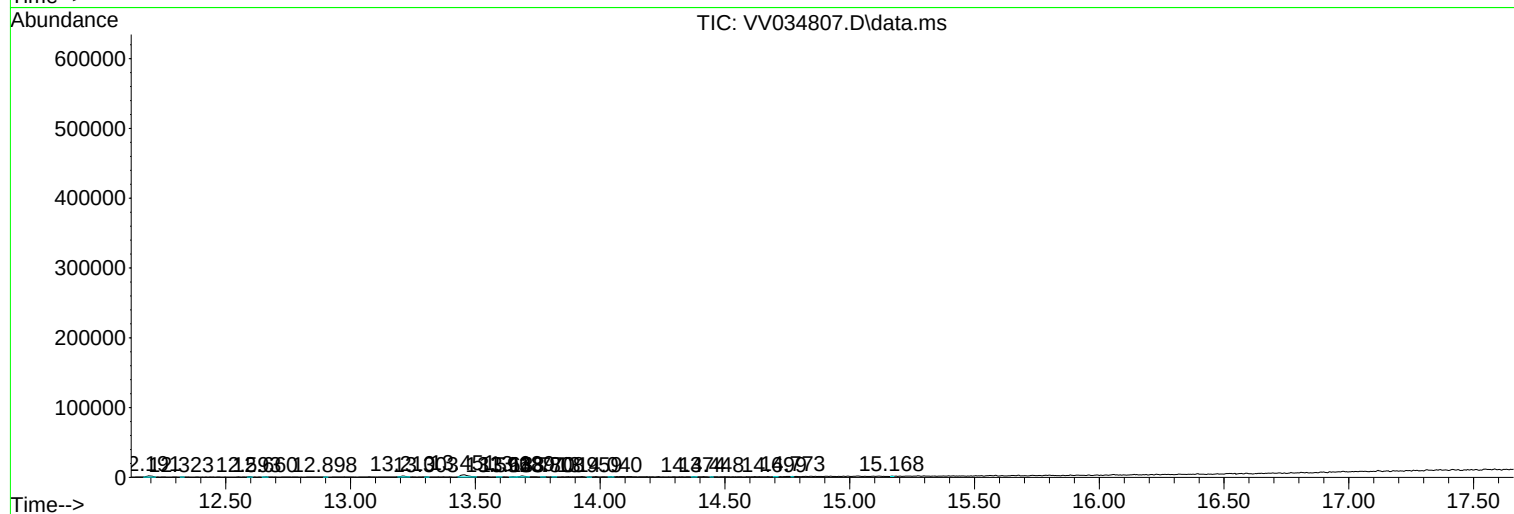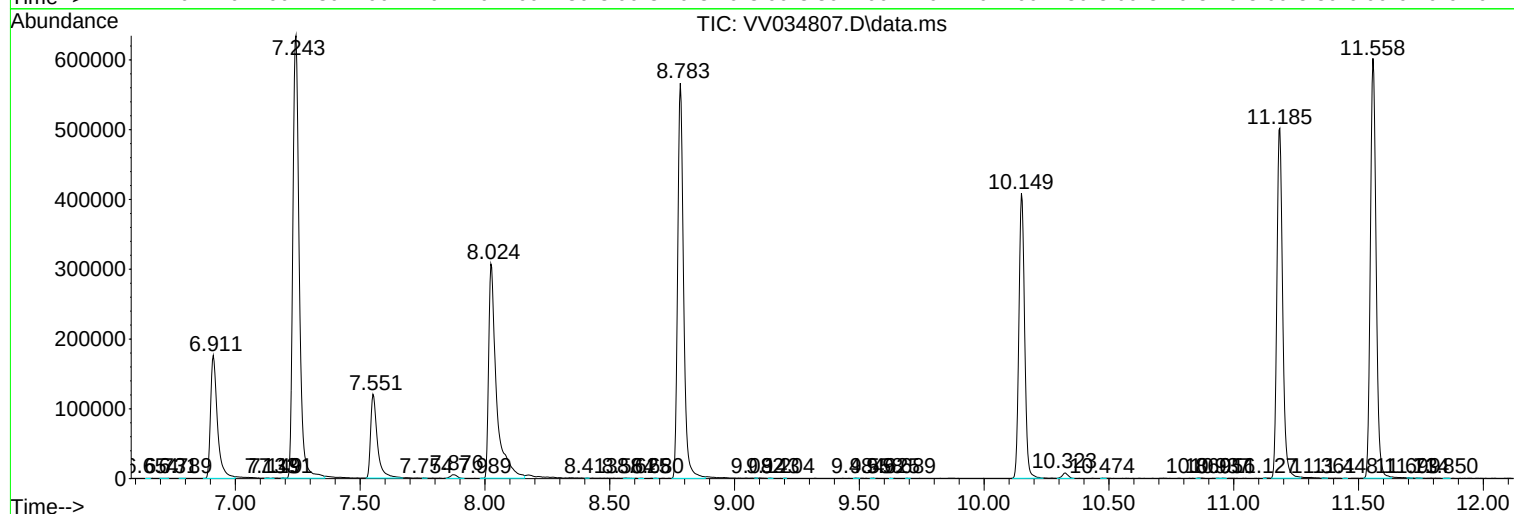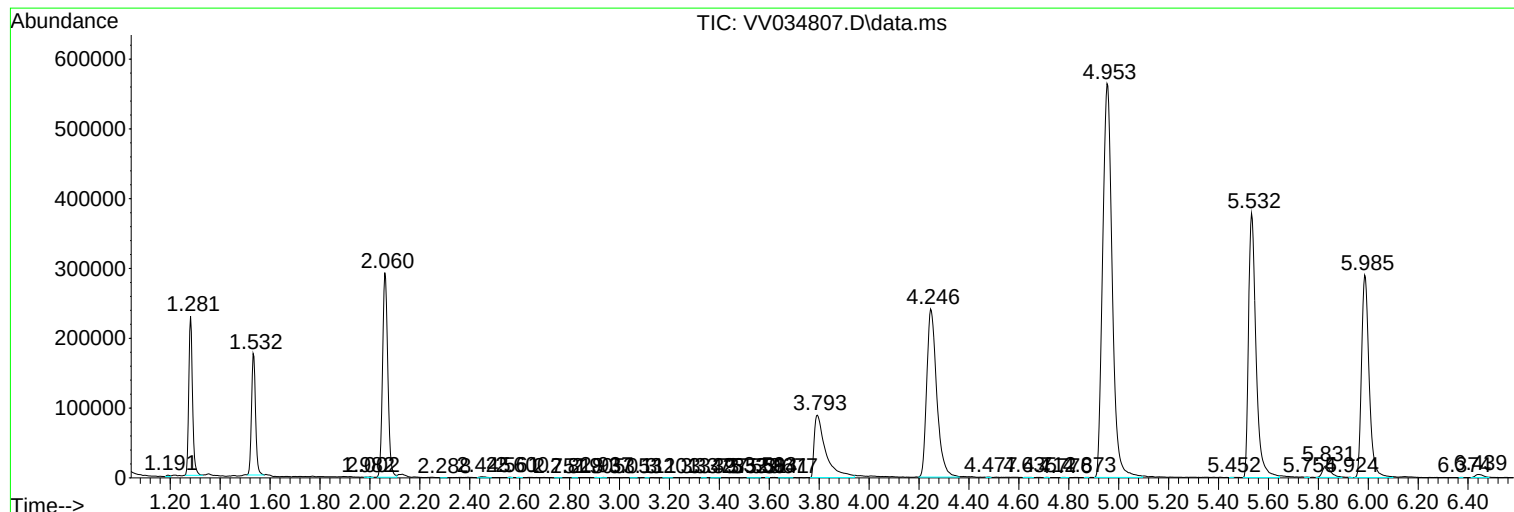

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034807.D
Acq On : 22 Mar 2024 10:33
Operator : SY/MD
Sample : P1822-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0778

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034807.D
Acq On : 22 Mar 2024 10:33
Operator : SY/MD
Sample : P1822-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0778

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc