

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034808.D
 Acq On : 22 Mar 2024 10:56
 Operator : SY/MD
 Sample : P1822-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0786

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.195	44	48	52	rBV2	2160	1923	0.13%	0.018%
2	1.217	52	55	60	rVV3	1681	1647	0.11%	0.015%
3	1.282	68	75	88	rBV	227592	239667	15.74%	2.212%
4	1.536	146	154	168	rBV	198600	226746	14.89%	2.093%
5	1.970	286	289	290	rBV2	394	236	0.02%	0.002%
6	2.015	301	303	306	rBV	272	224	0.01%	0.002%
7	2.060	306	317	332	rBV	292207	431625	28.35%	3.984%
8	2.236	367	372	373	rBV2	475	289	0.02%	0.003%
9	2.291	382	389	390	rBV	328	245	0.02%	0.002%
10	2.455	433	440	445	rBV4	1788	2291	0.15%	0.021%
11	2.616	483	490	492	rBV	580	535	0.04%	0.005%
12	2.629	492	494	501	rVB3	469	339	0.02%	0.003%
13	2.664	501	505	511	rBV2	264	297	0.02%	0.003%
14	2.748	527	531	535	rVB2	264	218	0.01%	0.002%
15	2.889	572	575	578	rBV3	501	340	0.02%	0.003%
16	3.179	661	665	669	rVB2	208	220	0.01%	0.002%
17	3.606	793	798	801	rBV3	510	536	0.04%	0.005%
18	3.796	848	857	893	rBV2	97655	303568	19.94%	2.802%
19	4.098	949	951	959	rVB3	775	640	0.04%	0.006%
20	4.249	982	998	1026	rBV	243336	673331	44.22%	6.215%
21	4.577	1098	1100	1104	rBV3	385	222	0.01%	0.002%
22	4.751	1150	1154	1158	rVB3	344	269	0.02%	0.002%
23	4.777	1158	1162	1165	rBV2	272	254	0.02%	0.002%
24	4.796	1165	1168	1176	rVB3	316	370	0.02%	0.003%
25	4.899	1196	1200	1202	rBV3	307	239	0.02%	0.002%
26	4.957	1202	1218	1253	rBV2	569331	1522652	100.00%	14.054%
27	5.249	1307	1309	1315	rVB4	445	359	0.02%	0.003%
28	5.349	1337	1340	1349	rVB5	438	433	0.03%	0.004%
29	5.420	1359	1362	1367	rVB2	376	330	0.02%	0.003%
30	5.445	1367	1370	1374	rBV3	291	262	0.02%	0.002%
31	5.474	1377	1379	1386	rVB2	333	282	0.02%	0.003%
32	5.532	1386	1397	1428	rBV	371096	775935	50.96%	7.162%
33	5.831	1480	1490	1514	rVB2	17724	41334	2.71%	0.382%
34	5.986	1525	1538	1573	rBV	322993	675499	44.36%	6.235%
35	6.127	1580	1582	1585	rBV3	427	290	0.02%	0.003%
36	6.243	1614	1618	1622	rBV2	494	327	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034808.D
Acq On : 22 Mar 2024 10:56
Operator : SY/MD
Sample : P1822-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0786

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis

37	6.442	1671	1680	1696	rVV4	5268	10474	0.69%	0.097%
38	6.912	1815	1826	1853	rBV2	176037	338951	22.26%	3.129%
39	7.114	1887	1889	1895	rVB3	485	415	0.03%	0.004%
40	7.182	1907	1910	1916	rVB3	429	392	0.03%	0.004%
41	7.243	1916	1929	1953	rBV	673901	1181820	77.62%	10.908%
42	7.551	2016	2025	2044	rBV	120613	219298	14.40%	2.024%
43	7.876	2116	2126	2136	rBV3	1994	3316	0.22%	0.031%
44	8.027	2161	2173	2216	rBV2	300327	665037	43.68%	6.138%
45	8.571	2340	2342	2346	rVB3	500	280	0.02%	0.003%
46	8.632	2358	2361	2366	rVB3	278	241	0.02%	0.002%
47	8.783	2394	2408	2438	rBV	568012	938115	61.61%	8.659%
48	9.008	2475	2478	2480	rBV2	456	244	0.02%	0.002%
49	9.101	2504	2507	2512	rVB2	706	648	0.04%	0.006%
50	9.127	2512	2515	2519	rBV2	351	336	0.02%	0.003%
51	9.204	2531	2539	2544	rBV2	469	575	0.04%	0.005%
52	9.471	2618	2622	2626	rBV2	231	215	0.01%	0.002%
53	9.493	2626	2629	2634	rVV2	499	511	0.03%	0.005%
54	9.513	2634	2635	2639	rVV	362	244	0.02%	0.002%
55	9.532	2639	2641	2650	rVB2	328	258	0.02%	0.002%
56	10.149	2822	2833	2863	rBV	409083	644749	42.34%	5.951%
57	10.326	2877	2888	2895	rBV4	2922	5216	0.34%	0.048%
58	10.407	2908	2913	2919	rBV2	421	409	0.03%	0.004%
59	10.715	3000	3009	3012	rBV3	535	715	0.05%	0.007%
60	10.956	3080	3084	3087	rVV2	456	362	0.02%	0.003%
61	11.133	3131	3139	3144	rBV2	730	928	0.06%	0.009%
62	11.185	3144	3155	3180	rBV	544837	867932	57.00%	8.011%
63	11.558	3260	3271	3297	rVV	653576	1029533	67.61%	9.503%
64	11.780	3338	3340	3344	rVB2	460	273	0.02%	0.003%
65	11.995	3405	3407	3414	rVB2	381	340	0.02%	0.003%
66	12.191	3462	3468	3476	rVB3	961	1223	0.08%	0.011%
67	12.336	3510	3513	3517	rBV2	428	356	0.02%	0.003%
68	12.435	3541	3544	3548	rVB	375	261	0.02%	0.002%
69	12.474	3552	3556	3560	rBV2	296	240	0.02%	0.002%
70	12.497	3560	3563	3569	rBV3	231	257	0.02%	0.002%
71	12.693	3619	3624	3625	rBV2	253	225	0.01%	0.002%
72	12.834	3662	3668	3671	rBV2	455	438	0.03%	0.004%
73	12.969	3705	3710	3718	rVB2	421	478	0.03%	0.004%
74	13.111	3748	3754	3757	rBV	454	481	0.03%	0.004%
75	13.197	3777	3781	3782	rBV2	333	221	0.01%	0.002%
76	13.207	3782	3784	3791	rVB4	1120	1143	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034808.D
 Acq On : 22 Mar 2024 10:56
 Operator : SY/MD
 Sample : P1822-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0786

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	13.242	3791	3795	3804	rBV3	326	437	0.03%	0.004%
78	13.310	3812	3816	3820	rBV	331	329	0.02%	0.003%
79	13.352	3826	3829	3832	rBV	322	240	0.02%	0.002%
80	13.451	3852	3860	3869	rBV6	2224	3768	0.25%	0.035%
81	13.570	3894	3897	3901	rVB3	562	481	0.03%	0.004%
82	13.593	3901	3904	3910	rVB	656	462	0.03%	0.004%
83	13.635	3912	3917	3919	rBV2	573	467	0.03%	0.004%
84	13.686	3927	3933	3935	rBV5	1068	1081	0.07%	0.010%
85	13.738	3945	3949	3954	rBV4	446	347	0.02%	0.003%
86	13.876	3989	3992	3995	rBV	370	285	0.02%	0.003%
87	13.892	3995	3997	4004	rVV3	286	238	0.02%	0.002%
88	14.027	4033	4039	4043	rBV3	561	704	0.05%	0.006%
89	14.101	4061	4062	4066	rBV2	257	215	0.01%	0.002%
90	14.268	4112	4114	4119	rVB2	434	334	0.02%	0.003%
91	14.300	4120	4124	4129	rBV2	300	364	0.02%	0.003%
92	14.345	4134	4138	4141	rVV2	471	295	0.02%	0.003%
93	14.458	4171	4173	4177	rVB	457	218	0.01%	0.002%
94	14.519	4190	4192	4198	rVB4	280	230	0.02%	0.002%
95	14.837	4289	4291	4294	rBV2	384	296	0.02%	0.003%
96	14.882	4303	4305	4309	rBV3	347	321	0.02%	0.003%
97	14.963	4325	4330	4333	rBV3	719	632	0.04%	0.006%
98	15.033	4350	4352	4355	rVB3	706	313	0.02%	0.003%
99	15.207	4404	4406	4412	rBV5	562	493	0.03%	0.005%
100	15.648	4541	4543	4547	rBV5	701	443	0.03%	0.004%




Sum of corrected areas: 10834117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034808.D
Acq On : 22 Mar 2024 10:56
Operator : SY/MD
Sample : P1822-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0786

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

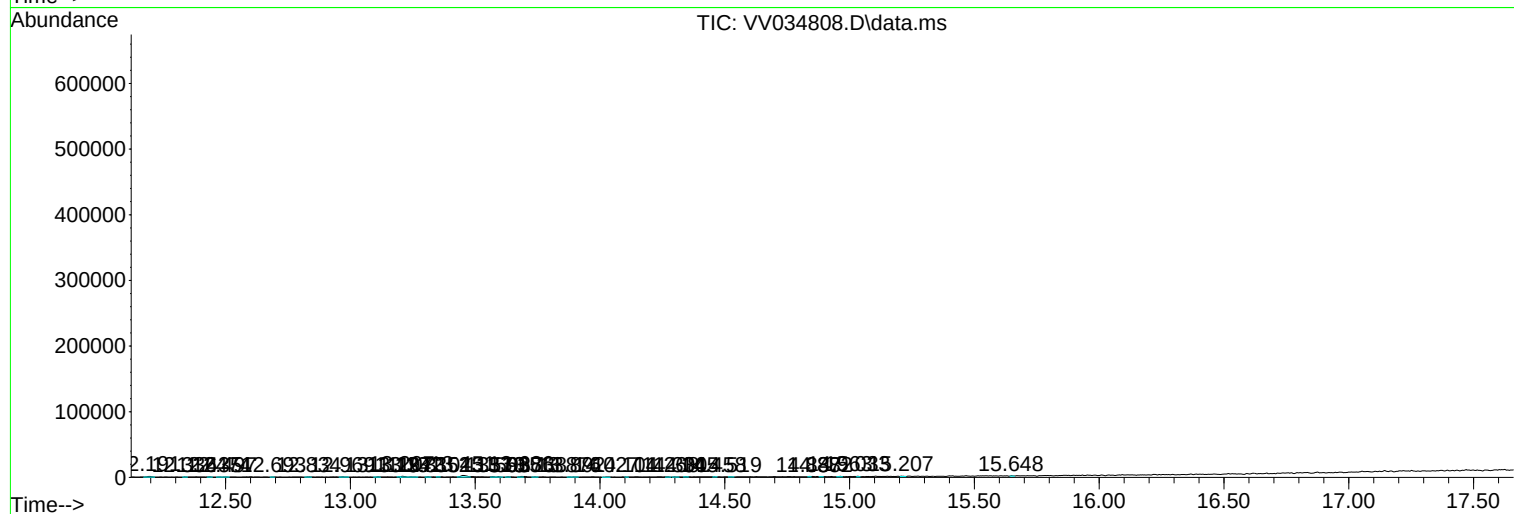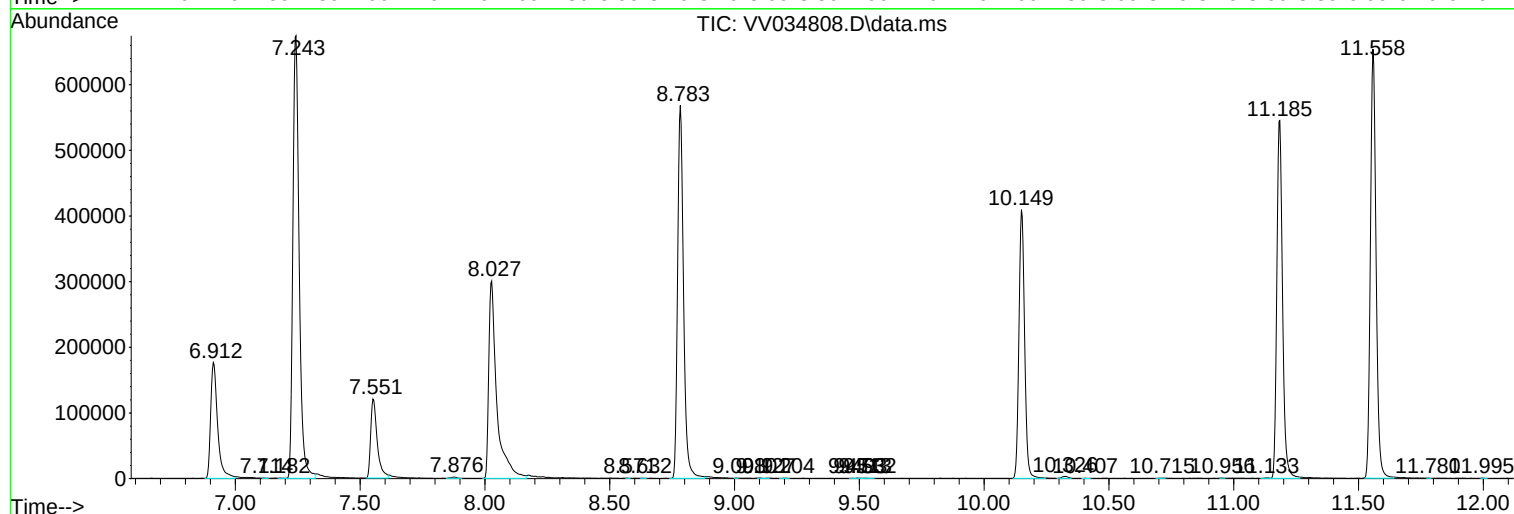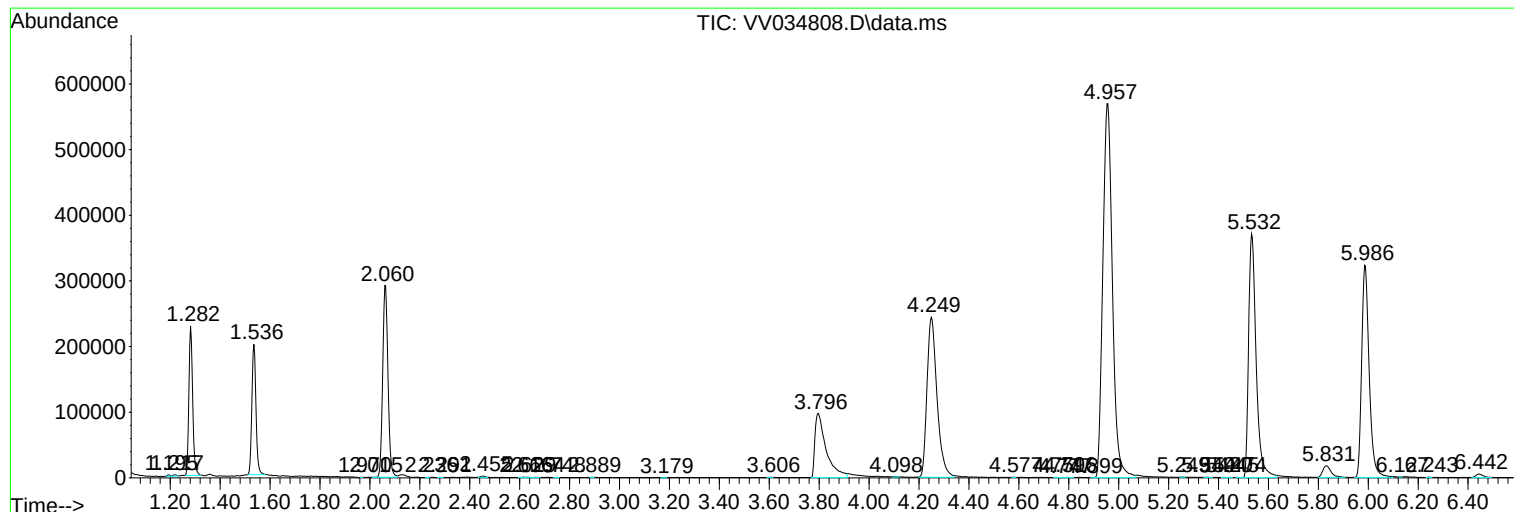

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034808.D
Acq On : 22 Mar 2024 10:56
Operator : SY/MD
Sample : P1822-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0786

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034808.D
Acq On : 22 Mar 2024 10:56
Operator : SY/MD
Sample : P1822-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0786

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------