

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034809.D
 Acq On : 22 Mar 2024 11:20
 Operator : SY/MD
 Sample : P1743-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034809.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	220695	235847	16.10%	2.254%
2	1.532	146	153	168	rVB	190777	218131	14.89%	2.085%
3	2.059	306	317	335	rBV	304588	450034	30.72%	4.301%
4	2.449	430	438	449	rVB3	2841	4732	0.32%	0.045%
5	2.613	485	489	494	rBV2	305	316	0.02%	0.003%
6	2.860	564	566	567	rVB2	249	64	0.00%	0.001%
7	2.915	582	583	584	rBV	200	58	0.00%	0.001%
8	3.043	622	623	624	rBV	179	36	0.00%	0.000%
9	3.252	685	688	692	rVB2	199	135	0.01%	0.001%
10	3.362	720	722	724	rBV	126	54	0.00%	0.001%
11	3.403	732	735	737	rBV2	163	90	0.01%	0.001%
12	3.426	741	742	743	rBV2	106	28	0.00%	0.000%
13	3.439	743	746	748	rBV2	176	125	0.01%	0.001%
14	3.793	847	856	910	rBV	94454	294525	20.10%	2.815%
15	4.246	983	997	1029	rBV	223007	579292	39.54%	5.536%
16	4.577	1099	1100	1110	rVB4	592	571	0.04%	0.005%
17	4.709	1138	1141	1142	rBV	240	119	0.01%	0.001%
18	4.757	1153	1156	1158	rBV2	202	144	0.01%	0.001%
19	4.780	1161	1163	1169	rVB2	264	187	0.01%	0.002%
20	4.828	1175	1178	1181	rBV	292	231	0.02%	0.002%
21	4.895	1198	1199	1202	rBV2	160	116	0.01%	0.001%
22	4.953	1202	1217	1256	rBV2	548173	1465096	100.00%	14.001%
23	5.362	1343	1344	1346	rBV2	167	55	0.00%	0.001%
24	5.374	1346	1348	1351	rBV3	231	109	0.01%	0.001%
25	5.532	1385	1397	1438	rBV	371940	776795	53.02%	7.424%
26	5.831	1480	1490	1513	rVB3	12307	27881	1.90%	0.266%
27	5.985	1525	1538	1569	rBV2	310150	646132	44.10%	6.175%
28	6.365	1653	1656	1657	rBV2	203	119	0.01%	0.001%
29	6.461	1683	1686	1690	rBV2	331	216	0.01%	0.002%
30	6.481	1690	1692	1695	rVB2	226	104	0.01%	0.001%
31	6.493	1695	1696	1697	rBV2	136	42	0.00%	0.000%
32	6.554	1714	1715	1716	rVB	169	33	0.00%	0.000%
33	6.657	1745	1747	1748	rBV	202	88	0.01%	0.001%
34	6.754	1774	1777	1779	rBV2	272	168	0.01%	0.002%
35	6.911	1815	1826	1856	rBV	170563	324783	22.17%	3.104%
36	7.239	1916	1928	1958	rBV	643540	1144342	78.11%	10.936%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034809.D
 Acq On : 22 Mar 2024 11:20
 Operator : SY/MD
 Sample : P1743-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	7.551	2016	2025	2061	rBV	112700	217159	14.82%	2.075%
38	7.831	2107	2112	2115	rBV2	320	180	0.01%	0.002%
39	7.953	2148	2150	2156	rVB	307	195	0.01%	0.002%
40	8.027	2164	2173	2223	rBV2	291548	636487	43.44%	6.083%
41	8.689	2377	2379	2380	rBV	340	114	0.01%	0.001%
42	8.722	2386	2389	2392	rBV2	140	105	0.01%	0.001%
43	8.783	2397	2408	2432	rBV	562617	931978	63.61%	8.907%
44	9.104	2504	2508	2509	rBV	345	246	0.02%	0.002%
45	9.152	2520	2523	2529	rVB3	366	353	0.02%	0.003%
46	9.259	2554	2556	2558	rBV2	203	98	0.01%	0.001%
47	9.423	2606	2607	2609	rBV	167	36	0.00%	0.000%
48	9.490	2627	2628	2630	rBV	226	83	0.01%	0.001%
49	9.522	2636	2638	2640	rBV	248	83	0.01%	0.001%
50	9.558	2647	2649	2650	rBV2	143	36	0.00%	0.000%
51	9.680	2684	2687	2691	rBV	207	194	0.01%	0.002%
52	9.776	2711	2717	2720	rBV	301	299	0.02%	0.003%
53	10.149	2821	2833	2860	rBV	407511	635945	43.41%	6.078%
54	10.371	2898	2902	2908	rBV2	306	241	0.02%	0.002%
55	10.403	2908	2912	2914	rBV2	221	179	0.01%	0.002%
56	10.484	2935	2937	2940	rBV2	302	148	0.01%	0.001%
57	10.921	3070	3073	3076	rBV2	232	177	0.01%	0.002%
58	11.014	3101	3102	3104	rBV	239	100	0.01%	0.001%
59	11.185	3143	3155	3190	rBV	549788	871068	59.45%	8.325%
60	11.558	3259	3271	3294	rBV	623593	990444	67.60%	9.465%
61	11.795	3342	3345	3346	rBV	201	97	0.01%	0.001%
62	11.824	3351	3354	3357	rBV	214	124	0.01%	0.001%
63	11.850	3360	3362	3365	rVB	142	64	0.00%	0.001%
64	11.934	3386	3388	3390	rVB	153	45	0.00%	0.000%
65	12.030	3415	3418	3421	rVB	172	86	0.01%	0.001%
66	12.066	3427	3429	3433	rBV2	130	80	0.01%	0.001%
67	12.104	3438	3441	3444	rBV	107	60	0.00%	0.001%
68	12.117	3444	3445	3447	rBV	157	36	0.00%	0.000%
69	12.139	3449	3452	3456	rBV2	217	183	0.01%	0.002%
70	12.184	3462	3466	3469	rBV4	734	756	0.05%	0.007%
71	12.239	3481	3483	3484	rBV	173	70	0.00%	0.001%
72	12.313	3503	3506	3511	rBV2	179	169	0.01%	0.002%
73	12.419	3535	3539	3542	rVB2	161	128	0.01%	0.001%
74	12.435	3542	3544	3547	rBV	126	71	0.00%	0.001%
75	12.455	3547	3550	3553	rVB2	185	104	0.01%	0.001%
76	12.480	3553	3558	3560	rBV	163	101	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034809.D
 Acq On : 22 Mar 2024 11:20
 Operator : SY/MD
 Sample : P1743-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

77	12.493	3560	3562	3565	rVB	136	75	0.01%	0.001%
78	12.512	3565	3568	3571	rBV2	65	57	0.00%	0.001%
79	12.538	3574	3576	3578	rBV2	90	60	0.00%	0.001%
80	12.580	3583	3589	3590	rBV	290	211	0.01%	0.002%
81	12.622	3599	3602	3605	rBV2	208	137	0.01%	0.001%
82	12.635	3605	3606	3607	rBV	160	52	0.00%	0.000%
83	12.670	3615	3617	3619	rBV	100	52	0.00%	0.000%
84	12.770	3644	3648	3650	rBV	328	260	0.02%	0.002%
85	13.104	3751	3752	3756	rBV2	310	164	0.01%	0.002%
86	13.127	3756	3759	3763	rBV2	363	354	0.02%	0.003%
87	13.458	3852	3862	3871	rBV5	1641	3066	0.21%	0.029%
88	14.329	4129	4133	4139	rBV4	493	475	0.03%	0.005%




Sum of corrected areas: 10463883

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034809.D
Acq On : 22 Mar 2024 11:20
Operator : SY/MD
Sample : P1743-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

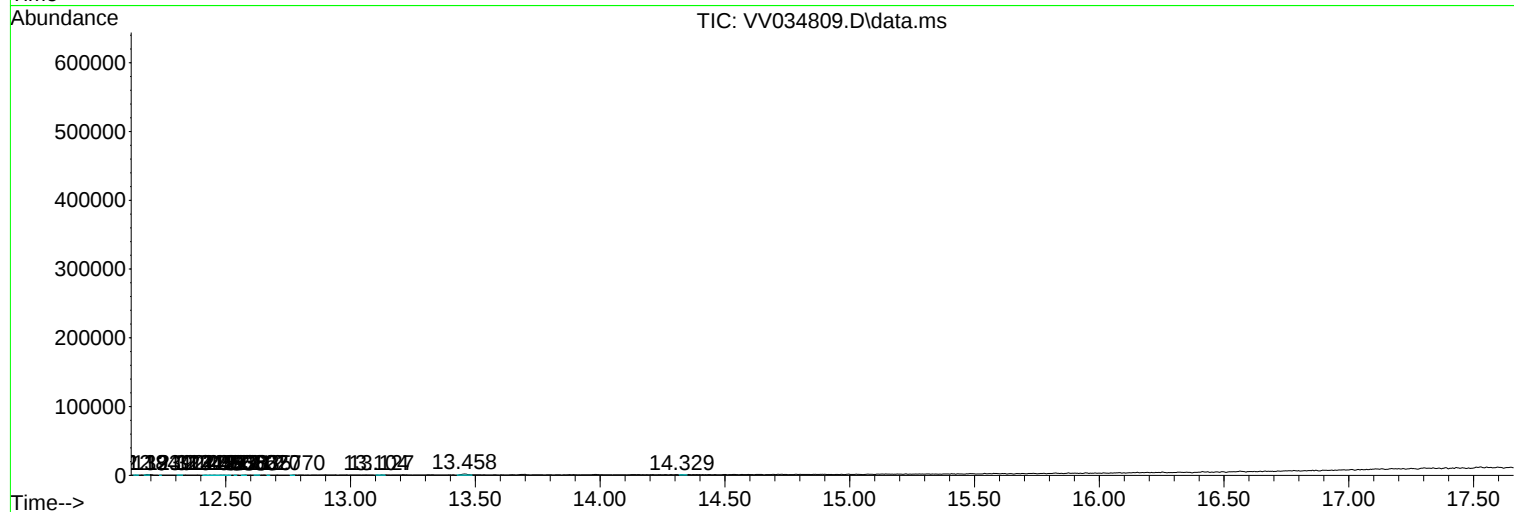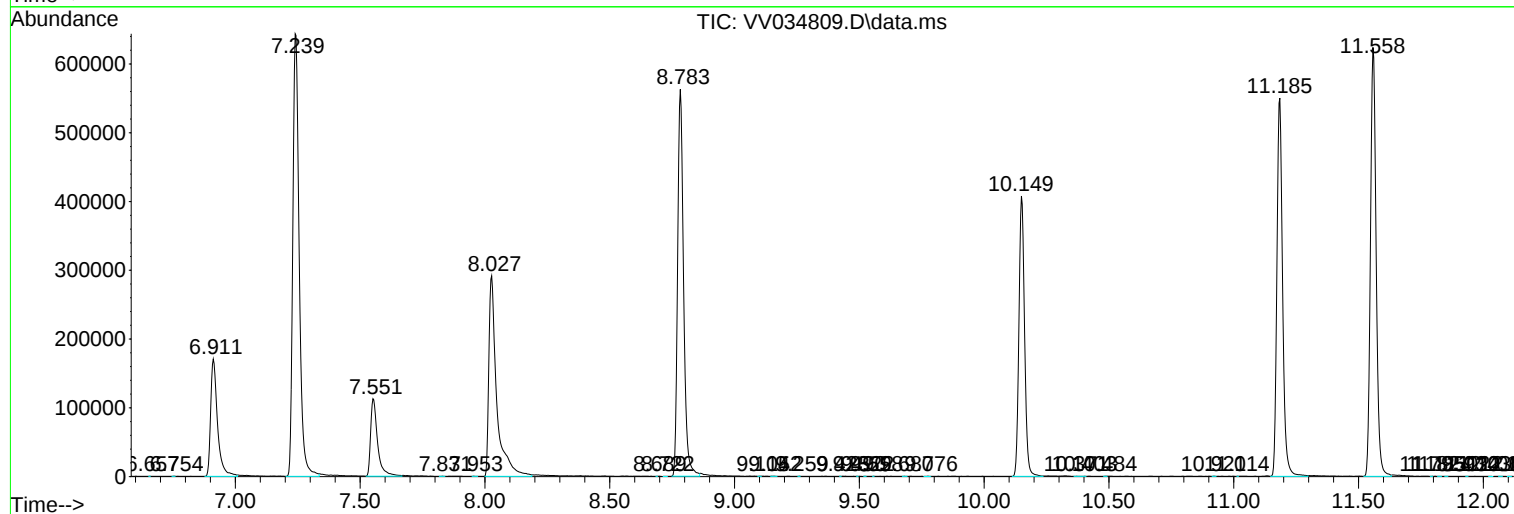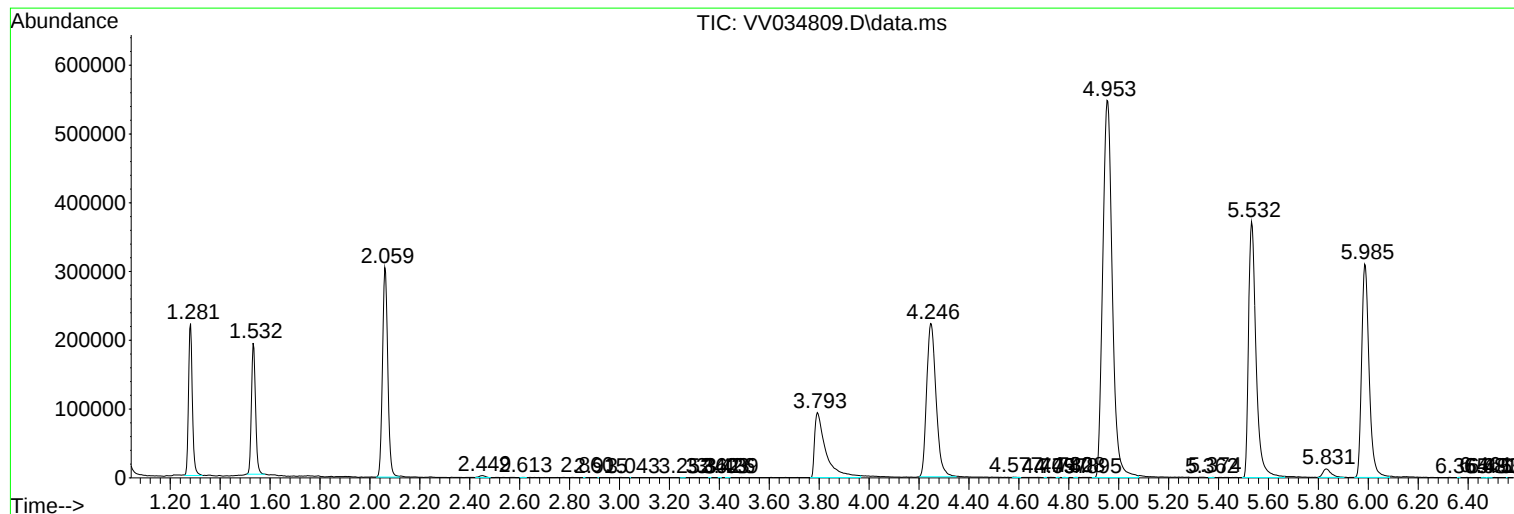

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034809.D
Acq On : 22 Mar 2024 11:20
Operator : SY/MD
Sample : P1743-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034809.D
Acq On : 22 Mar 2024 11:20
Operator : SY/MD
Sample : P1743-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------