

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034811.D
 Acq On : 22 Mar 2024 12:07
 Operator : SY/MD
 Sample : P1757-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034811.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	91	rVB	219336	234913	11.16%	1.946%
2	1.532	146	153	168	rVB	194757	217104	10.31%	1.798%
3	1.986	292	294	296	rBV2	407	190	0.01%	0.002%
4	2.018	301	304	306	rBV	432	176	0.01%	0.001%
5	2.060	306	317	339	rBV	283279	416154	19.77%	3.447%
6	2.449	431	438	448	rVB5	2063	3410	0.16%	0.028%
7	2.629	493	494	495	rBV5	146	43	0.00%	0.000%
8	2.690	509	513	514	rBV	302	179	0.01%	0.001%
9	2.783	538	542	544	rBV2	261	159	0.01%	0.001%
10	2.815	549	552	556	rBV	186	155	0.01%	0.001%
11	2.982	598	604	606	rBV	189	178	0.01%	0.001%
12	2.992	606	607	608	rVB	133	30	0.00%	0.000%
13	3.031	616	619	621	rBV	127	72	0.00%	0.001%
14	3.105	638	642	644	rBV	167	144	0.01%	0.001%
15	3.179	664	665	666	rVB	155	30	0.00%	0.000%
16	3.188	666	668	670	rVV2	134	71	0.00%	0.001%
17	3.214	673	676	679	rVB	167	100	0.00%	0.001%
18	3.317	706	708	711	rBV	192	89	0.00%	0.001%
19	3.365	720	723	726	rBV2	187	110	0.01%	0.001%
20	3.384	726	729	735	rBV2	146	161	0.01%	0.001%
21	3.513	767	769	770	rBV2	140	34	0.00%	0.000%
22	3.593	791	794	796	rBV2	159	103	0.00%	0.001%
23	3.609	796	799	804	rVV	192	139	0.01%	0.001%
24	3.671	812	818	819	rBV2	143	166	0.01%	0.001%
25	3.706	828	829	831	rBV	147	37	0.00%	0.000%
26	3.722	832	834	837	rVB	183	107	0.01%	0.001%
27	3.748	837	842	847	rBV2	211	247	0.01%	0.002%
28	3.793	847	856	896	rBV2	102708	315928	15.01%	2.617%
29	4.246	982	997	1032	rBV	239300	617897	29.36%	5.118%
30	4.706	1132	1140	1142	rBV3	357	449	0.02%	0.004%
31	4.953	1200	1217	1268	rBV2	577893	1625066	77.21%	13.459%
32	5.394	1352	1354	1355	rBV2	159	38	0.00%	0.000%
33	5.439	1366	1368	1371	rBV	271	196	0.01%	0.002%
34	5.532	1386	1397	1427	rBV	395318	809238	38.45%	6.702%
35	5.831	1480	1490	1506	rBV5	12337	26672	1.27%	0.221%
36	5.986	1526	1538	1571	rBV	330008	680250	32.32%	5.634%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034811.D
 Acq On : 22 Mar 2024 12:07
 Operator : SY/MD
 Sample : P1757-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.362	1652	1655	1658	rBV2	189	131	0.01%	0.001%
38	6.394	1664	1665	1667	rBV	132	55	0.00%	0.000%
39	6.413	1667	1671	1675	rVB2	300	236	0.01%	0.002%
40	6.452	1679	1683	1687	rBV3	165	183	0.01%	0.002%
41	6.468	1687	1688	1690	rVB	149	56	0.00%	0.000%
42	6.497	1694	1697	1702	rBV2	180	196	0.01%	0.002%
43	6.551	1710	1714	1716	rBV	200	147	0.01%	0.001%
44	6.683	1753	1755	1756	rBV	204	45	0.00%	0.000%
45	6.728	1768	1769	1771	rVB	154	54	0.00%	0.000%
46	6.805	1790	1793	1795	rBV2	124	62	0.00%	0.001%
47	6.822	1795	1798	1799	rBV	121	70	0.00%	0.001%
48	6.912	1816	1826	1858	rBV	176512	342289	16.26%	2.835%
49	7.178	1907	1909	1910	rBV2	278	92	0.00%	0.001%
50	7.239	1917	1928	1969	rBV	673745	1193639	56.71%	9.886%
51	7.551	2016	2025	2054	rBV	122530	227671	10.82%	1.886%
52	7.870	2121	2124	2126	rBV2	356	218	0.01%	0.002%
53	7.899	2132	2133	2134	rBV2	137	41	0.00%	0.000%
54	7.989	2158	2161	2163	rBV2	341	203	0.01%	0.002%
55	8.024	2163	2172	2211	rBV	319129	679063	32.26%	5.624%
56	8.471	2309	2311	2314	rBV3	469	213	0.01%	0.002%
57	8.542	2329	2333	2336	rBV3	240	232	0.01%	0.002%
58	8.625	2357	2359	2360	rBV	173	68	0.00%	0.001%
59	8.725	2388	2390	2392	rBV	148	76	0.00%	0.001%
60	8.783	2397	2408	2410	rBV	668419	812881	38.62%	6.732%
61	9.217	2540	2543	2544	rBV	316	137	0.01%	0.001%
62	9.281	2561	2563	2567	rVB2	304	164	0.01%	0.001%
63	9.301	2567	2569	2571	rBV	283	114	0.01%	0.001%
64	9.381	2589	2594	2597	rBV3	424	348	0.02%	0.003%
65	9.484	2624	2626	2627	rBV	232	91	0.00%	0.001%
66	9.561	2647	2650	2653	rBV2	204	140	0.01%	0.001%
67	9.699	2691	2693	2694	rBV2	149	66	0.00%	0.001%
68	9.873	2741	2747	2754	rBV4	405	571	0.03%	0.005%
69	9.976	2777	2779	2783	rVB2	301	92	0.00%	0.001%
70	10.082	2809	2812	2814	rBV	181	90	0.00%	0.001%
71	10.149	2821	2833	2857	rBV	430666	684819	32.53%	5.672%
72	10.310	2881	2883	2885	rBV2	277	123	0.01%	0.001%
73	10.413	2912	2915	2918	rBV2	335	199	0.01%	0.002%
74	10.490	2933	2939	2942	rBV2	523	643	0.03%	0.005%
75	10.651	2986	2989	2993	rBV2	300	264	0.01%	0.002%
76	10.866	3053	3056	3059	rBV3	492	304	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
 Data File : VV034811.D
 Acq On : 22 Mar 2024 12:07
 Operator : SY/MD
 Sample : P1757-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.117	3125	3134	3145	rBV2	90740	145299	6.90%	1.203%
78	11.185	3145	3155	3157	rBV	702065	881343	41.87%	7.299%
79	11.452	3235	3238	3239	rBV2	291	137	0.01%	0.001%
80	11.564	3259	3273	3300	rBV2	887528	2104870	100.00%	17.433%
81	11.834	3354	3357	3360	rBV2	321	186	0.01%	0.002%
82	11.905	3376	3379	3384	rBV2	530	208	0.01%	0.002%
83	12.046	3419	3423	3428	rBV2	247	244	0.01%	0.002%
84	12.175	3461	3463	3464	rBV	385	130	0.01%	0.001%
85	12.355	3514	3519	3522	rBV2	748	699	0.03%	0.006%
86	12.403	3532	3534	3536	rBV	271	138	0.01%	0.001%
87	12.529	3571	3573	3575	rBV3	256	126	0.01%	0.001%
88	12.593	3585	3593	3598	rBV2	683	905	0.04%	0.007%
89	12.715	3629	3631	3633	rBV	257	93	0.00%	0.001%
90	12.824	3663	3665	3669	rBV	377	262	0.01%	0.002%
91	13.201	3774	3782	3794	rBV3	17270	27100	1.29%	0.224%
92	13.423	3848	3851	3854	rBV2	420	353	0.02%	0.003%
93	13.683	3923	3932	3945	rBV4	9290	15533	0.74%	0.129%
94	13.796	3965	3967	3969	rBV3	368	88	0.00%	0.001%
95	13.831	3976	3978	3981	rBV2	481	251	0.01%	0.002%

Sum of corrected areas: 12074086




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034811.D
Acq On : 22 Mar 2024 12:07
Operator : SY/MD
Sample : P1757-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

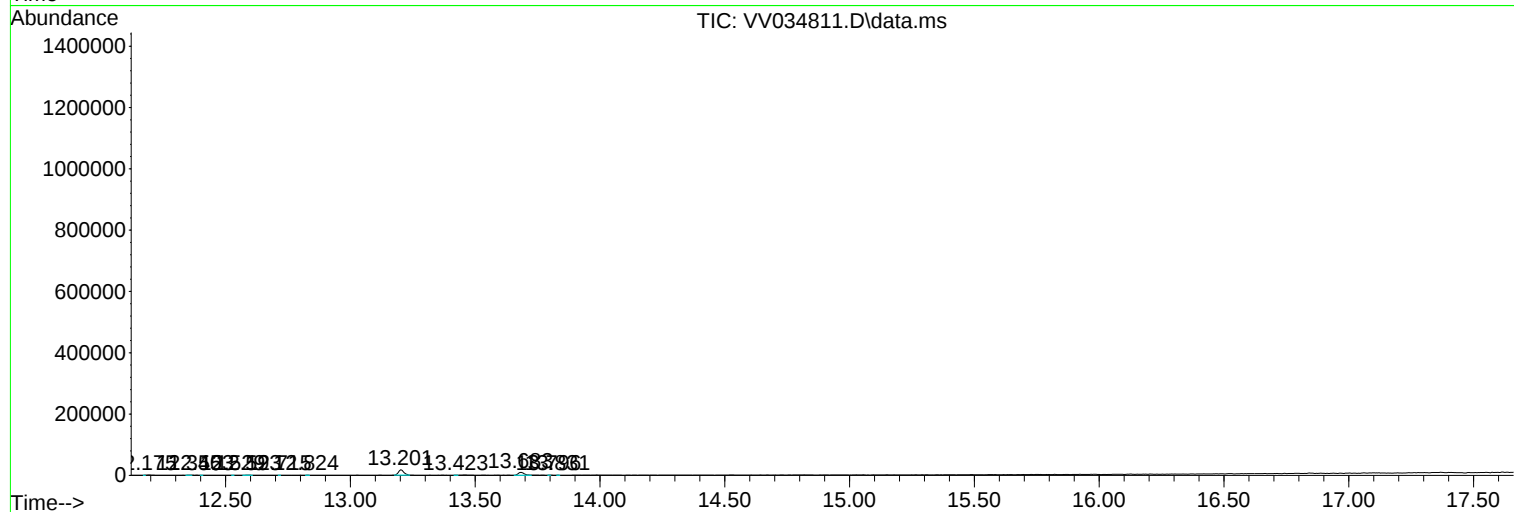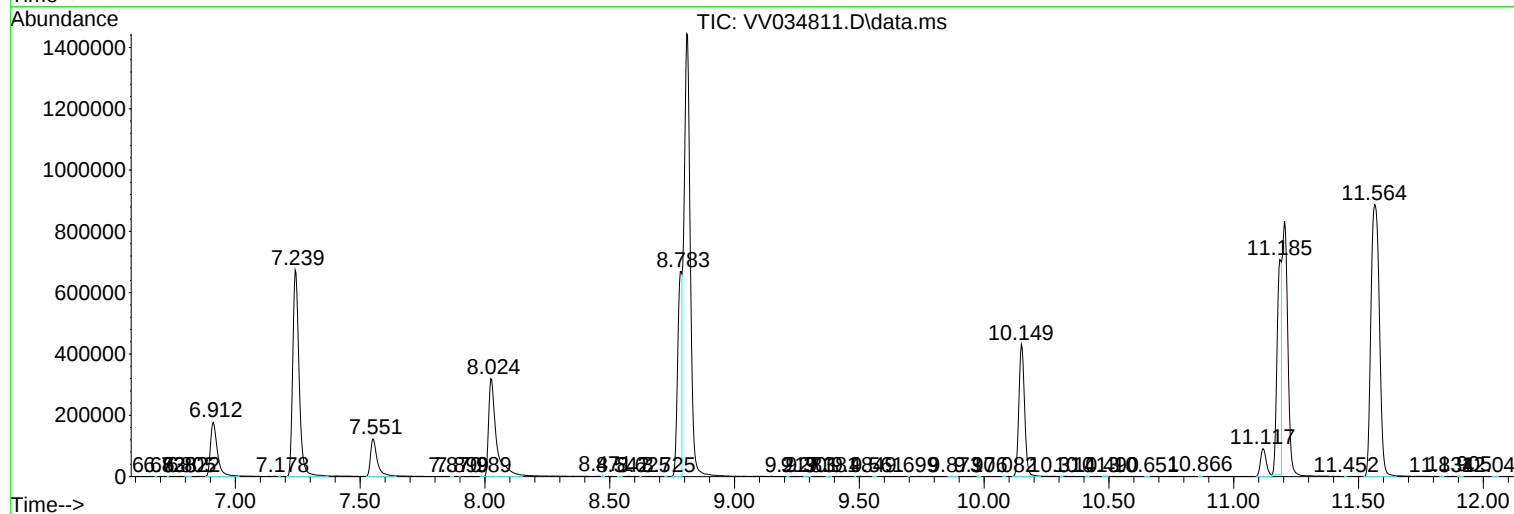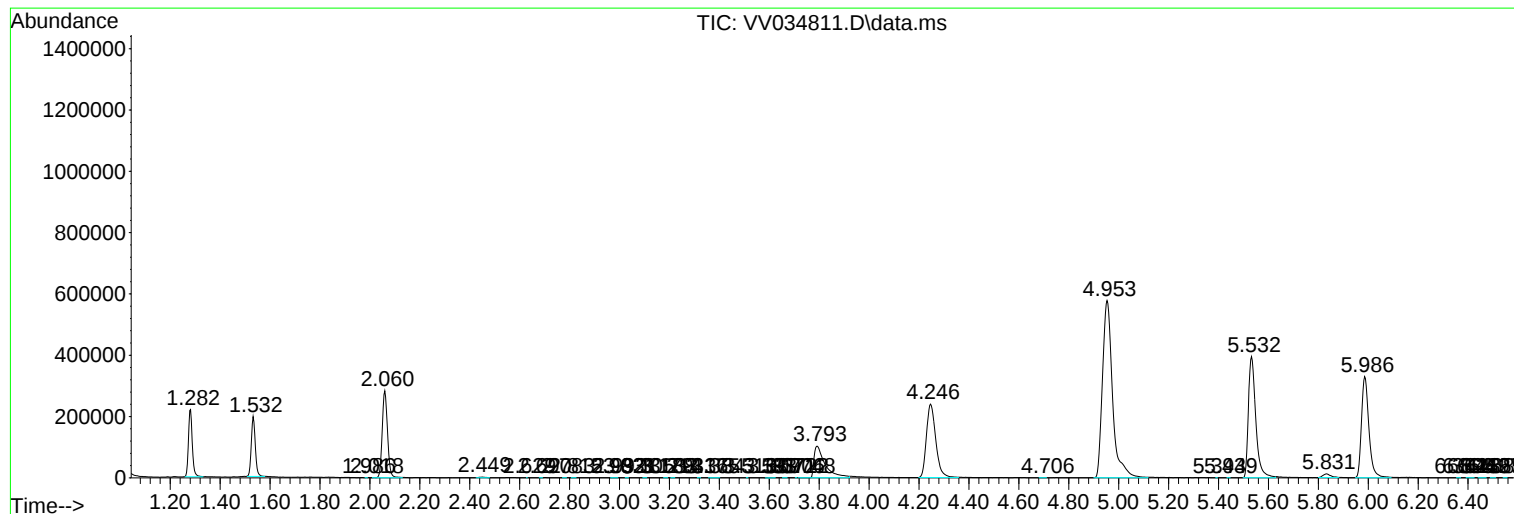

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034811.D
Acq On : 22 Mar 2024 12:07
Operator : SY/MD
Sample : P1757-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032224\
Data File : VV034811.D
Acq On : 22 Mar 2024 12:07
Operator : SY/MD
Sample : P1757-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
