


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032319\
 Data File : VV009844.D
 Acq On : 23 Mar 2019 09:44
 Operator : SY/MD
 Sample : BFB34
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB34

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR032119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Mar 23 21:59:27 2019

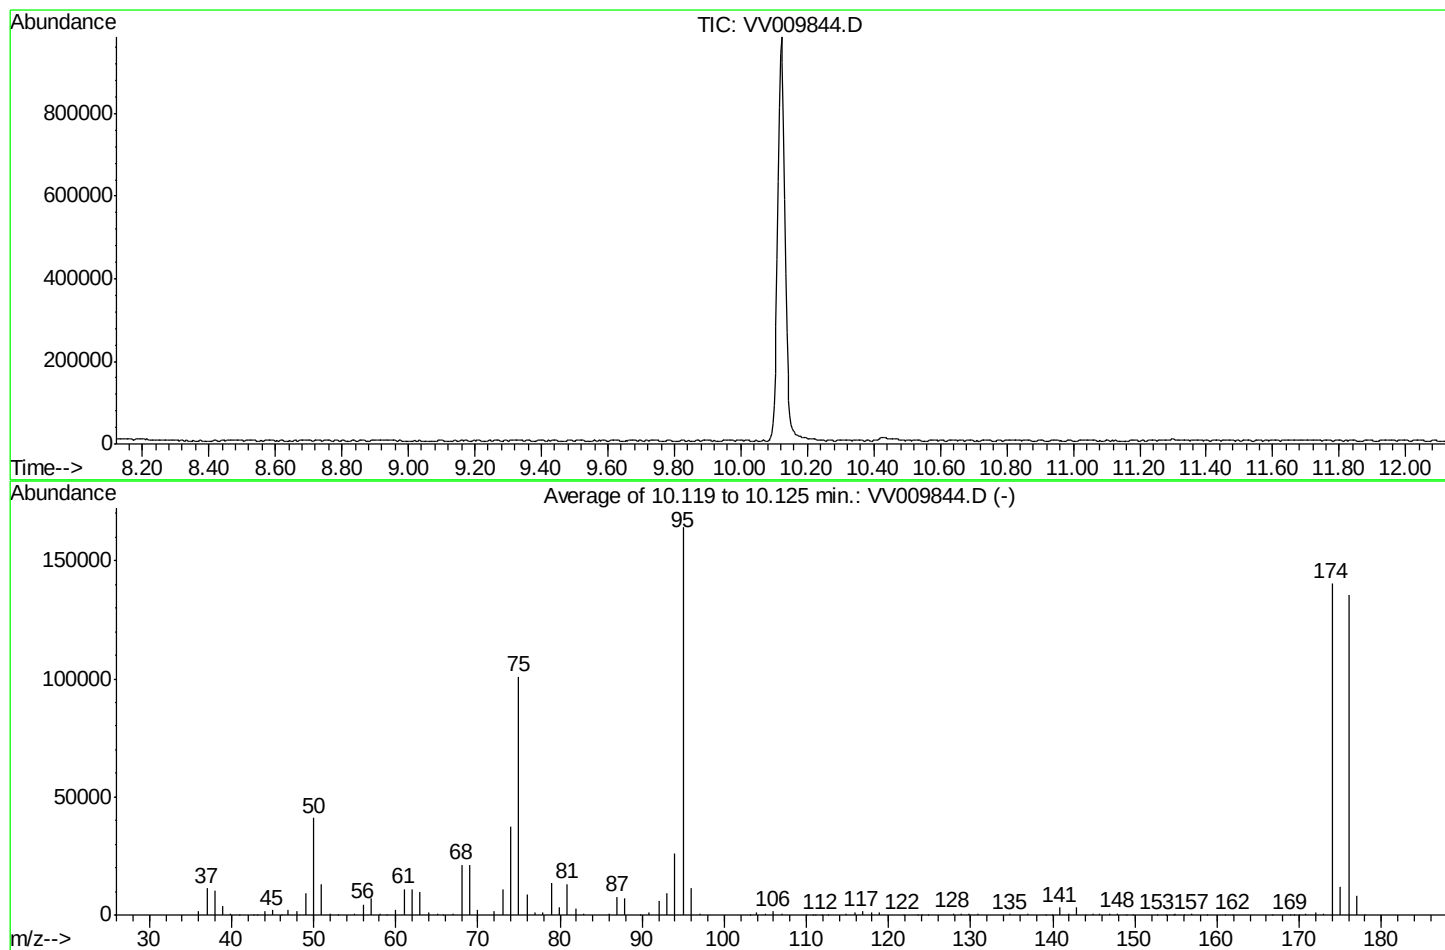

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	40984	PASS
75	95	30	80	61.6	101093	PASS
95	95	100	100	100.0	164202	PASS
96	95	5	9	6.9	11297	PASS
173	174	0.00	2	0.5	650	PASS
174	95	50	120	85.4	140181	PASS
175	174	5	9	8.4	11792	PASS
176	174	95	101	96.8	135656	PASS
177	176	5	9	6.1	8232	PASS

Scan 2794 (10.074 min): VV009844.D
BFB34

m/z	Abundance
35.20	101.0
39.10	129.0
39.90	7035.0
44.10	293.0
106.10	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	2000.0
37.00	11293.0
38.00	10691.0
39.00	4106.0
39.90	7962.0
40.90	137.0
43.10	293.0
44.00	2357.0
45.00	2174.0
46.10	305.0
46.90	1870.0
48.00	1649.0
49.00	9529.0
50.00	41344.0
51.00	12337.0
52.00	675.0
53.00	193.0
55.00	778.0
56.00	4714.0
57.00	7608.0
58.00	314.0
58.80	113.0
60.00	2396.0
61.00	10943.0
62.00	11057.0
63.00	9480.0
64.00	883.0
65.10	521.0
66.90	520.0
68.00	21904.0
69.00	21664.0
70.00	2213.0
72.00	1480.0
73.00	11201.0
74.00	38384.0
75.00	101920.0
76.00	8929.0
76.90	1131.0
78.00	783.0
78.90	13611.0
79.90	3301.0
80.90	13479.0
81.90	2850.0
82.90	453.0
86.00	392.0
87.00	7518.0
87.90	7019.0
89.80	146.0
90.80	1017.0
92.00	6078.0
93.00	8891.0
94.00	25648.0
95.00	164608.0
96.00	11397.0
97.00	329.0
103.90	1102.0
104.90	371.0
105.90	1564.0
106.90	334.0
109.90	275.0
111.00	413.0
111.80	302.0
112.60	278.0
114.80	488.0
115.90	836.0
116.80	1468.0
117.90	1083.0
118.90	1157.0
121.80	108.0
124.00	143.0
124.80	127.0
127.80	742.0
128.90	319.0
129.90	778.0
130.90	358.0
134.90	391.0
136.90	407.0
139.90	103.0
140.90	3246.0
141.80	396.0
142.90	2926.0
143.90	230.0
144.80	322.0
145.70	342.0
146.90	368.0
147.90	588.0
148.90	101.0
149.70	210.0
152.70	187.0
153.70	133.0
154.70	331.0
156.00	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

156.90	393.0
158.80	172.0
160.90	355.0
168.90	164.0
170.00	165.0
170.80	381.0
171.90	1198.0
174.00	135360.0
175.00	11390.0
176.00	130680.0
177.00	8249.0
177.90	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	1925.0
37.00	11824.0
38.00	10629.0
39.00	4212.0
39.90	7727.0
40.90	120.0
43.10	263.0
44.00	2190.0
45.00	2084.0
46.10	291.0
47.00	2004.0
48.00	1563.0
49.00	9324.0
50.00	42808.0
51.00	13576.0
52.00	686.0
52.90	218.0
55.00	833.0
56.00	4640.0
57.00	7480.0
58.00	358.0
60.00	2200.0
61.00	11340.0
62.00	11192.0
63.00	9894.0
64.00	993.0
65.10	498.0
65.80	101.0
66.80	488.0
68.00	22160.0
69.00	21592.0
70.00	2209.0
72.00	1426.0
73.00	11489.0
74.00	38704.0
75.00	105152.0
76.00	8890.0
76.90	1055.0
78.00	829.0
78.90	14056.0
79.90	3310.0
80.90	13633.0
81.90	3010.0
82.90	488.0
86.00	335.0
87.00	7793.0
87.90	7233.0
89.80	118.0
90.80	1137.0
92.00	6446.0
93.00	9402.0
94.00	26872.0
95.00	170688.0
96.00	11839.0
97.00	379.0
103.10	110.0
103.90	1284.0
105.00	345.0
106.00	1832.0
106.90	350.0
109.90	320.0
110.70	403.0
111.80	292.0
112.70	265.0
114.90	418.0
115.90	952.0
116.80	1545.0
117.90	1039.0
118.90	1243.0
123.50	101.0
124.10	184.0
124.90	111.0
127.80	809.0
128.90	320.0
129.80	673.0
130.80	338.0
134.80	392.0
136.90	443.0
139.10	119.0
139.80	215.0
140.90	3296.0
141.90	469.0
142.90	3270.0
144.00	223.0
144.90	329.0
145.70	393.0
146.90	342.0
147.90	662.0
149.70	166.0
152.70	235.0
153.80	116.0
154.90	387.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

155.90	115.0
156.90	441.0
158.80	253.0
160.90	300.0
166.70	138.0
168.90	174.0
169.30	177.0
169.90	147.0
170.80	298.0
172.00	1340.0
174.00	144960.0
175.00	12259.0
176.00	140608.0
177.00	8530.0
177.90	237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	1699.0
37.00	10901.0
38.00	9802.0
39.00	3934.0
39.90	7577.0
42.70	121.0
43.20	255.0
44.00	2066.0
45.00	1777.0
46.10	288.0
47.00	2063.0
48.00	1248.0
49.00	8432.0
50.00	38800.0
51.00	12998.0
52.00	579.0
52.90	198.0
55.10	746.0
56.00	4354.0
57.00	6720.0
58.10	375.0
60.00	1930.0
61.00	10357.0
62.00	10187.0
63.00	9441.0
64.00	871.0
65.10	490.0
65.80	121.0
67.00	427.0
68.00	19848.0
69.00	19752.0
70.00	1954.0
72.00	1306.0
73.00	10628.0
74.00	35824.0
75.00	96208.0
76.10	7654.0
77.00	1020.0
77.90	904.0
78.90	12826.0
79.90	3044.0
80.90	12409.0
81.90	2752.0
82.80	429.0
86.10	203.0
86.90	7556.0
87.90	6685.0
90.90	1169.0
92.00	6128.0
93.00	8985.0
94.00	25584.0
95.00	157312.0
96.00	10655.0
97.00	329.0
103.90	1265.0
105.00	369.0
106.00	1761.0
107.00	267.0
110.00	266.0
110.70	357.0
111.90	209.0
112.80	253.0
114.90	278.0
115.80	943.0
116.80	1454.0
117.90	839.0
118.90	1247.0
124.10	166.0
124.90	107.0
127.90	763.0
128.90	324.0
129.90	620.0
130.90	283.0
134.70	397.0
136.90	416.0
139.80	299.0
140.90	2926.0
141.90	465.0
142.90	3242.0
144.00	186.0
144.90	296.0
145.70	317.0
146.80	217.0
147.90	619.0
152.70	229.0
153.80	112.0
154.90	535.0
156.90	405.0
158.80	264.0
160.90	225.0
161.90	113.0
166.70	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

168.90	100.0
169.30	217.0
169.90	108.0
170.80	234.0
172.00	1372.0
173.00	1950.0
174.00	140224.0
175.00	11727.0
176.00	135680.0
177.00	7919.0
177.90	221.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34