

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032321\
 Data File : VW020713.D
 Acq On : 23 Mar 2021 14:08
 Operator : SY/MD
 Sample : M1783-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G12

Quant Time: Mar 24 04:18:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 23 02:12:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	483859	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	475073	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	217030	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	163146	41.80	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.60%		
7) Chloroethane-d5	1.571	69	118020	37.80	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	75.60%		
11) 1,1-Dichloroethene-d2	2.108	63	214458	28.91	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	57.82%#		
21) 2-Butanone-d5	3.883	46	201655	80.50	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	80.50%		
24) Chloroform-d	4.346	84	286259	42.20	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.40%		
26) 1,2-Dichloroethane-d4	5.030	65	190810	42.63	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.26%		
32) Benzene-d6	5.050	84	553051	42.13	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.26%		
36) 1,2-Dichloropropane-d6	6.069	67	179860	42.83	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	85.66%		
41) Toluene-d8	7.316	98	473696	40.61	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.22%		
43) trans-1,3-Dichloroprop...	7.622	79	82583	42.08	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.16%		
47) 2-Hexanone-d5	8.088	63	140005	89.11	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.11%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	234503	44.68	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.36%		
64) 1,2-Dichlorobenzene-d4	11.631	152	185387	44.08	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.16%		
Target Compounds						Qvalue
13) Acetone	2.182	43	9718	4.75	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032321\
Data File : VV020713.D
Acq On : 23 Mar 2021 14:08
Operator : SY/MD
Sample : M1783-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G12

Quant Time: Mar 24 04:18:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 23 02:12:43 2021
Response via : Initial Calibration

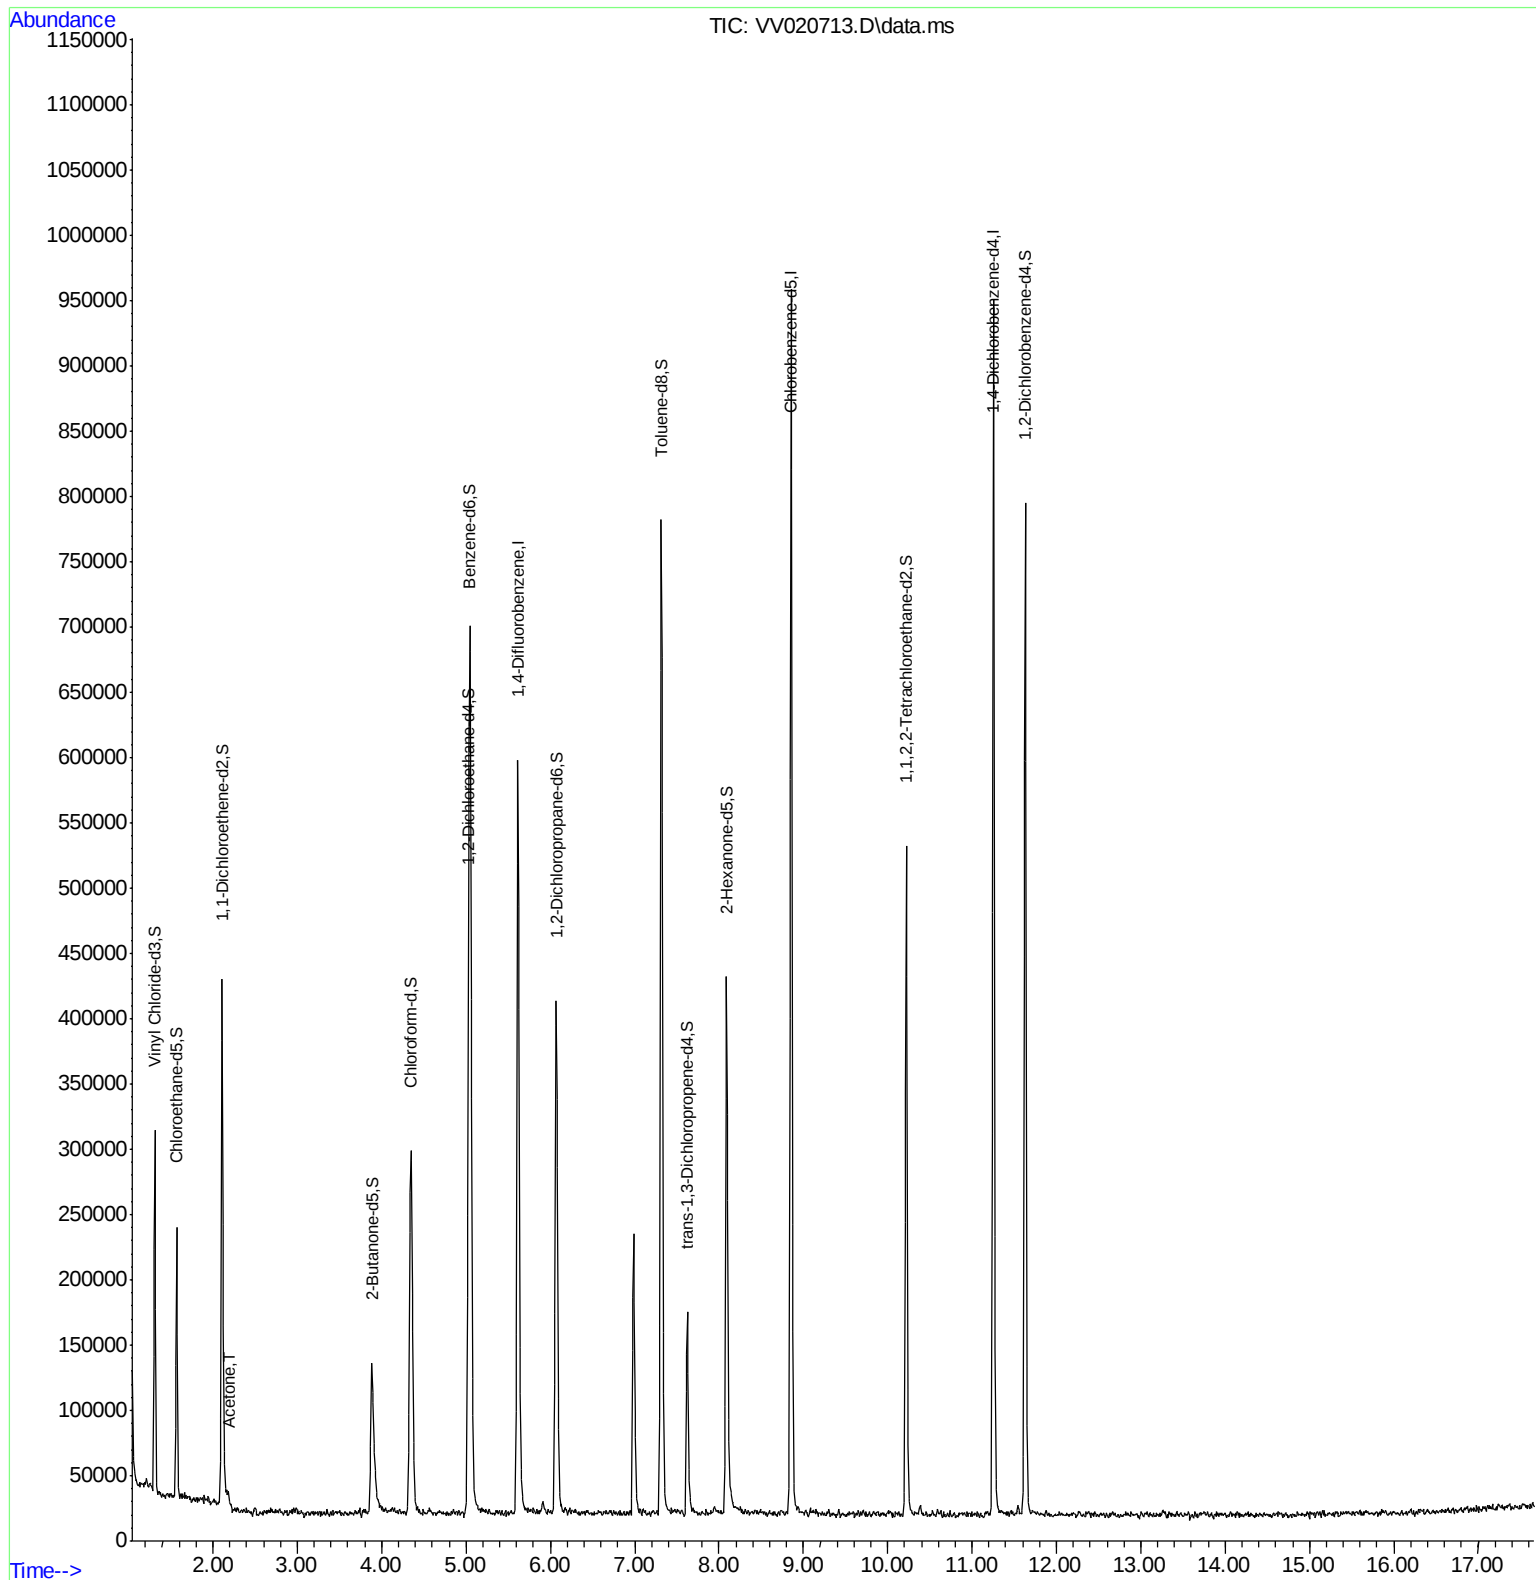

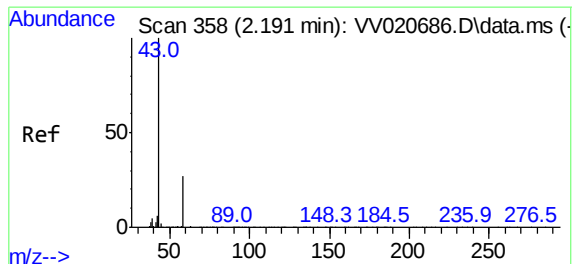

#13
 Acetone
 Concen: 4.75 ug/L
 RT: 2.182 min Scan# 355
 Delta R.T. -0.007 min
 Lab File: VV020713.D
 Acq: 23 Mar 2021 14:08

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G12

Tgt Ion: 43 Resp: 9718
 Ion Ratio Lower Upper
 43 100
 58 25.4 0.0 60.2

