


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032321\
 Data File : VV020714.D
 Acq On : 23 Mar 2021 15:57
 Operator : SY/MD
 Sample : BFB68
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB68

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 24 04:46:49 2021

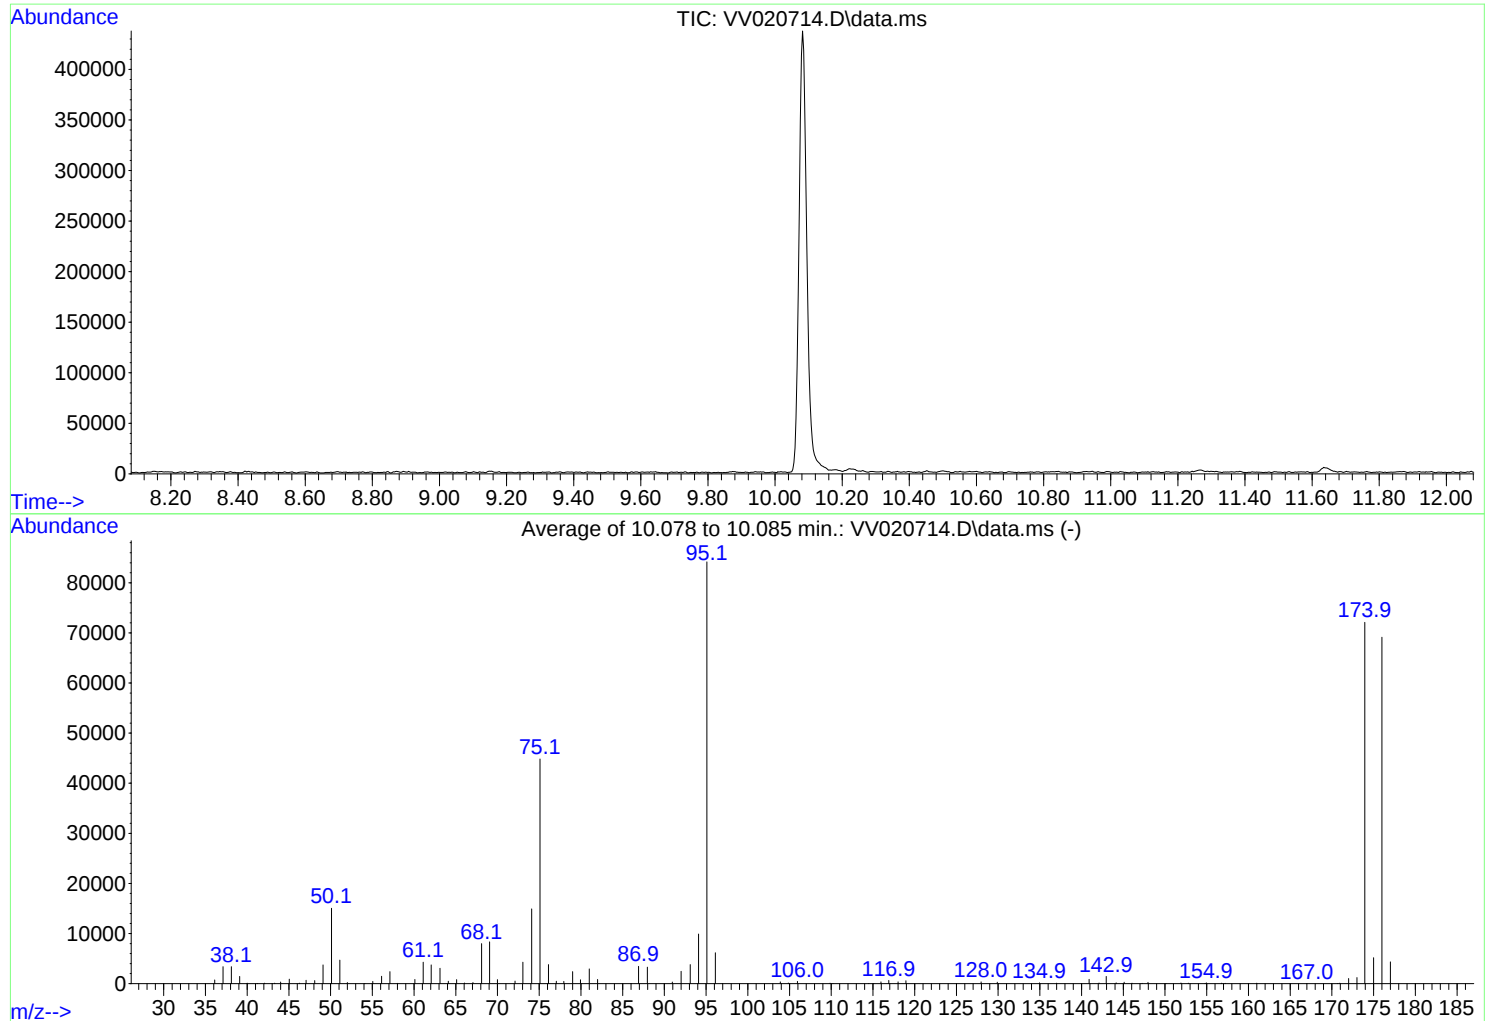

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	15031	PASS
75	95	30	80	53.3	44832	PASS
95	95	100	100	100.0	84184	PASS
96	95	5	9	7.3	6154	PASS
173	174	0.00	2	1.7	1223	PASS
174	95	50	120	85.7	72121	PASS
175	174	5	9	7.2	5191	PASS
176	174	95	101	95.9	69133	PASS
177	176	5	9	6.3	4334	PASS

m/z	Abundance
36.10	943.0
37.10	3308.0
38.10	3367.0
39.10	1430.0
40.00	501.0
43.00	139.0
43.30	140.0
44.00	907.0
45.10	914.0
46.20	181.0
47.00	628.0
48.10	580.0
49.10	3754.0
50.10	14883.0
51.10	4697.0
52.00	161.0
55.10	444.0
56.10	1433.0
57.10	2385.0
60.10	931.0
61.10	4497.0
62.00	3301.0
63.10	3220.0
64.10	501.0
65.10	865.0
66.00	104.0
67.00	254.0
68.10	7862.0
69.10	8333.0
70.00	706.0
72.10	624.0
73.10	4150.0
74.10	14930.0
75.10	43568.0
76.10	3658.0
77.10	514.0
78.00	368.0
79.00	2445.0
80.00	894.0
81.00	2818.0
82.00	924.0
86.90	3284.0
88.00	3157.0
91.00	321.0
92.00	2255.0
93.10	3815.0
94.10	9776.0
95.10	81928.0
96.10	5925.0
97.00	177.0
103.90	282.0
104.90	149.0
105.90	420.0
110.20	107.0
114.50	114.0
116.00	318.0
116.90	491.0
118.00	377.0
118.90	586.0
128.00	360.0
129.80	278.0
135.00	179.0
140.90	852.0
142.10	128.0
142.90	1442.0
144.20	101.0
145.00	252.0
146.10	117.0
147.20	128.0
148.00	325.0
150.10	126.0
151.90	115.0
152.80	143.0
154.90	273.0
156.80	169.0
161.00	130.0
170.70	133.0
170.90	124.0
172.00	950.0
173.00	1247.0
174.00	71952.0
175.00	5269.0
176.00	70448.0
177.00	4090.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
36.10	858.0
37.10	3493.0
38.10	3512.0
39.10	1486.0
40.00	462.0
42.10	119.0
43.30	143.0
44.00	957.0
45.10	929.0
46.30	140.0
47.00	685.0
48.10	631.0
49.10	3926.0
50.10	15357.0
51.10	4786.0
52.00	215.0
55.10	487.0
56.10	1549.0
57.10	2481.0
58.00	107.0
60.10	881.0
61.10	4440.0
62.10	3914.0
63.10	3150.0
64.10	465.0
65.10	821.0
66.10	140.0
67.00	217.0
68.10	8260.0
69.10	8854.0
70.00	862.0
72.10	544.0
73.10	4771.0
74.10	15441.0
75.10	46392.0
76.10	3889.0
77.10	459.0
77.90	469.0
79.00	2481.0
80.00	942.0
81.00	3007.0
82.00	870.0
86.90	3595.0
87.90	3336.0
90.90	315.0
92.00	2547.0
93.10	3984.0
94.10	10124.0
95.10	86776.0
96.10	6480.0
97.00	147.0
103.90	370.0
104.80	111.0
105.90	441.0
109.90	125.0
116.00	381.0
116.90	643.0
118.00	335.0
118.90	565.0
128.00	361.0
129.90	261.0
135.00	169.0
137.00	129.0
140.90	893.0
142.10	148.0
142.90	1497.0
144.20	170.0
145.10	295.0
146.00	118.0
147.30	110.0
147.90	254.0
151.90	161.0
152.80	129.0
155.00	244.0
156.80	121.0
157.20	113.0
161.00	129.0
171.00	133.0
172.00	1041.0
173.00	1364.0
174.00	74672.0
175.00	5469.0
176.00	71664.0
177.00	4439.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
36.10	700.0
37.10	3344.0
38.10	3296.0
39.10	1377.0
40.00	385.0
41.20	139.0
42.10	134.0
44.00	1037.0
45.00	839.0
47.10	749.0
48.10	577.0
49.10	3551.0
50.10	14853.0
51.10	4605.0
52.00	291.0
54.10	120.0
55.00	435.0
56.10	1430.0
57.10	2297.0
58.00	111.0
60.10	706.0
61.10	3891.0
62.10	4024.0
63.10	2818.0
64.10	447.0
65.10	727.0
66.10	136.0
67.10	227.0
68.10	7816.0
69.10	8218.0
70.00	810.0
72.10	400.0
73.10	4432.0
74.10	14402.0
75.10	44536.0
76.10	3872.0
77.00	437.0
77.90	498.0
79.00	2306.0
80.00	845.0
81.00	3009.0
82.00	722.0
86.00	111.0
86.90	3521.0
88.00	3346.0
91.00	290.0
92.00	2593.0
93.10	3634.0
94.10	9828.0
95.10	83848.0
96.10	6057.0
97.10	144.0
103.90	436.0
104.80	130.0
106.00	450.0
109.80	128.0
115.10	135.0
115.90	364.0
116.90	757.0
118.00	337.0
119.00	583.0
127.90	327.0
130.00	305.0
134.90	137.0
137.00	169.0
140.90	852.0
142.10	105.0
143.00	1376.0
144.10	175.0
145.20	326.0
146.00	104.0
147.90	189.0
151.90	110.0
154.80	183.0
157.20	119.0
167.00	110.0
172.00	1040.0
173.00	1058.0
174.00	70072.0
175.00	4835.0
176.00	65288.0
177.00	4473.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
36.20	106.0
40.00	340.0
44.00	651.0
68.90	134.0
73.00	161.0
79.80	120.0
92.80	117.0
96.90	120.0
173.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68