




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
 Data File : VV025140.D
 Acq On : 23 Mar 2022 18:40
 Operator : SY/MD
 Sample : N2083-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW609

Manual IntegrationsAPPROVED

Quant Time: Mar 24 01:18:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 24 01:12:55 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/24/2022
 Supervised By :Mahesh Dadoda 03/24/2022

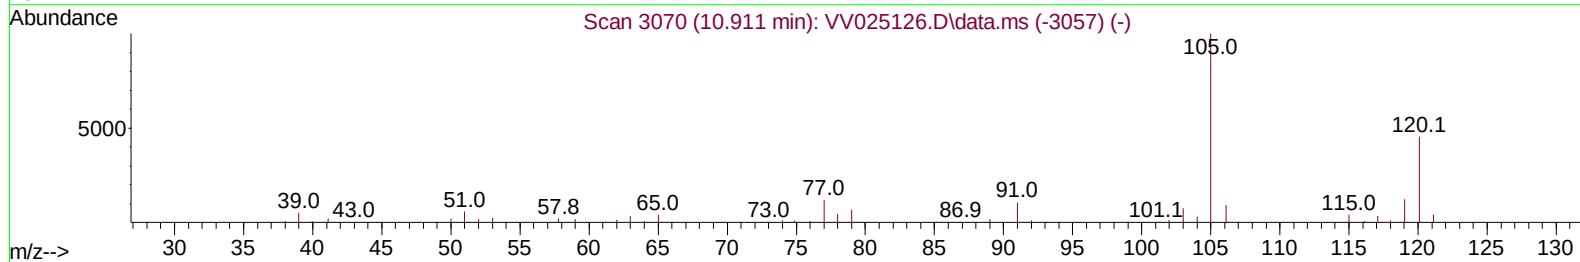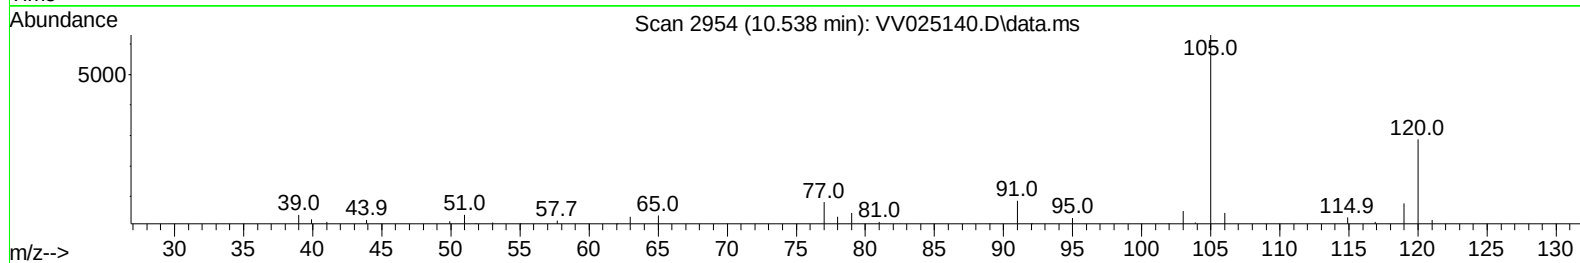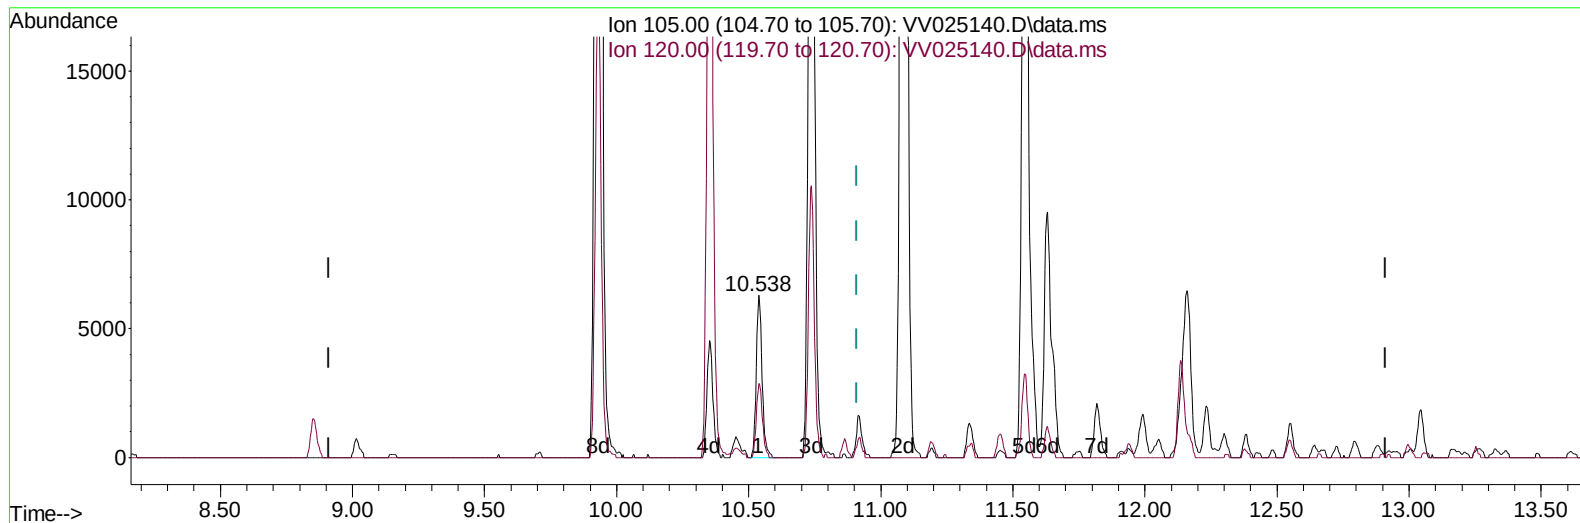

TIC: VV025140.D\data.ms

(63) 1,2,4-Trimethylbenzene (T)

10.538min (-0.373) 0.28 ug/L

response 9612

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	44.80	47.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025142.D
Acq On : 23 Mar 2022 19:27
Operator : SY/MD
Sample : N2083-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW609

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

Quant Time: Mar 24 01:19:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 24 01:12:55 2022
Response via : Initial Calibration

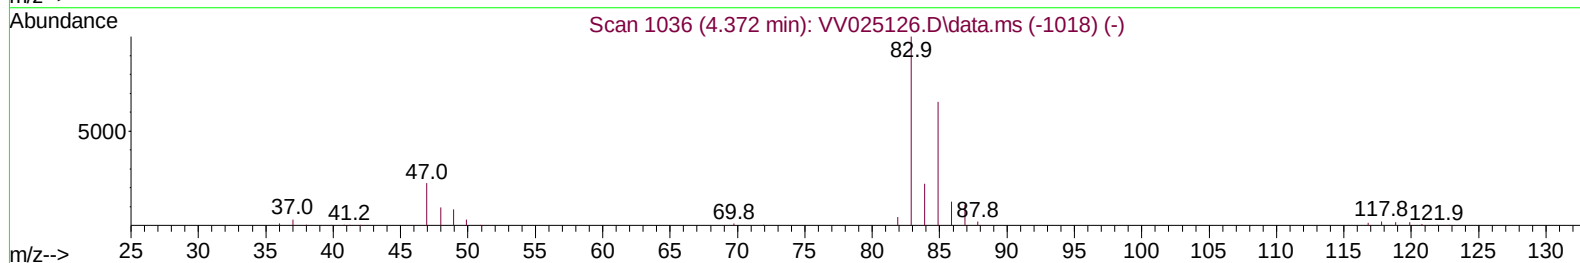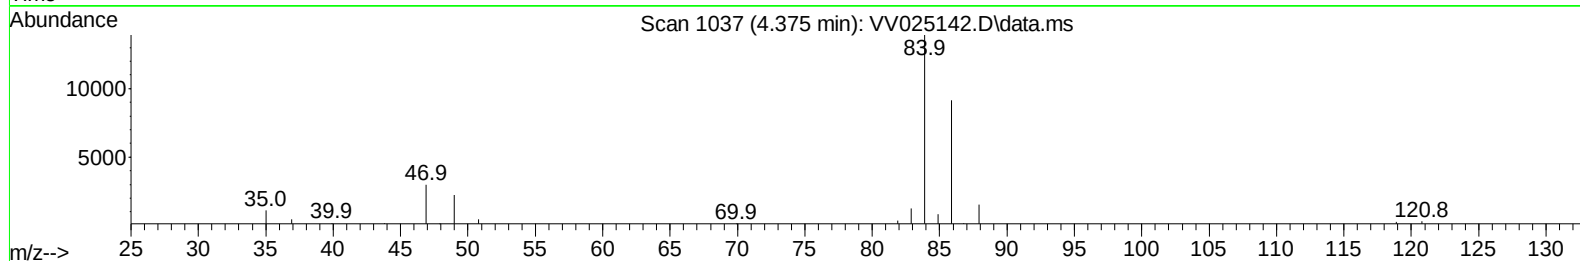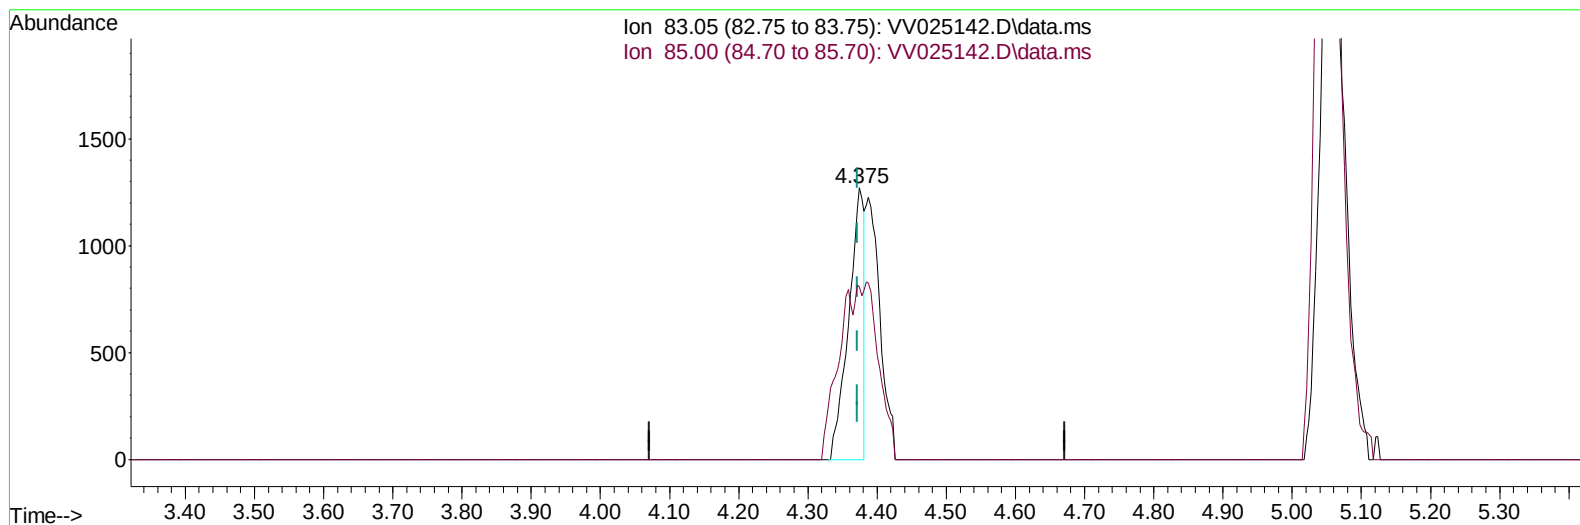

TIC: VV025142.D\data.ms

(25) Chloroform (T)

4.375min (+ 0.003) 0.11 ug/L

response 1953

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.60	63.62
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025142.D
Acq On : 23 Mar 2022 19:27
Operator : SY/MD
Sample : N2083-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW609

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

Quant Time: Mar 24 01:19:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 24 01:12:55 2022
Response via : Initial Calibration

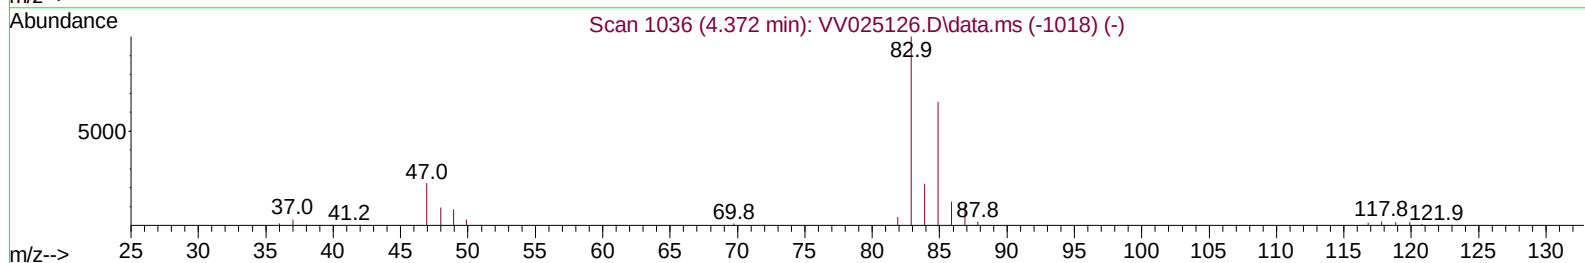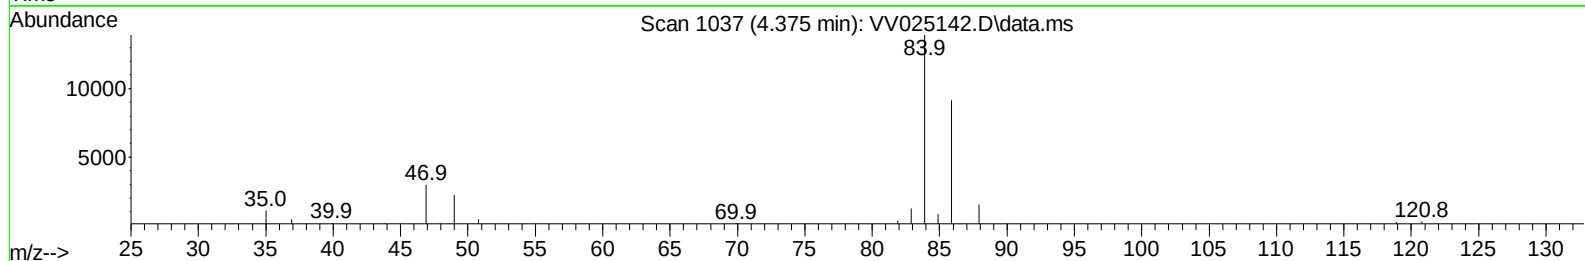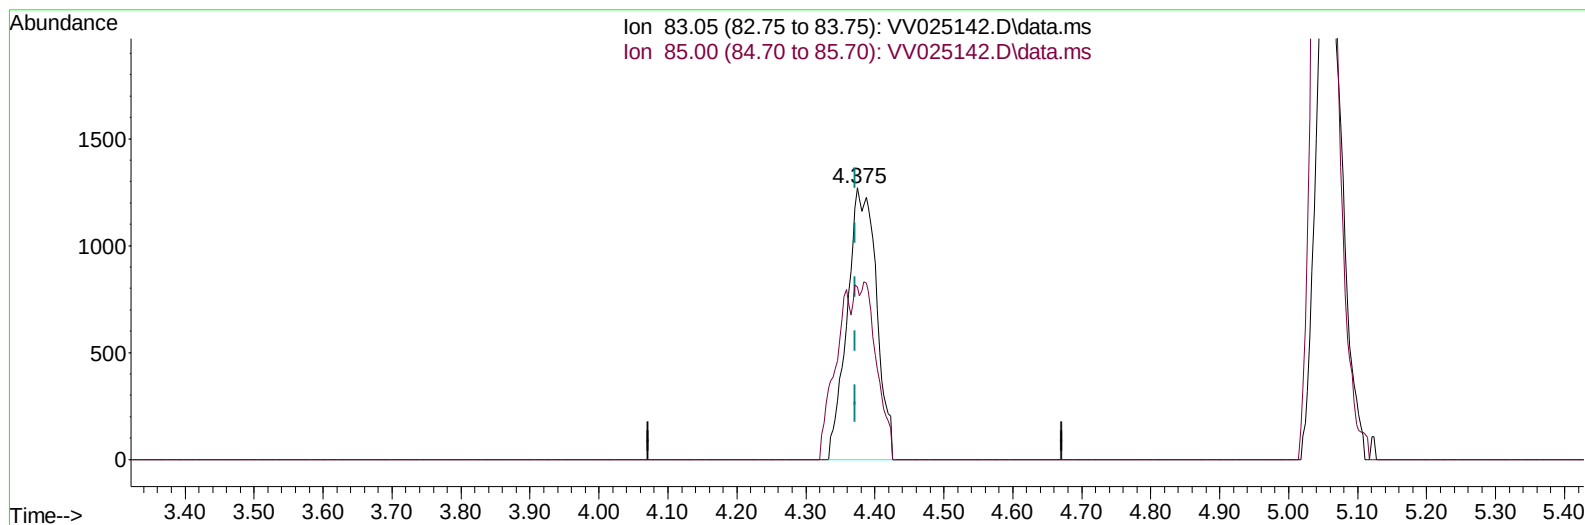

TIC: VV025142.D\data.ms

(25) Chloroform (T)

4.375min (+ 0.003) 0.22 ug/L m

response 3727

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.60	63.62
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
 Data File : VV025142.D
 Acq On : 23 Mar 2022 19:27
 Operator : SY/MD
 Sample : N2083-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW609

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/24/2022
 Supervised By :Mahesh Dadoda 03/24/2022

Quant Time: Mar 24 01:19:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 24 01:12:55 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		126932	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		121955	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		54681	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		41373	4.129	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.600%	
7) Chloroethane-d5	1.571	69		37051	5.049	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.000%	
11) 1,1-Dichloroethene-d2	2.111	63		55206	3.409	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.200%	
20) 2-Butanone-d5	3.896	46		91244	75.341	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	150.680%#	
24) Chloroform-d	4.352	84		88234	5.309	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.200%	
26) 1,2-Dichloroethane-d4	5.034	65		39007	5.614	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.200%	
32) Benzene-d6	5.050	84		172656	4.880	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%	
36) 1,2-Dichloropropane-d6	6.072	67		54229	5.331	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.600%	
41) Toluene-d8	7.317	98		146544	4.545	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.000%	
43) trans-1,3-Dichloroprop...	7.625	79		14830	4.182	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%	
46) 2-Hexanone-d5	8.088	63		76073	62.887	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	125.780%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		37000	6.182	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	123.600%#	
66) 1,2-Dichlorobenzene-d4	11.625	152		51268	5.538	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.800%	
Target Compounds							
25) Chloroform	4.375	83		3727m	0.216	ug/L	
29) 1,1,1-Trichloroethane	4.619	97		2334	0.150	ug/L	95
47) Tetrachloroethene	7.979	164		2390	0.322	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025142.D
Acq On : 23 Mar 2022 19:27
Operator : SY/MD
Sample : N2083-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW609

Manual IntegrationsAPPROVED

Quant Time: Mar 24 01:19:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 24 01:12:55 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

