

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
 Data File : VV025127.D
 Acq On : 23 Mar 2022 13:02
 Operator : SY/MD
 Sample : VV0323WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK322

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	77450	76324	15.46%	2.034%
2	1.568	156	164	176	rBV	64073	71995	14.59%	1.918%
3	2.108	321	332	350	rVB	119893	172958	35.04%	4.608%
4	2.507	447	456	468	rVB	7536	11762	2.38%	0.313%
5	3.896	878	888	916	rBV2	30069	101643	20.59%	2.708%
6	4.346	1012	1028	1059	rVB	85049	214218	43.40%	5.708%
7	5.044	1230	1245	1291	rBV2	200834	493581	100.00%	13.151%
8	5.613	1411	1422	1450	rBV	146816	298894	60.56%	7.964%
9	5.912	1504	1515	1529	rVB6	3784	8425	1.71%	0.224%
10	6.066	1551	1563	1589	rBV	111671	229447	46.49%	6.113%
11	6.986	1839	1849	1870	rBV2	48267	90533	18.34%	2.412%
12	7.314	1939	1951	1972	rBV	236216	413067	83.69%	11.006%
13	7.394	1973	1976	1994	rVB3	3057	5354	1.08%	0.143%
14	7.622	2037	2047	2067	rBV	25890	47030	9.53%	1.253%
15	8.088	2181	2192	2227	rBV	165263	363976	73.74%	9.698%
16	8.850	2417	2429	2455	rBV	216850	361222	73.18%	9.624%
17	10.214	2843	2853	2877	rVB	72419	116135	23.53%	3.094%
18	11.246	3164	3174	3197	rBV	210769	335155	67.90%	8.930%
19	11.622	3280	3291	3311	rBV	210635	335302	67.93%	8.934%
20	12.246	3475	3485	3498	rVB2	3865	6233	1.26%	0.166%




Sum of corrected areas: 3753254

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025127.D
Acq On : 23 Mar 2022 13:02
Operator : SY/MD
Sample : VV0323WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

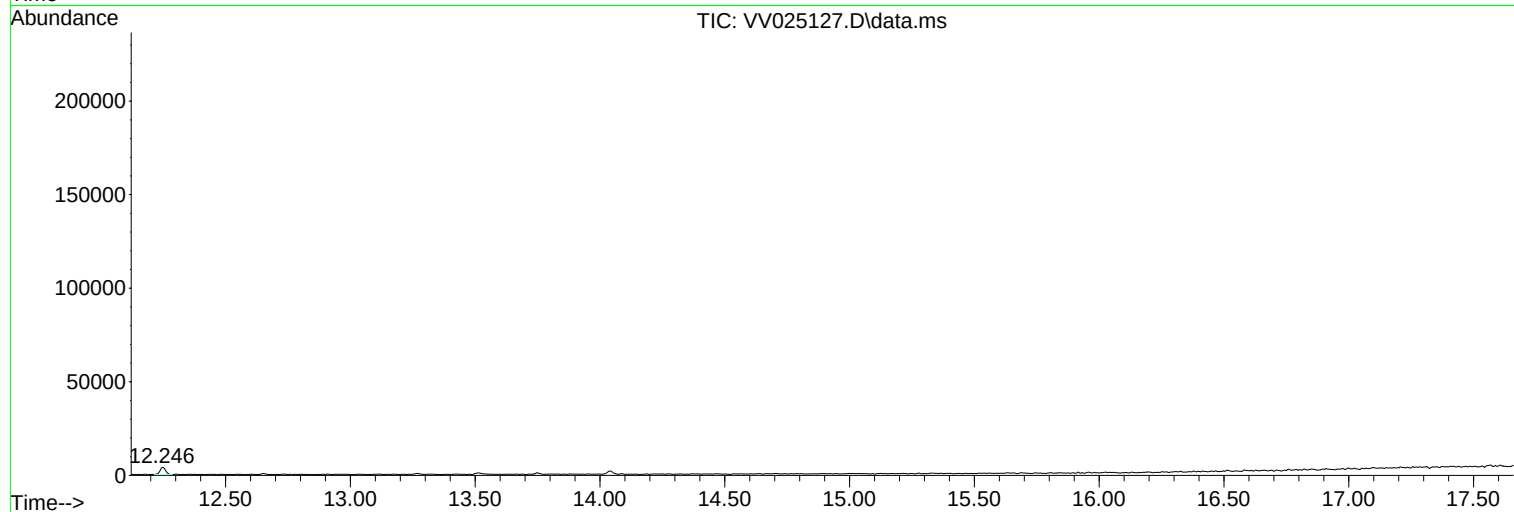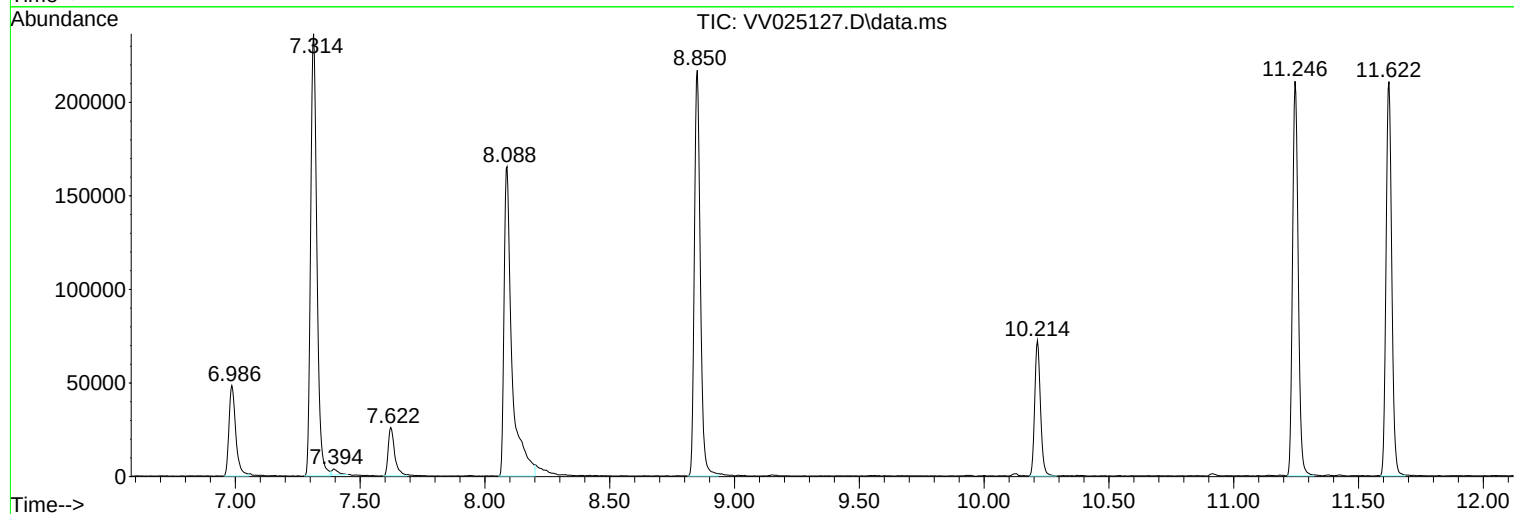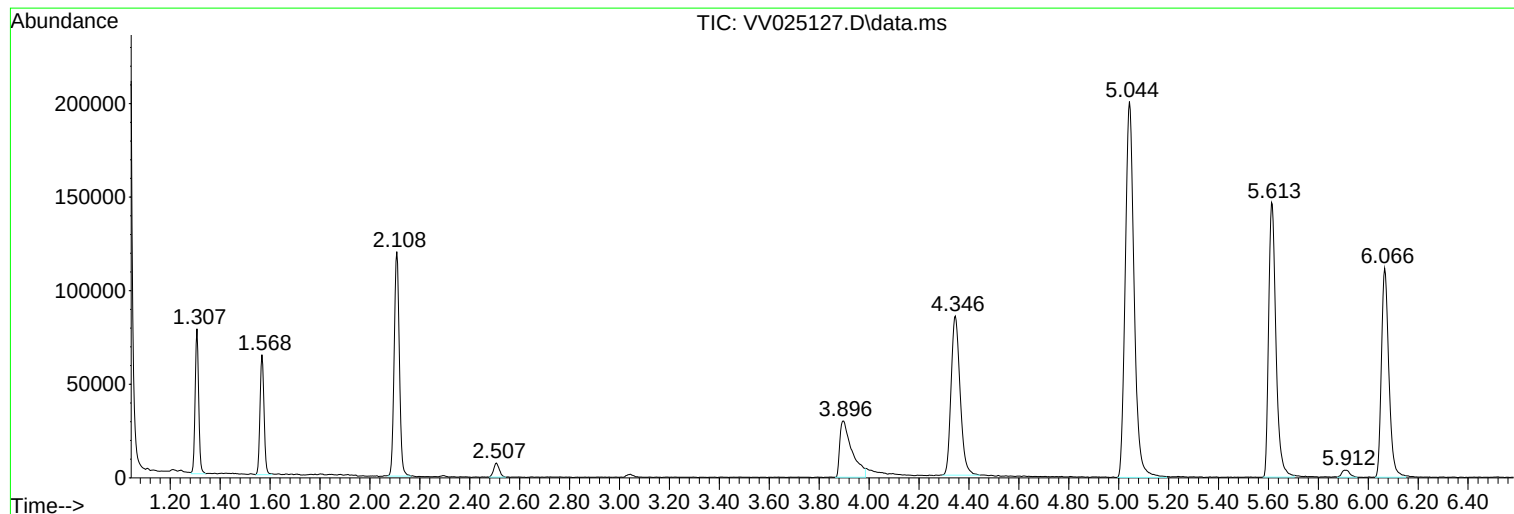

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025127.D
Acq On : 23 Mar 2022 13:02
Operator : SY/MD
Sample : VV0323WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025127.D
Acq On : 23 Mar 2022 13:02
Operator : SY/MD
Sample : VV0323WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------