

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
 Data File : VV025134.D
 Acq On : 23 Mar 2022 15:56
 Operator : SY/MD
 Sample : N2083-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW5Y9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	100	rVB	65290	66056	15.87%	1.643%
2	1.568	156	164	176	rBV	55276	61445	14.76%	1.528%
3	2.111	322	333	350	rBV2	121722	198269	47.64%	4.930%
4	3.191	656	669	686	rBV	30764	63706	15.31%	1.584%
5	3.905	878	891	923	rBV4	52163	182714	43.90%	4.543%
6	4.349	1011	1029	1057	rBV2	73405	187961	45.16%	4.674%
7	4.609	1092	1110	1144	rBV2	125516	321518	77.25%	7.995%
8	4.828	1164	1178	1200	rBV3	12513	30645	7.36%	0.762%
9	5.047	1228	1246	1277	rBV2	167245	416208	100.00%	10.350%
10	5.619	1412	1424	1454	rBV	132530	273028	65.60%	6.789%
11	5.918	1506	1517	1541	rVB5	27046	58352	14.02%	1.451%
12	6.069	1552	1564	1593	rBV	95223	196559	47.23%	4.888%
13	6.989	1837	1850	1873	rBV	41141	76915	18.48%	1.913%
14	7.317	1941	1952	1971	rBV	195423	349291	83.92%	8.686%
15	7.397	1971	1977	1996	rVB	6760	12841	3.09%	0.319%
16	7.625	2038	2048	2065	rBV	22767	40273	9.68%	1.001%
17	7.940	2135	2146	2148	rBV2	5518	7562	1.82%	0.188%
18	7.976	2148	2157	2175	rVB3	50109	87395	21.00%	2.173%
19	8.088	2182	2192	2235	rBV	170839	332720	79.94%	8.274%
20	8.850	2419	2429	2449	rBV	199644	328675	78.97%	8.173%
21	10.217	2838	2854	2876	rBV	65518	102202	24.56%	2.541%
22	10.381	2890	2905	2915	rBV3	11415	18388	4.42%	0.457%
23	11.249	3164	3175	3195	rBV	200795	305880	73.49%	7.606%
24	11.622	3279	3291	3316	rBV	184061	287470	69.07%	7.148%
25	12.249	3472	3486	3497	rVB	4920	7412	1.78%	0.184%
26	14.036	4033	4042	4052	rBV	5019	8027	1.93%	0.200%




Sum of corrected areas: 4021512

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025134.D
Acq On : 23 Mar 2022 15:56
Operator : SY/MD
Sample : N2083-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5Y9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

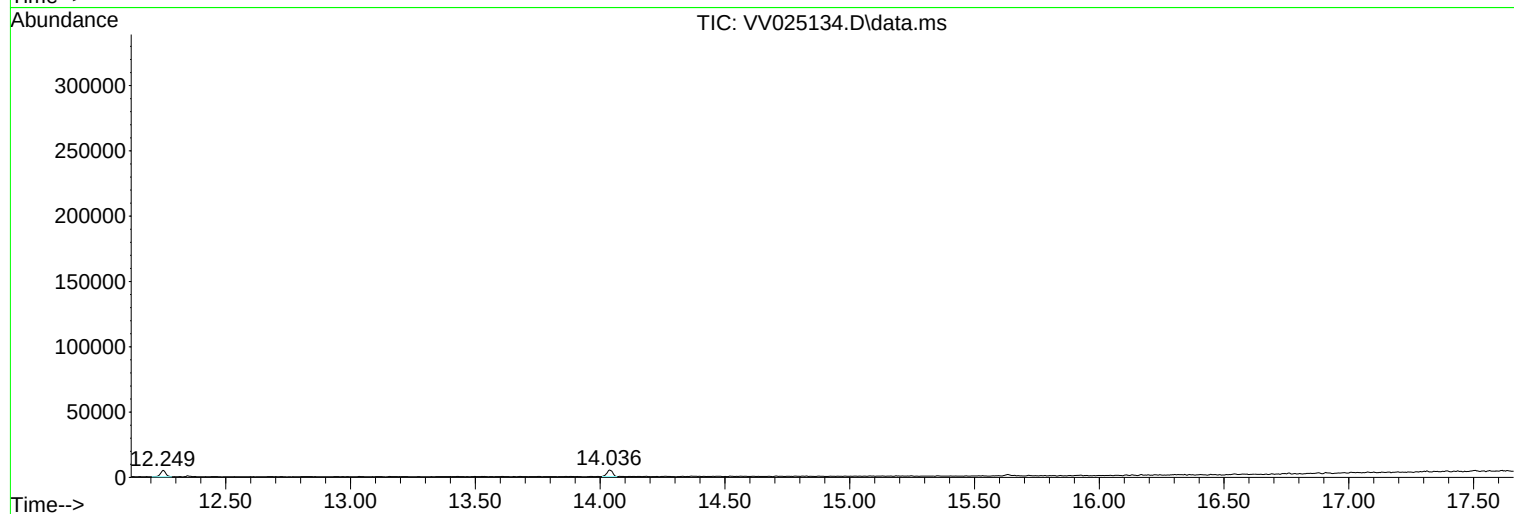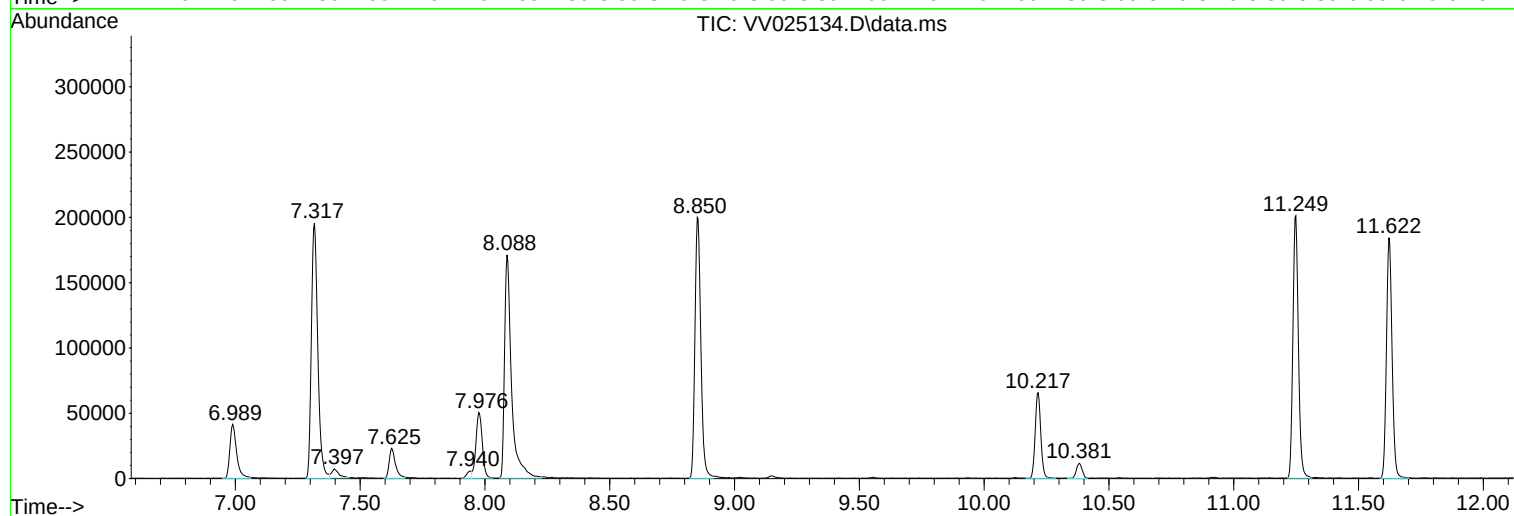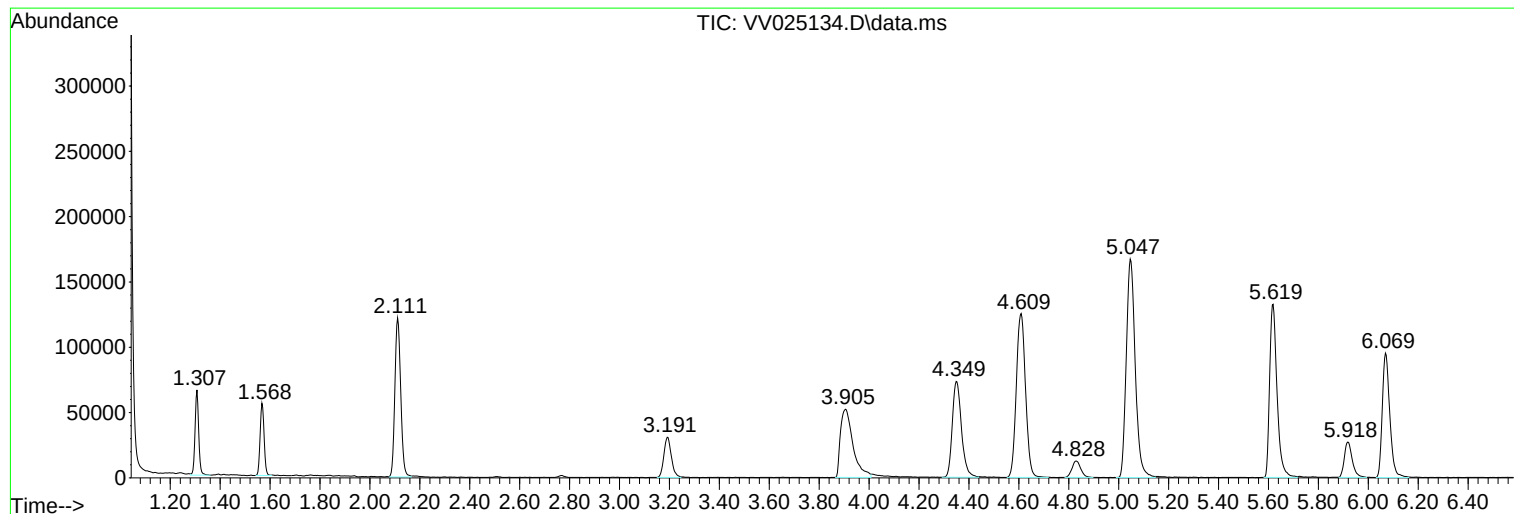

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025134.D
Acq On : 23 Mar 2022 15:56
Operator : SY/MD
Sample : N2083-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5Y9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025134.D
Acq On : 23 Mar 2022 15:56
Operator : SY/MD
Sample : N2083-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5Y9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc