

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
 Data File : VV025138.D
 Acq On : 23 Mar 2022 17:30
 Operator : SY/MD
 Sample : N2083-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW5Z8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	94	rBV	67543	69854	16.29%	1.794%
2	1.571	155	165	176	rBV	55050	64569	15.06%	1.659%
3	2.111	323	333	350	rVB	106900	159703	37.24%	4.102%
4	2.770	525	538	554	rVB3	7969	15019	3.50%	0.386%
5	3.195	658	670	689	rBV	23502	49547	11.55%	1.273%
6	3.912	879	893	928	rBV2	102133	319025	74.39%	8.195%
7	4.352	1014	1030	1065	rBV	78967	206411	48.13%	5.302%
8	4.613	1096	1111	1130	rBV4	21608	54199	12.64%	1.392%
9	4.834	1165	1180	1196	rVB3	9955	24159	5.63%	0.621%
10	5.050	1230	1247	1269	rBV2	171569	428836	100.00%	11.016%
11	5.619	1412	1424	1456	rBV	132392	274587	64.03%	7.054%
12	5.921	1508	1518	1540	rVB4	15848	35212	8.21%	0.905%
13	6.069	1552	1564	1591	rBV	98417	202179	47.15%	5.194%
14	6.989	1838	1850	1872	rBV	42632	80118	18.68%	2.058%
15	7.317	1940	1952	1972	rBV	200331	355127	82.81%	9.123%
16	7.400	1972	1978	1997	rVB2	4392	8854	2.06%	0.227%
17	7.625	2035	2048	2069	rBV	22944	41665	9.72%	1.070%
18	7.937	2135	2145	2150	rBV2	7551	11868	2.77%	0.305%
19	7.979	2150	2158	2173	rVB3	16804	29983	6.99%	0.770%
20	8.088	2182	2192	2230	rBV	186382	359650	83.87%	9.239%
21	8.850	2419	2429	2455	rBV	201607	333169	77.69%	8.558%
22	10.214	2840	2853	2867	rBV	70223	111789	26.07%	2.872%
23	10.381	2895	2905	2916	rBV2	14315	22694	5.29%	0.583%
24	11.249	3164	3175	3196	rBV	201280	309815	72.25%	7.959%
25	11.622	3281	3291	3314	rBV	192497	301712	70.36%	7.750%
26	12.249	3476	3486	3500	rBV2	6507	10114	2.36%	0.260%
27	14.040	4031	4043	4055	rBV	7951	13005	3.03%	0.334%




Sum of corrected areas: 3892863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025138.D
Acq On : 23 Mar 2022 17:30
Operator : SY/MD
Sample : N2083-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5Z8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

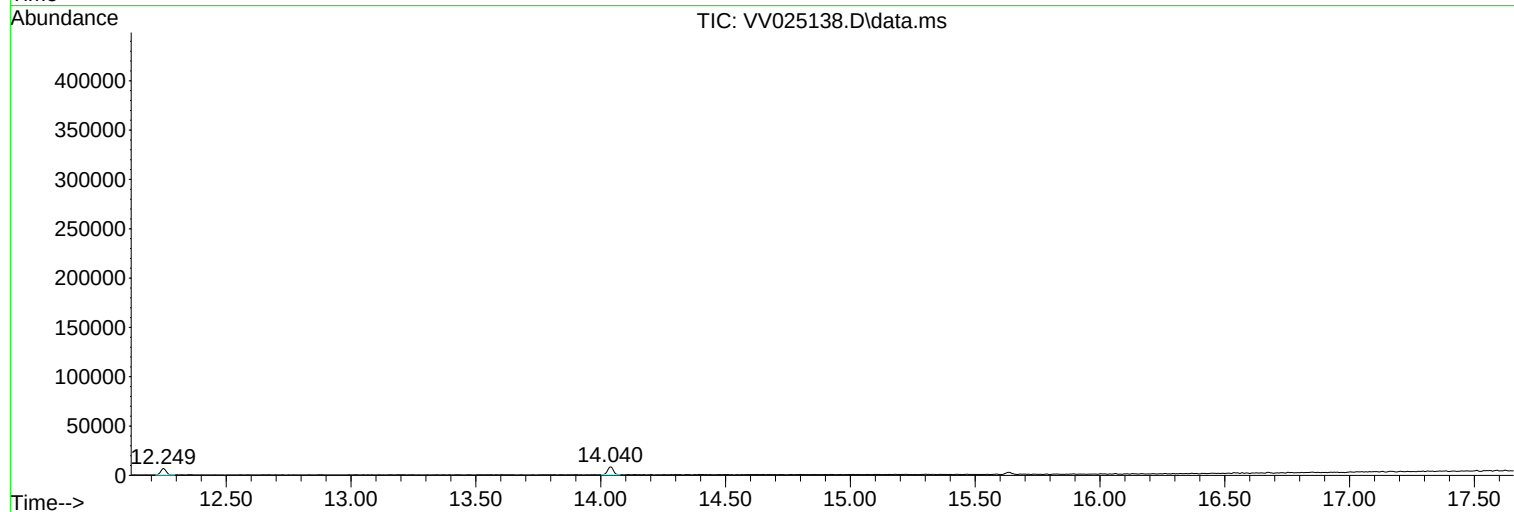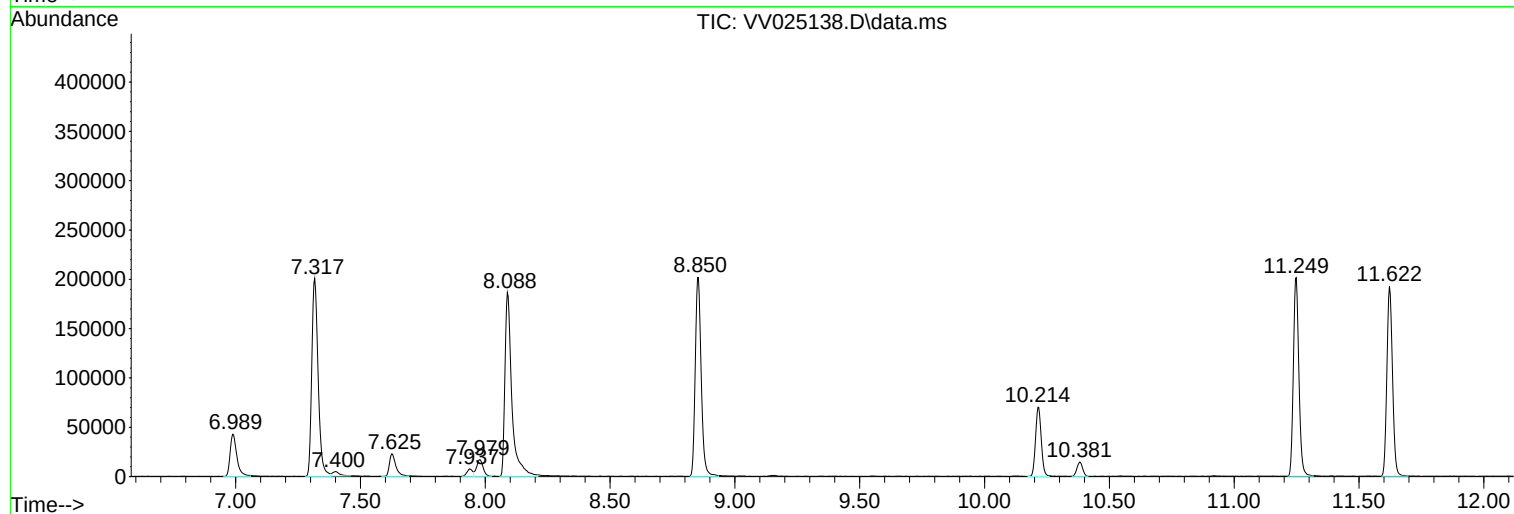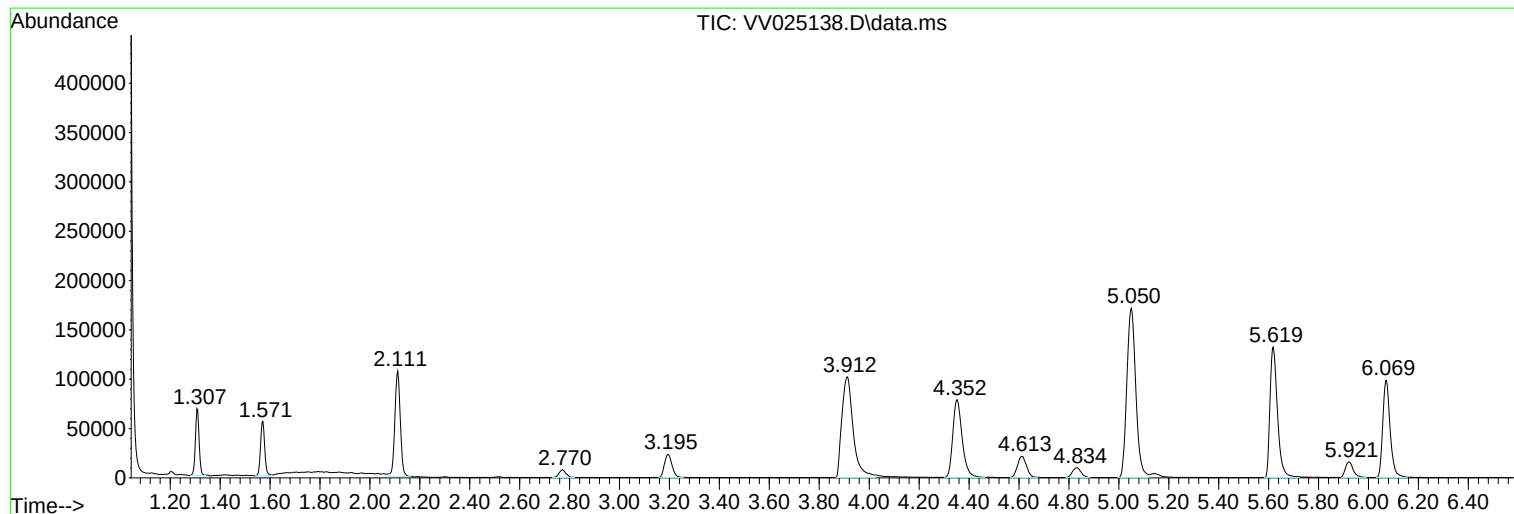

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025138.D
Acq On : 23 Mar 2022 17:30
Operator : SY/MD
Sample : N2083-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5Z8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025138.D
Acq On : 23 Mar 2022 17:30
Operator : SY/MD
Sample : N2083-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5Z8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc