

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
 Data File : VV025143.D
 Acq On : 23 Mar 2022 19:50
 Operator : SY/MD
 Sample : N2083-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW610

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	57815	58519	14.07%	1.578%
2	1.568	157	164	180	rVB	51100	58149	13.98%	1.568%
3	2.111	323	333	346	rVB2	97282	142467	34.24%	3.842%
4	2.773	528	539	555	rVB5	5963	12363	2.97%	0.333%
5	3.195	660	670	687	rVB3	3959	8021	1.93%	0.216%
6	3.902	879	890	923	rBV2	50231	173290	41.65%	4.674%
7	4.352	1015	1030	1062	rBV2	77839	211841	50.92%	5.713%
8	4.612	1095	1111	1129	rBV3	27063	65296	15.69%	1.761%
9	5.050	1231	1247	1281	rBV2	166336	416058	100.00%	11.221%
10	5.619	1412	1424	1446	rBV	135947	271505	65.26%	7.322%
11	5.921	1506	1518	1538	rBV3	27877	58217	13.99%	1.570%
12	6.069	1553	1564	1591	rBV2	95214	197588	47.49%	5.329%
13	6.989	1840	1850	1872	rBV2	38583	71865	17.27%	1.938%
14	7.317	1941	1952	1971	rBV	192213	338293	81.31%	9.124%
15	7.397	1974	1977	1994	rVB3	3307	5960	1.43%	0.161%
16	7.625	2040	2048	2067	rBV2	19986	36934	8.88%	0.996%
17	7.940	2134	2146	2147	rBV2	8326	10081	2.42%	0.272%
18	7.976	2148	2157	2176	rVB	73771	128292	30.84%	3.460%
19	8.088	2183	2192	2230	rBV	184504	352252	84.66%	9.500%
20	8.853	2419	2430	2460	rBV	205475	336119	80.79%	9.065%
21	10.214	2842	2853	2873	rVB	70367	109662	26.36%	2.958%
22	10.381	2895	2905	2917	rVB	17823	27648	6.65%	0.746%
23	11.249	3163	3175	3197	rBV	200542	311677	74.91%	8.406%
24	11.622	3279	3291	3313	rBV	182858	288535	69.35%	7.782%
25	12.249	3476	3486	3499	rVB	7469	12335	2.96%	0.333%
26	14.037	4033	4042	4052	rBV	3070	4879	1.17%	0.132%




Sum of corrected areas: 3707846

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025143.D
Acq On : 23 Mar 2022 19:50
Operator : SY/MD
Sample : N2083-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

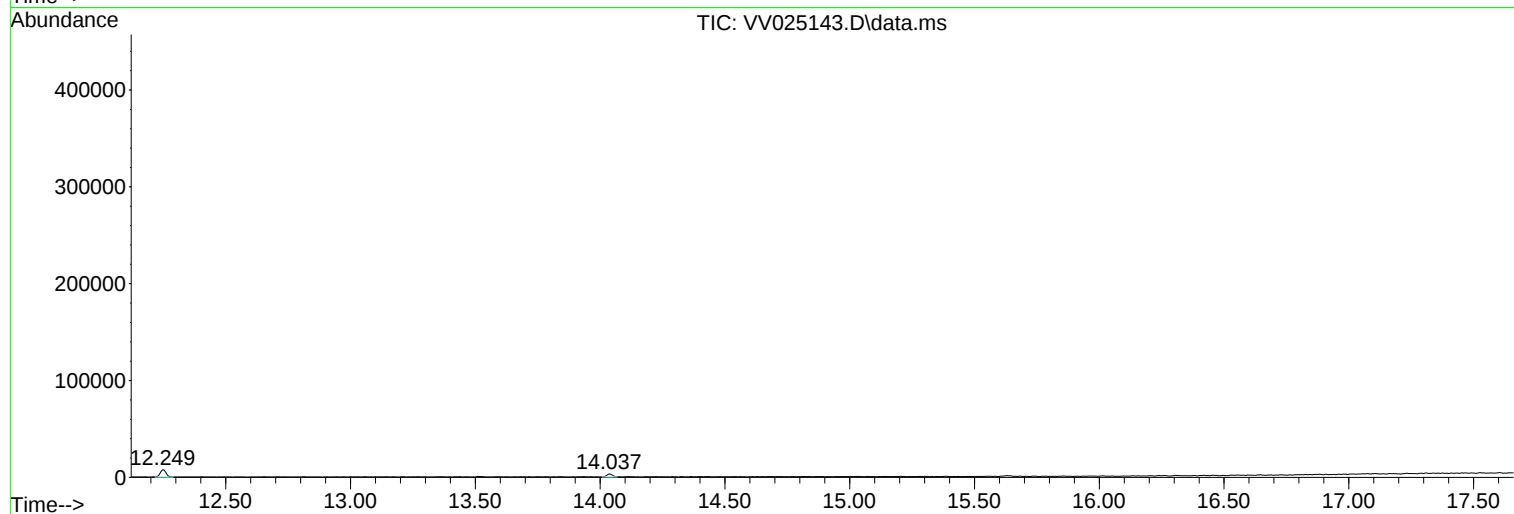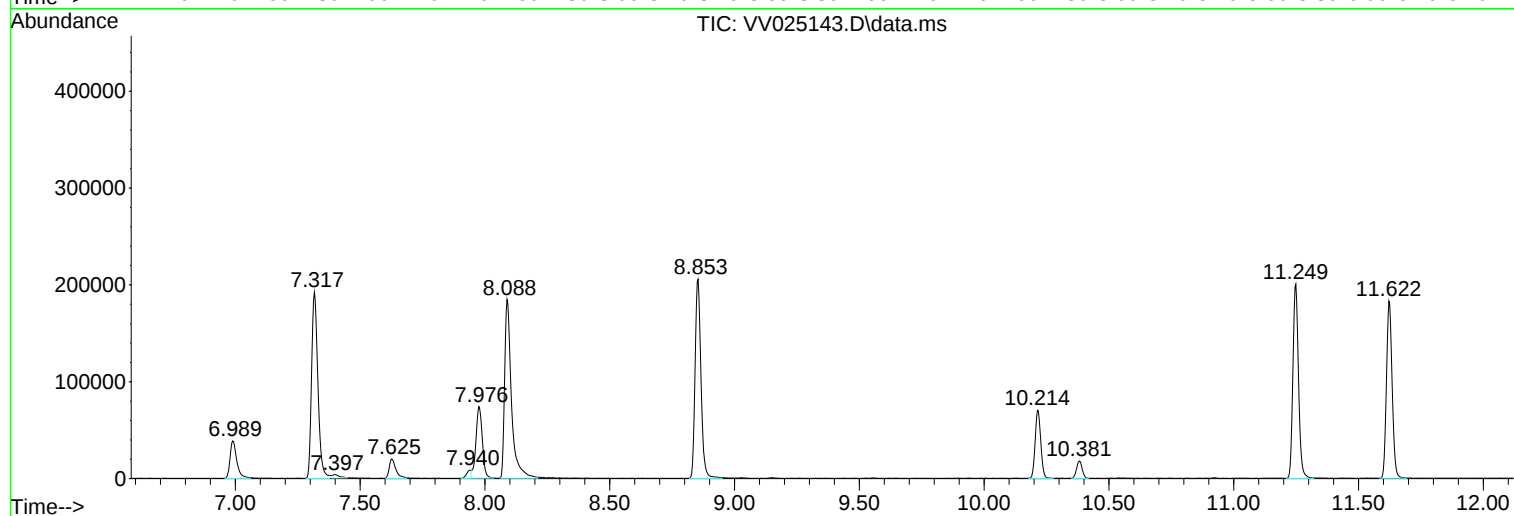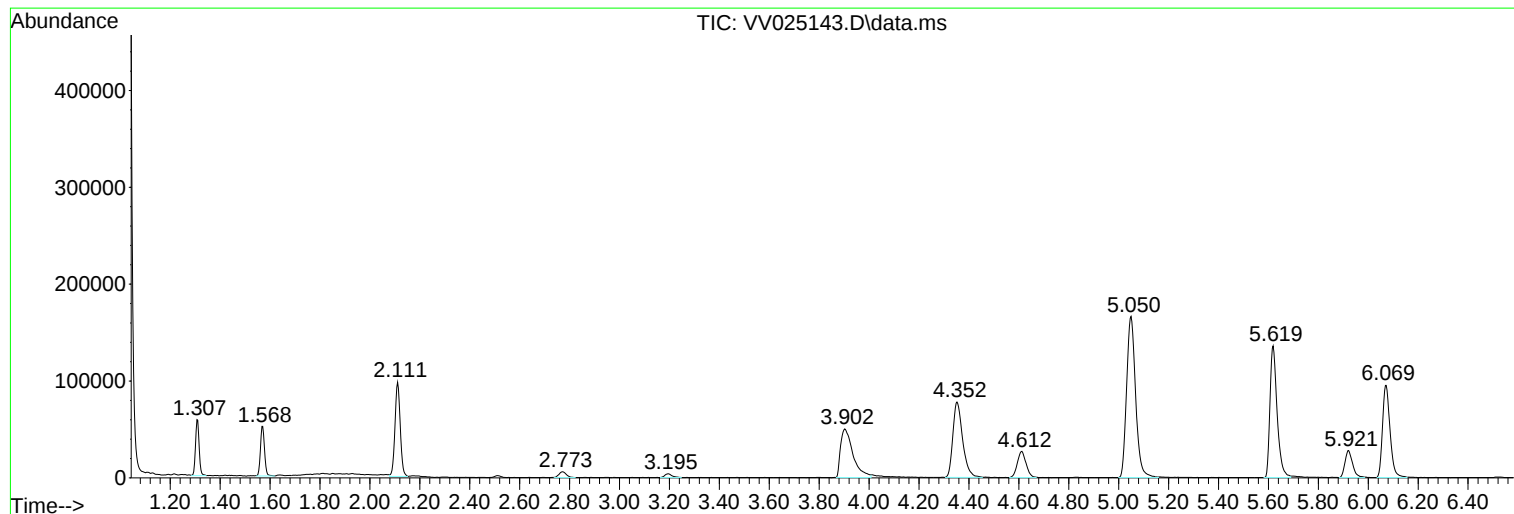

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025143.D
Acq On : 23 Mar 2022 19:50
Operator : SY/MD
Sample : N2083-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
Data File : VV025143.D
Acq On : 23 Mar 2022 19:50
Operator : SY/MD
Sample : N2083-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------