


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032322\
 Data File : VV025125.D
 Acq On : 23 Mar 2022 09:31
 Operator : SY/MD
 Sample : BFB285
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB285

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Mar 24 01:12:55 2022

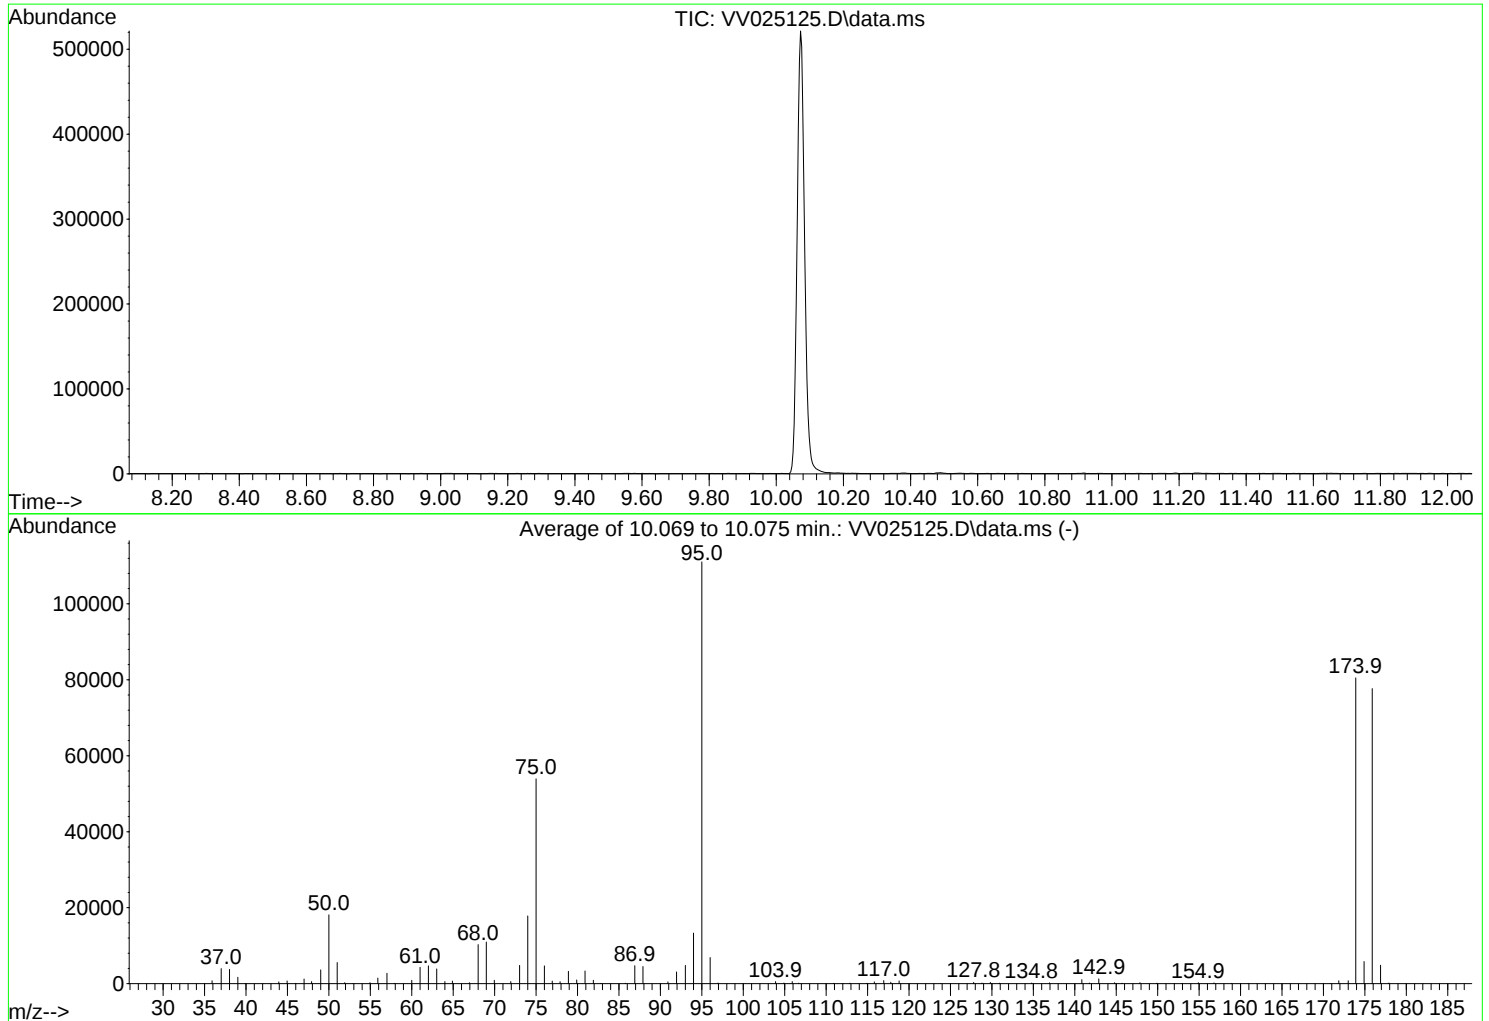

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	18104	PASS
75	95	30	80	48.6	53939	PASS
95	95	100	100	100.0	111059	PASS
96	95	5	9	6.2	6862	PASS
173	174	0.00	2	0.9	742	PASS
174	95	50	120	72.5	80509	PASS
175	174	5	9	7.2	5817	PASS
176	174	95	105	96.5	77683	PASS
177	176	5	10	6.3	4865	PASS

m/z	Abundance
39.90	148.0
44.00	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
35.90	791.0
37.00	3957.0
38.00	3651.0
39.00	1687.0
39.90	188.0
43.90	691.0
45.00	660.0
46.00	137.0
47.00	1087.0
47.90	608.0
49.00	3661.0
50.00	18008.0
51.00	5428.0
51.90	247.0
54.90	233.0
55.90	1384.0
57.00	2636.0
57.90	120.0
60.00	828.0
61.00	4256.0
62.00	4503.0
63.00	3843.0
64.00	506.0
64.90	663.0
67.00	281.0
68.00	10202.0
69.00	10918.0
70.00	878.0
71.90	593.0
73.00	4647.0
74.00	17496.0
75.00	52616.0
76.00	4692.0
76.90	723.0
77.90	518.0
78.90	3109.0
79.90	926.0
80.90	3288.0
81.90	803.0
85.70	155.0
86.90	4563.0
87.90	4092.0
90.90	432.0
91.90	3114.0
93.00	4854.0
94.00	12957.0
95.00	108144.0
96.00	6823.0
96.90	172.0
103.90	568.0
104.90	207.0
105.90	539.0
106.70	106.0
112.90	116.0
114.90	110.0
115.80	432.0
117.00	734.0
117.80	358.0
118.80	675.0
127.80	335.0
128.80	150.0
129.80	347.0
130.90	118.0
134.80	179.0
136.90	169.0
140.80	1005.0
141.80	154.0
142.90	1290.0
144.90	233.0
145.70	104.0
147.90	285.0
149.90	128.0
152.00	114.0
153.00	110.0
154.90	227.0
156.80	203.0
171.90	800.0
173.00	683.0
173.90	75488.0
174.90	5595.0
175.90	73024.0
176.90	4481.0
177.90	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
35.90	821.0
37.00	4090.0
38.00	3929.0
39.00	1722.0
39.90	211.0
43.90	674.0
45.00	735.0
46.00	125.0
47.00	1259.0
47.90	590.0
49.00	3703.0
50.00	18744.0
51.00	5736.0
51.90	259.0
52.90	107.0
54.90	240.0
55.90	1529.0
57.00	2867.0
57.90	109.0
60.00	898.0
61.00	4353.0
62.00	4794.0
63.00	4058.0
64.00	584.0
64.90	692.0
66.90	268.0
68.00	10606.0
69.00	11352.0
70.00	936.0
71.90	546.0
73.00	4998.0
74.00	18504.0
75.00	55776.0
76.00	4831.0
77.00	667.0
77.90	516.0
78.90	3393.0
79.90	979.0
80.90	3434.0
81.90	898.0
82.80	113.0
85.80	134.0
86.90	4825.0
87.90	4603.0
90.90	471.0
92.00	3199.0
93.00	4960.0
94.00	13801.0
95.00	115056.0
96.00	7027.0
96.90	153.0
103.90	601.0
104.90	170.0
105.90	565.0
106.70	140.0
110.90	113.0
112.00	101.0
112.90	120.0
114.90	105.0
115.80	473.0
116.90	812.0
117.80	390.0
118.80	740.0
127.80	367.0
128.80	169.0
129.80	337.0
130.90	144.0
134.80	196.0
137.00	208.0
140.90	1085.0
141.80	164.0
142.90	1305.0
144.80	259.0
145.70	123.0
147.90	277.0
149.90	147.0
152.90	108.0
154.90	249.0
156.80	225.0
159.00	107.0
160.90	114.0
171.90	779.0
173.00	767.0
173.90	83408.0
174.90	6030.0
175.90	80480.0
176.90	5067.0
177.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
35.90	722.0
37.00	3796.0
38.00	3697.0
39.00	1607.0
39.90	245.0
44.00	669.0
44.90	750.0
47.00	1265.0
47.90	487.0
49.00	3529.0
50.00	17560.0
51.00	5513.0
51.90	246.0
55.00	236.0
55.90	1552.0
57.00	2752.0
60.00	908.0
61.00	4260.0
62.00	4689.0
63.00	3787.0
64.00	552.0
64.90	613.0
66.90	262.0
68.00	10039.0
69.00	10653.0
69.90	907.0
72.00	472.0
73.00	4734.0
74.00	17496.0
75.00	53424.0
76.00	4484.0
76.90	614.0
77.90	470.0
78.90	3269.0
79.90	997.0
80.90	3310.0
81.90	924.0
82.80	116.0
85.80	129.0
86.90	4723.0
87.90	4797.0
90.90	454.0
92.00	2947.0
93.00	4558.0
94.00	13167.0
95.00	109976.0
96.00	6735.0
97.00	171.0
103.90	512.0
104.90	133.0
105.90	527.0
106.70	128.0
110.90	114.0
112.80	114.0
115.80	428.0
116.90	809.0
117.80	342.0
118.80	712.0
123.80	106.0
127.80	371.0
128.80	199.0
129.80	341.0
130.90	150.0
134.80	176.0
136.90	215.0
140.90	1129.0
141.70	149.0
142.90	1192.0
144.70	223.0
145.70	108.0
147.80	241.0
149.90	126.0
154.90	242.0
156.80	227.0
158.80	110.0
160.90	117.0
170.90	110.0
171.80	745.0
173.00	777.0
173.90	82632.0
174.90	5825.0
175.90	79544.0
176.90	5048.0
177.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285