

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
 Data File : VV030308.D
 Acq On : 23 Mar 2023 14:07
 Operator : SY/MD
 Sample : 02041-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB958

Quant Time: Mar 24 02:51:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 24 02:42:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	147412	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	145354	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	70099	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	42474	4.350	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.000%
7) Chloroethane-d5	1.539	69	42755	4.513	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	2.066	63	70454	3.041	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.800%
20) 2-Butanone-d5	3.812	46	118856	47.100	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.200%
24) Chloroform-d	4.262	84	104281	4.413	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.200%
26) 1,2-Dichloroethane-d4	4.953	65	52033	4.667	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.400%
32) Benzene-d6	4.973	84	194439	4.747	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
36) 1,2-Dichloropropane-d6	5.998	67	62060	4.840	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.800%
41) Toluene-d8	7.252	98	158365	4.210	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	7.564	79	19783	4.097	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.000%
46) 2-Hexanone-d5	8.034	63	89209	45.982	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.960%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	44360	4.389	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.800%
66) 1,2-Dichlorobenzene-d4	11.571	152	61614	4.918	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.400%
Target Compounds						Qvalue
13) Acetone	2.143	43	4153	1.721	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030308.D
Acq On : 23 Mar 2023 14:07
Operator : SY/MD
Sample : 02041-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB958

Quant Time: Mar 24 02:51:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 24 02:42:05 2023
Response via : Initial Calibration

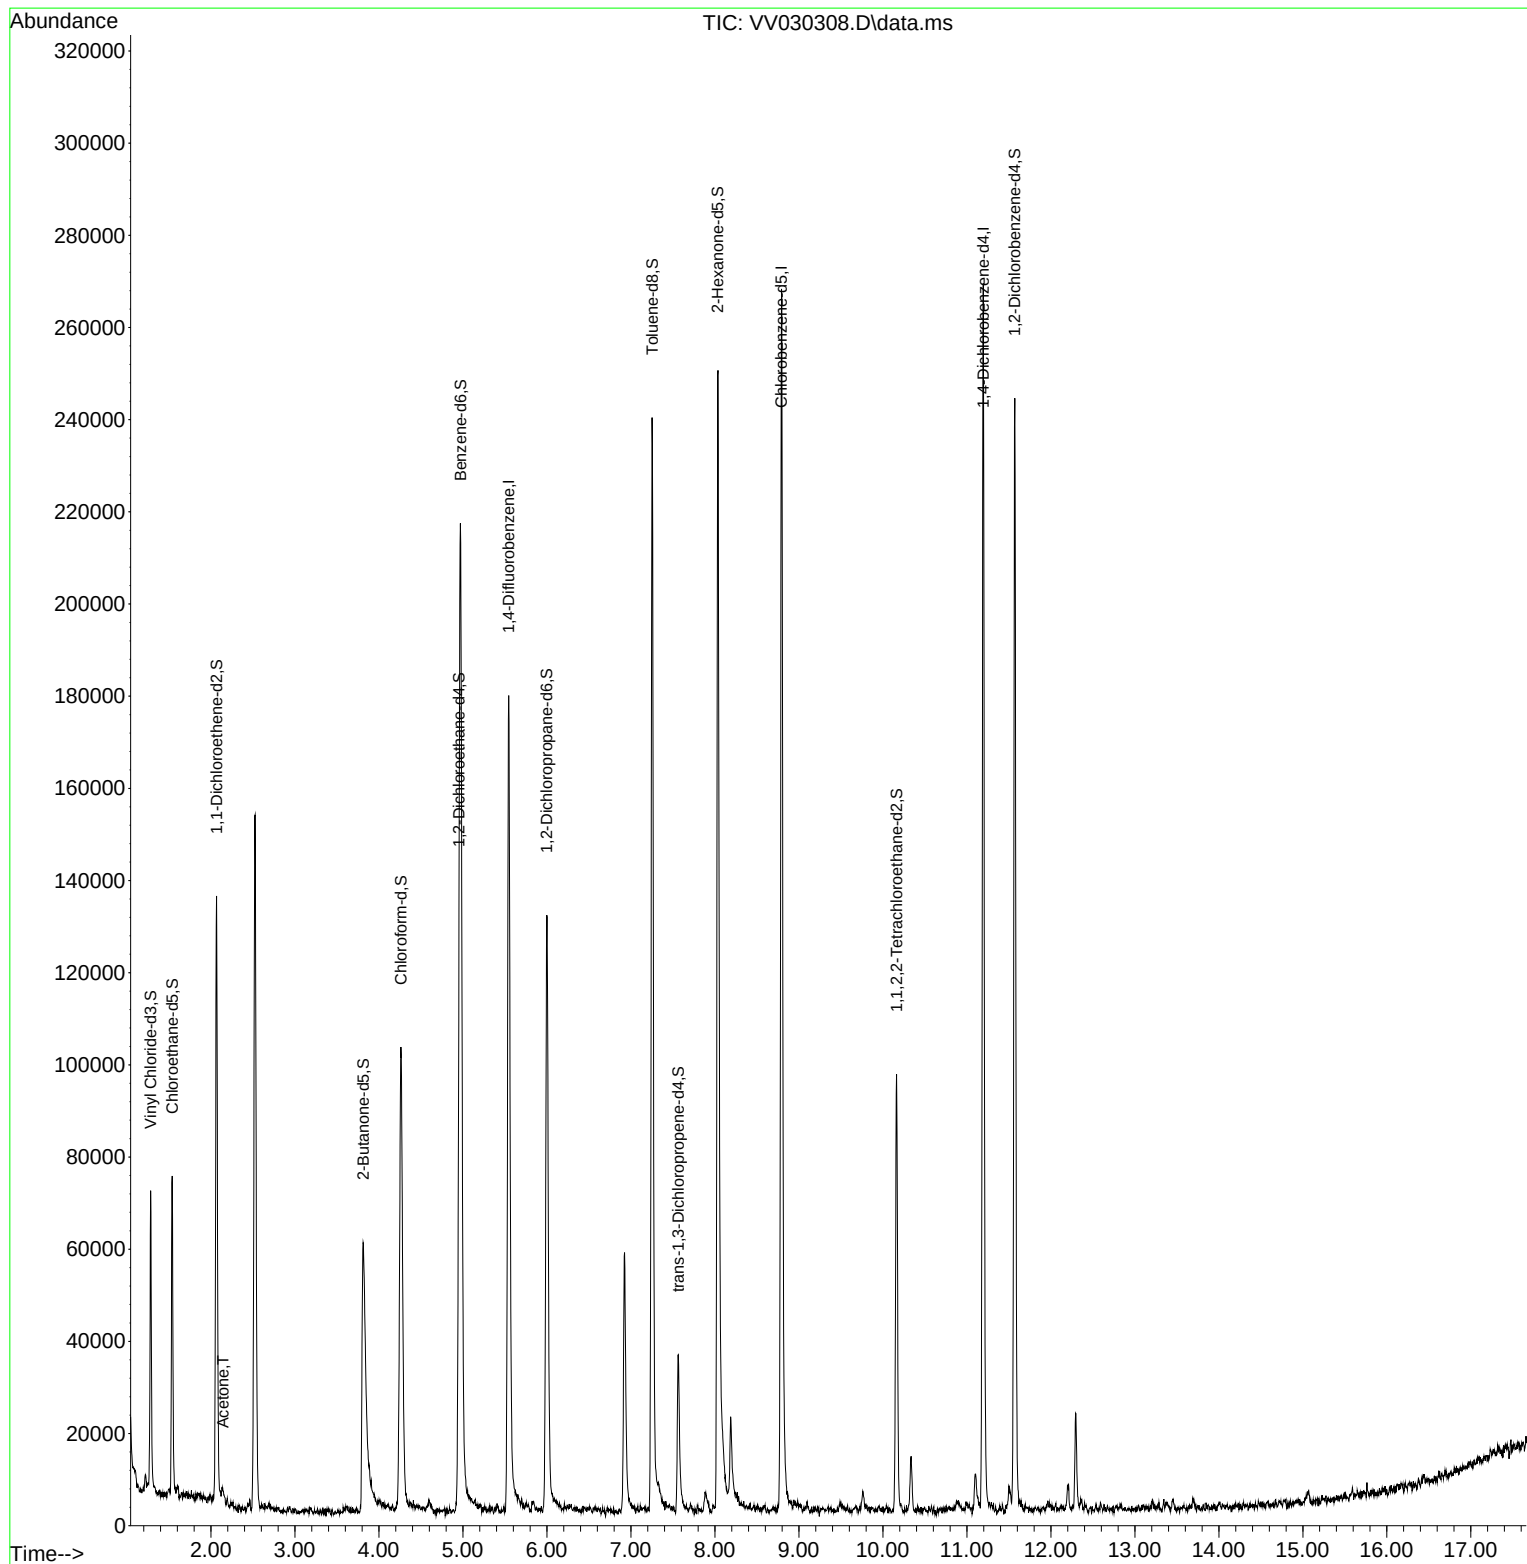

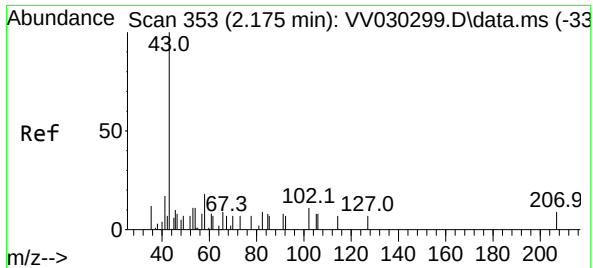

#13
 Acetone
 Concen: 1.721 ug/L
 RT: 2.143 min Scan# 34
 Delta R.T. -0.039 min
 Lab File: VV030308.D
 Acq: 23 Mar 2023 14:07

Instrument :
 MSVOA_V
 ClientSampleId :
 CB958

Tgt Ion: 43 Resp: 4153
 Ion Ratio Lower Upper
 43 100
 58 25.5 0.0 40.8

