

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032323\
 Data File : VW030313.D
 Acq On : 23 Mar 2023 16:08
 Operator : SY/MD
 Sample : 02053-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF70

Quant Time: Mar 24 02:52:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 24 02:42:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	130272	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	126076	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	60872	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	40746	4.723	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.400%
7) Chloroethane-d5	1.539	69	41319	4.935	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.600%
11) 1,1-Dichloroethene-d2	2.066	63	68579	3.350	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.000%
20) 2-Butanone-d5	3.818	46	115800	51.927	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.860%
24) Chloroform-d	4.262	84	104567	5.007	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
26) 1,2-Dichloroethane-d4	4.953	65	51204	5.197	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%
32) Benzene-d6	4.973	84	183905	5.176	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.600%
36) 1,2-Dichloropropane-d6	5.998	67	59742	5.371	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.400%
41) Toluene-d8	7.252	98	152174	4.664	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
43) trans-1,3-Dichloroprop...	7.564	79	19631	4.688	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.800%
46) 2-Hexanone-d5	8.033	63	84814	50.401	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.800%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	43418	4.953	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.000%
66) 1,2-Dichlorobenzene-d4	11.570	152	59902	5.506	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.200%
Target Compounds					Qvalue	
13) Acetone	2.140	43	28901	13.552	ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030313.D
Acq On : 23 Mar 2023 16:08
Operator : SY/MD
Sample : 02053-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF70

Quant Time: Mar 24 02:52:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 24 02:42:05 2023
Response via : Initial Calibration

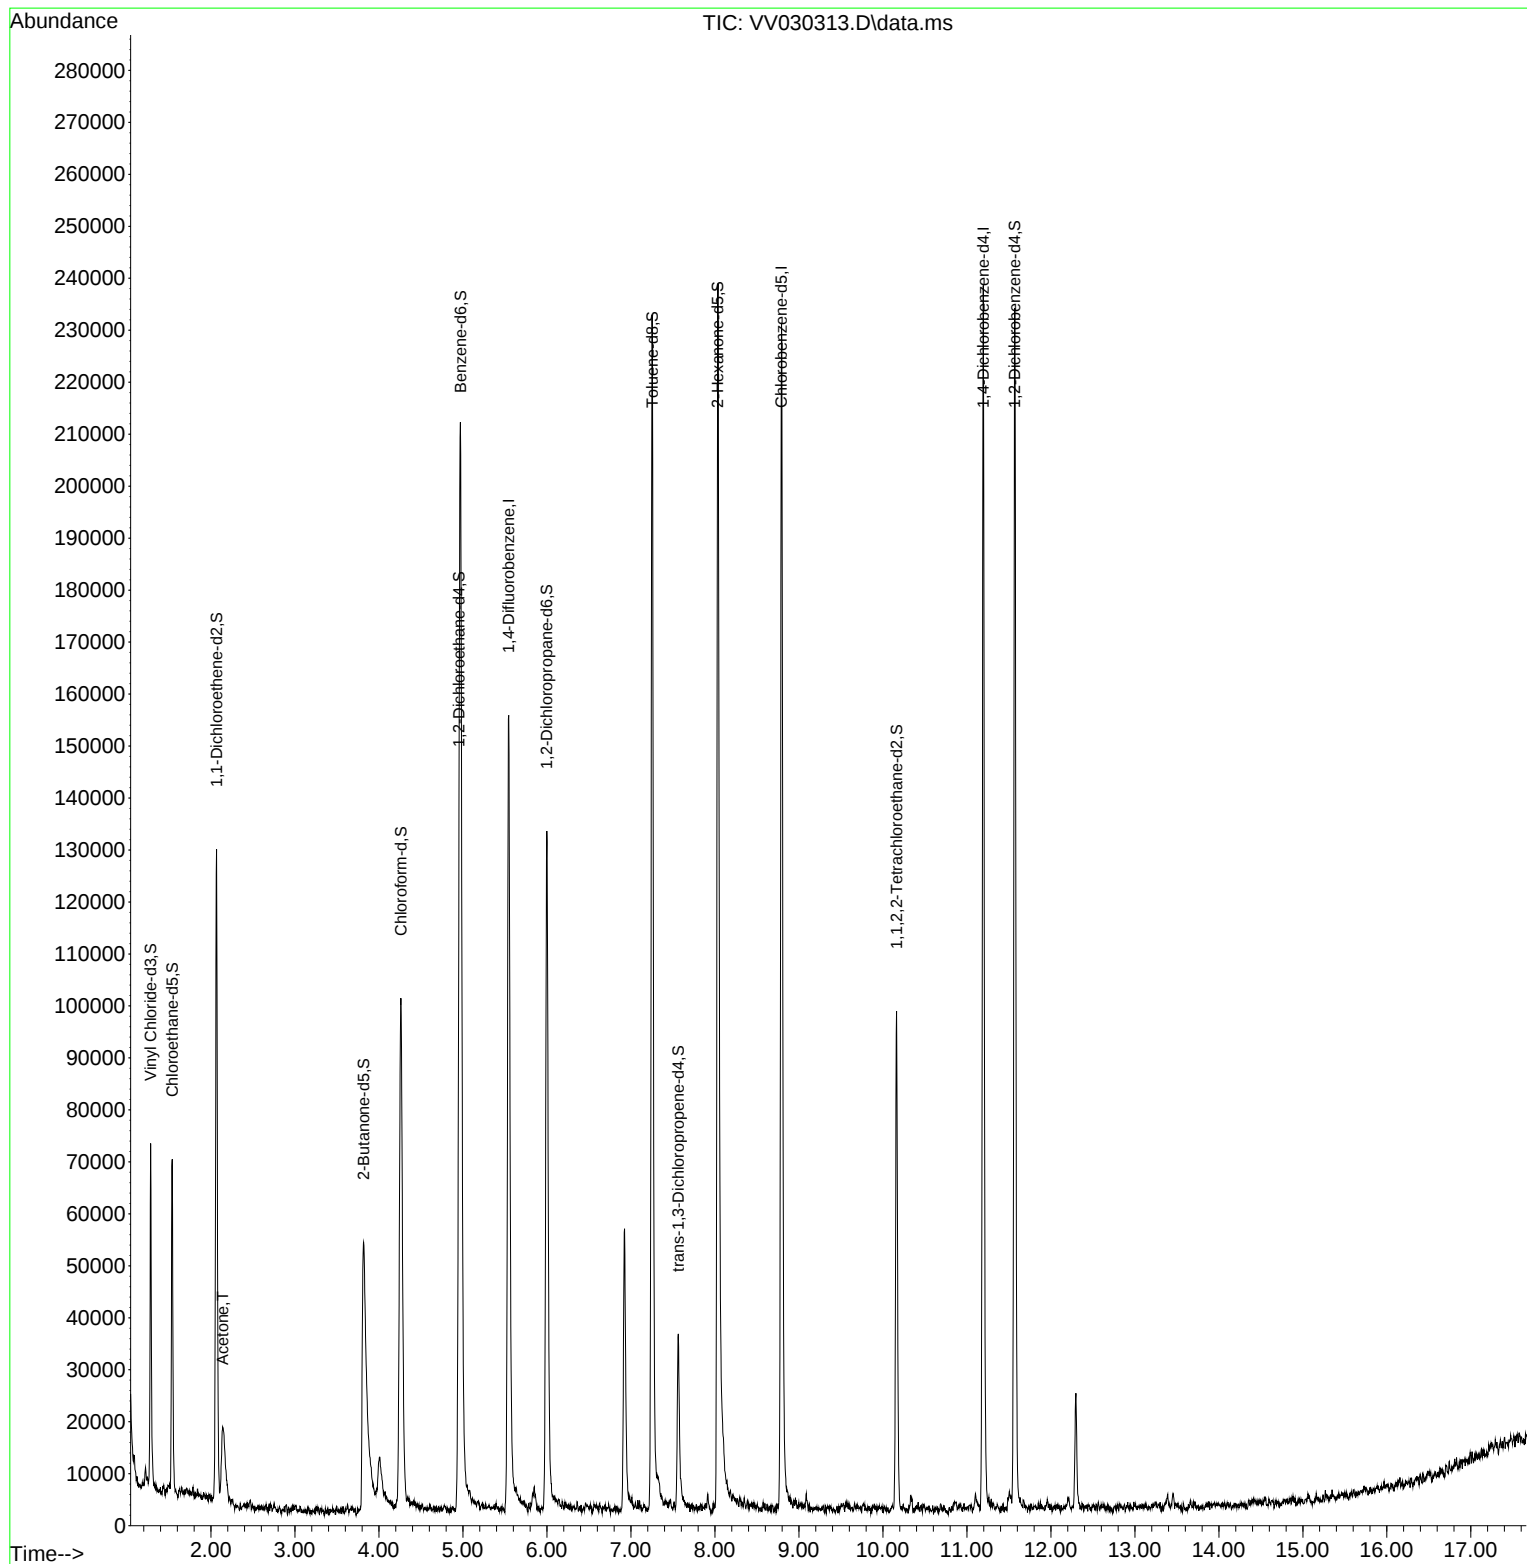

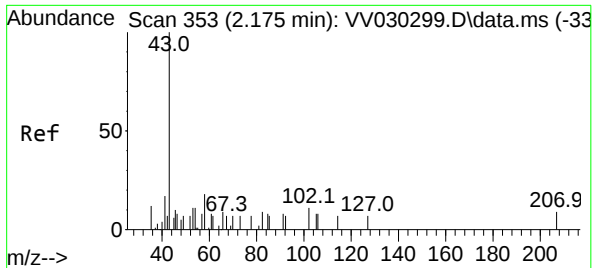

#13
 Acetone
 Concen: 13.552 ug/L
 RT: 2.140 min Scan# 34
 Delta R.T. -0.042 min
 Lab File: VV030313.D
 Acq: 23 Mar 2023 16:08

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF70

Tgt Ion: 43 Resp: 28901
 Ion Ratio Lower Upper
 43 100
 58 30.9 0.0 40.8

