

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
 Data File : VV030305.D
 Acq On : 23 Mar 2023 12:43
 Operator : SY/MD
 Sample : VV0323WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK318

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	61	rBV	7223	8877	1.57%	0.205%
2	1.278	68	74	89	rVB	70619	78215	13.85%	1.806%
3	1.535	146	154	164	rBV	69431	79172	14.02%	1.828%
4	2.063	308	318	332	rBV	135681	199184	35.27%	4.599%
5	2.455	429	440	449	rBV	10777	18845	3.34%	0.435%
6	3.838	855	870	871	rBV2	29389	40824	7.23%	0.943%
7	4.259	983	1001	1022	rBV	99557	252880	44.77%	5.839%
8	4.966	1203	1221	1251	rBV2	216174	564786	100.00%	13.041%
9	5.542	1384	1400	1418	rBV	169377	355389	62.92%	8.206%
10	5.834	1480	1491	1496	rBV	3698	7796	1.38%	0.180%
11	5.995	1528	1541	1564	rBV	129822	281225	49.79%	6.493%
12	6.921	1819	1829	1845	rBV2	56461	107127	18.97%	2.474%
13	7.252	1917	1932	1952	rBV	236812	434857	77.00%	10.041%
14	7.561	2016	2028	2041	rBV	34015	65113	11.53%	1.503%
15	8.037	2162	2176	2219	rBV	209625	484000	85.70%	11.175%
16	8.792	2398	2411	2432	rBV	253598	433178	76.70%	10.002%
17	10.162	2825	2837	2850	rBV	93872	150621	26.67%	3.478%
18	11.194	3146	3158	3180	rBV	233771	382061	67.65%	8.822%
19	11.570	3263	3275	3289	rBV	231178	365750	64.76%	8.445%
20	13.207	3777	3784	3792	rBV	4211	7233	1.28%	0.167%
21	13.451	3852	3860	3868	rBV6	4513	6776	1.20%	0.156%
22	13.689	3928	3934	3943	rVB10	4288	7004	1.24%	0.162%




Sum of corrected areas: 4330913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030305.D
Acq On : 23 Mar 2023 12:43
Operator : SY/MD
Sample : VV0323WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

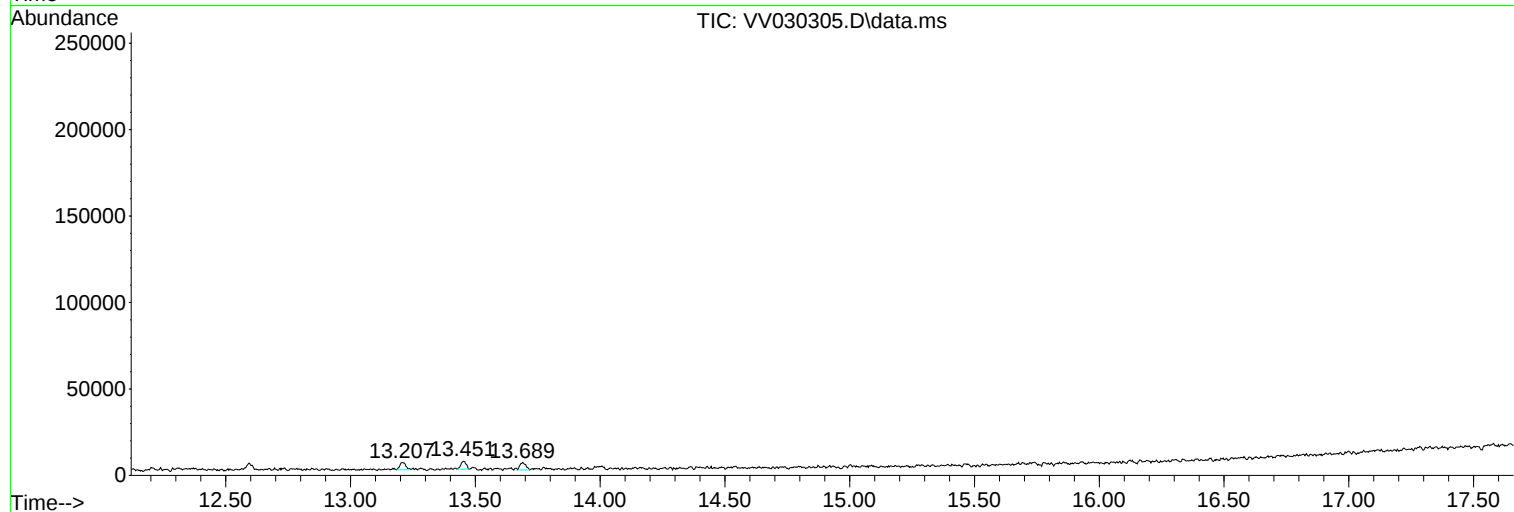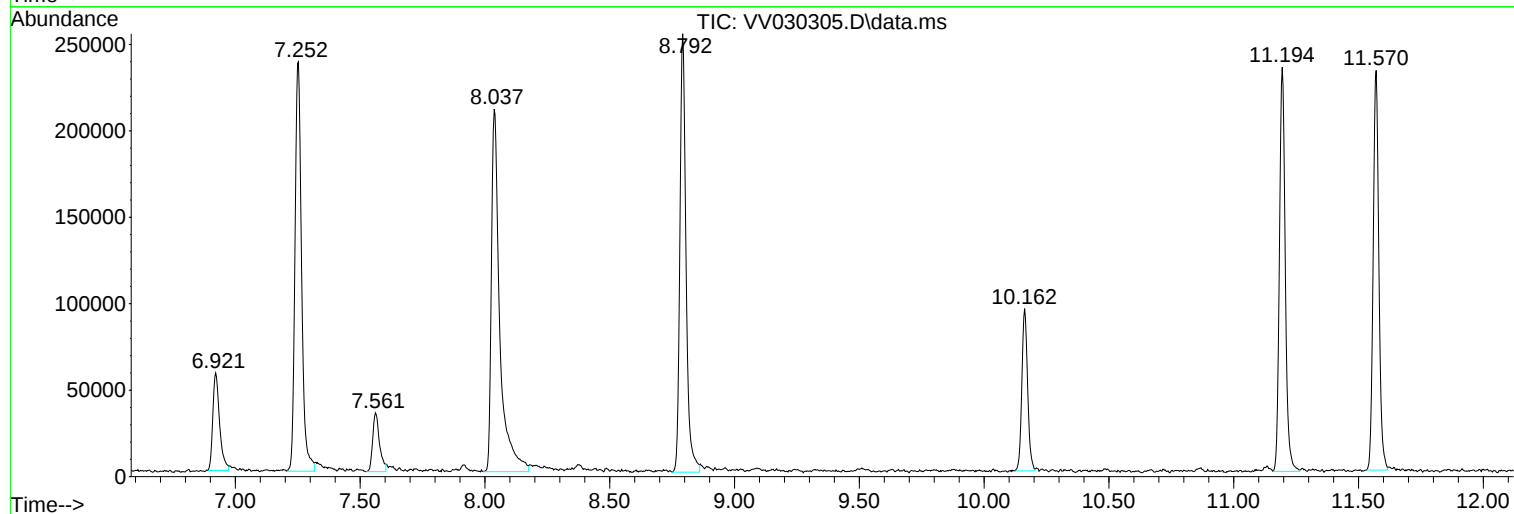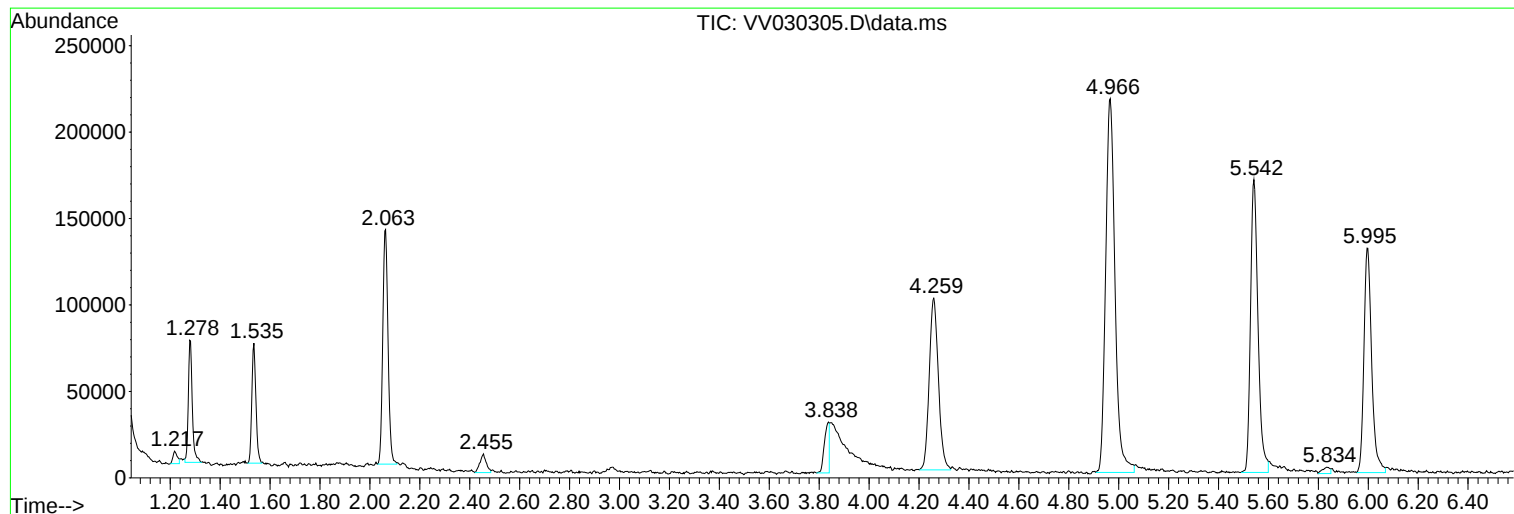

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030305.D
Acq On : 23 Mar 2023 12:43
Operator : SY/MD
Sample : VV0323WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030305.D
Acq On : 23 Mar 2023 12:43
Operator : SY/MD
Sample : VV0323WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc