

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
 Data File : VV030313.D
 Acq On : 23 Mar 2023 16:08
 Operator : SY/MD
 Sample : 02053-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF70

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rVB	65910	69829	12.95%	1.600%
2	1.539	147	155	166	rVB	63945	75249	13.96%	1.724%
3	2.066	308	319	331	rBV	124900	183915	34.11%	4.214%
4	2.140	332	342	364	rVB2	14309	46007	8.53%	1.054%
5	3.818	851	864	899	rBV2	51441	192366	35.68%	4.408%
6	4.008	914	923	938	rVB3	7347	19130	3.55%	0.438%
7	4.262	983	1002	1023	rBV	97946	251468	46.64%	5.762%
8	4.969	1204	1222	1245	rBV2	209658	539130	100.00%	12.354%
9	5.545	1387	1401	1423	rBV	153359	330757	61.35%	7.579%
10	5.998	1528	1542	1562	rBV	130471	273596	50.75%	6.269%
11	6.924	1816	1830	1847	rBV2	54388	105192	19.51%	2.410%
12	7.252	1919	1932	1954	rBV	229986	420085	77.92%	9.626%
13	7.564	2018	2029	2038	rBV	33832	60031	11.13%	1.376%
14	8.037	2165	2176	2207	rBV	235496	479569	88.95%	10.989%
15	8.792	2399	2411	2430	rBV	228083	395517	73.36%	9.063%
16	10.162	2826	2837	2853	rVB	95841	150753	27.96%	3.454%
17	11.194	3146	3158	3174	rBV	235748	368018	68.26%	8.433%
18	11.570	3264	3275	3293	rBV	229938	368648	68.38%	8.447%
19	12.297	3491	3501	3512	rBV3	22023	34897	6.47%	0.800%




Sum of corrected areas: 4364157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030313.D
Acq On : 23 Mar 2023 16:08
Operator : SY/MD
Sample : 02053-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

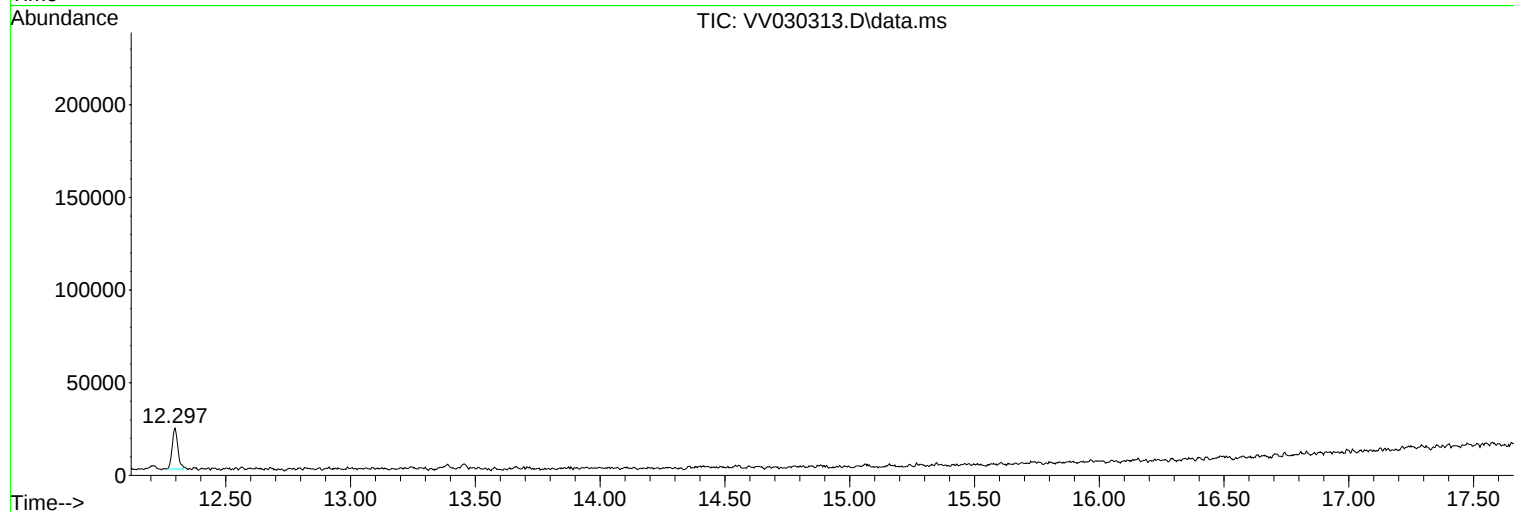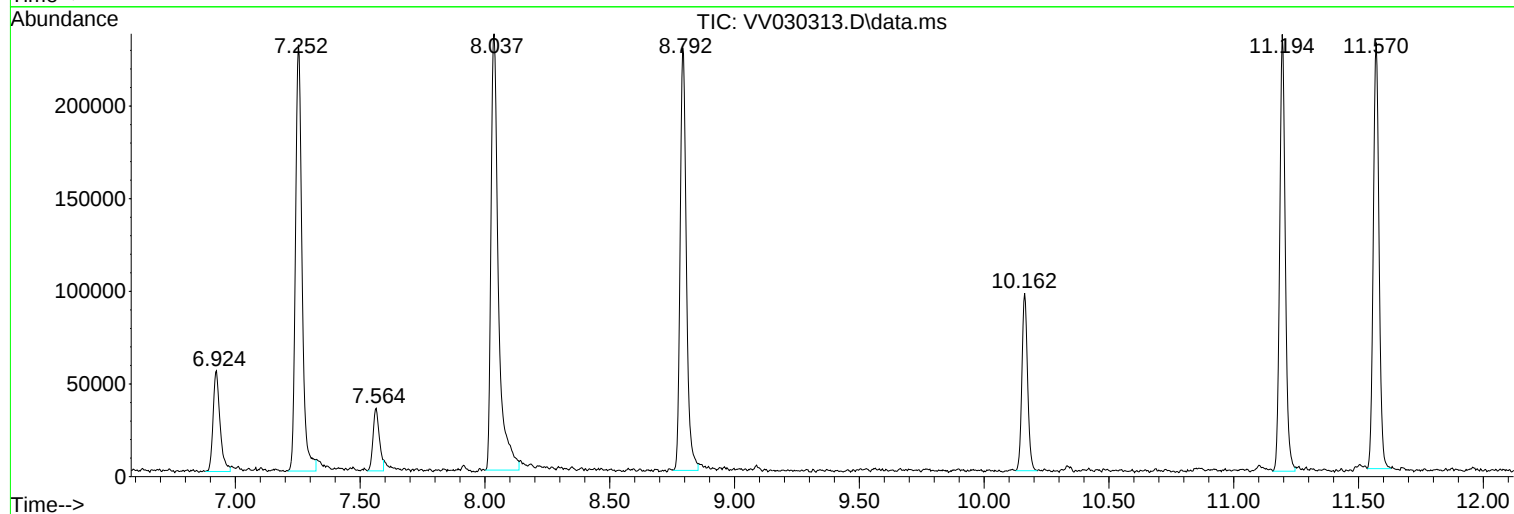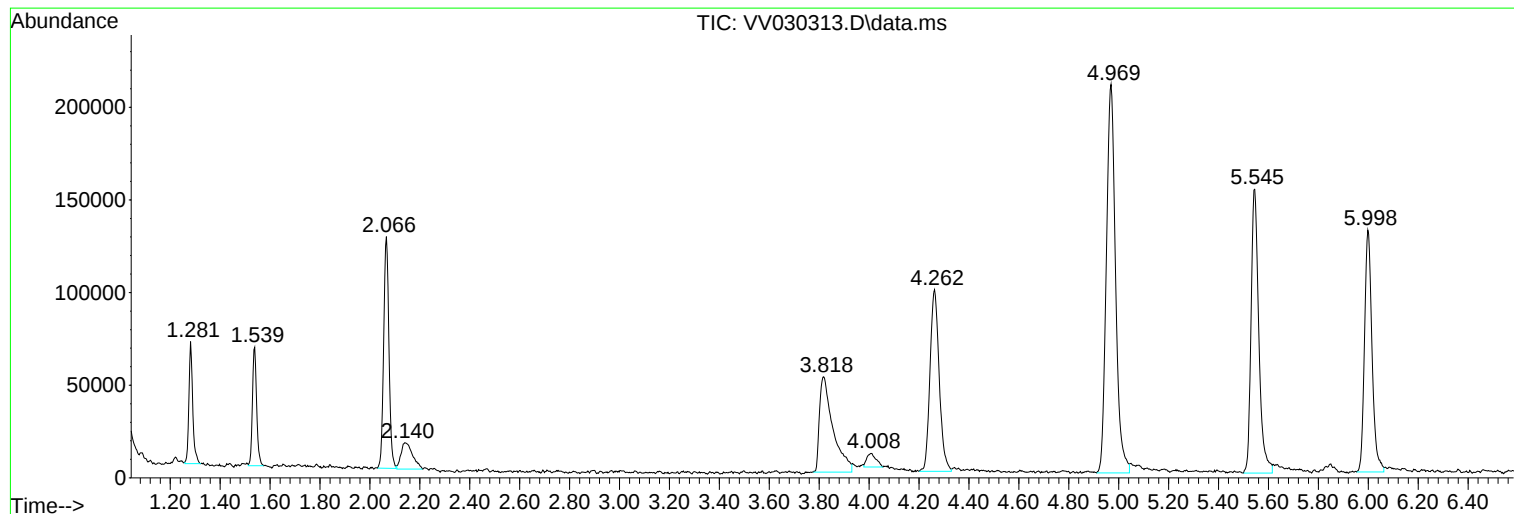

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030313.D
Acq On : 23 Mar 2023 16:08
Operator : SY/MD
Sample : 02053-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030313.D
Acq On : 23 Mar 2023 16:08
Operator : SY/MD
Sample : 02053-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------