

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
 Data File : VV030316.D
 Acq On : 23 Mar 2023 17:22
 Operator : SY/MD
 Sample : 02053-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF73

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rVB	61284	67390	12.37%	1.547%
2	1.539	147	155	167	rVB	63531	77256	14.18%	1.774%
3	2.066	308	319	333	rBV	124590	182981	33.59%	4.201%
4	3.815	850	863	888	rBV2	54573	190298	34.93%	4.369%
5	3.999	910	920	946	rVB2	20463	60190	11.05%	1.382%
6	4.262	987	1002	1023	rBV2	95676	242740	44.56%	5.572%
7	4.970	1203	1222	1247	rBV2	207678	544808	100.00%	12.507%
8	5.545	1388	1401	1423	rBV	157801	333485	61.21%	7.656%
9	5.998	1528	1542	1559	rBV	128327	269174	49.41%	6.179%
10	6.921	1818	1829	1847	rBV2	54227	105024	19.28%	2.411%
11	7.252	1919	1932	1946	rBV	224717	407068	74.72%	9.345%
12	7.561	2017	2028	2045	rBV2	33612	65729	12.06%	1.509%
13	8.037	2162	2176	2205	rBV	248200	494995	90.86%	11.363%
14	8.796	2399	2412	2433	rBV	240683	414289	76.04%	9.511%
15	10.162	2826	2837	2852	rBV	95489	151729	27.85%	3.483%
16	10.336	2883	2891	2900	rVB5	4861	8082	1.48%	0.186%
17	11.194	3147	3158	3175	rBV	238394	372082	68.30%	8.542%
18	11.571	3263	3275	3290	rBV	231424	368734	67.68%	8.465%




Sum of corrected areas: 4356054

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030316.D
Acq On : 23 Mar 2023 17:22
Operator : SY/MD
Sample : 02053-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

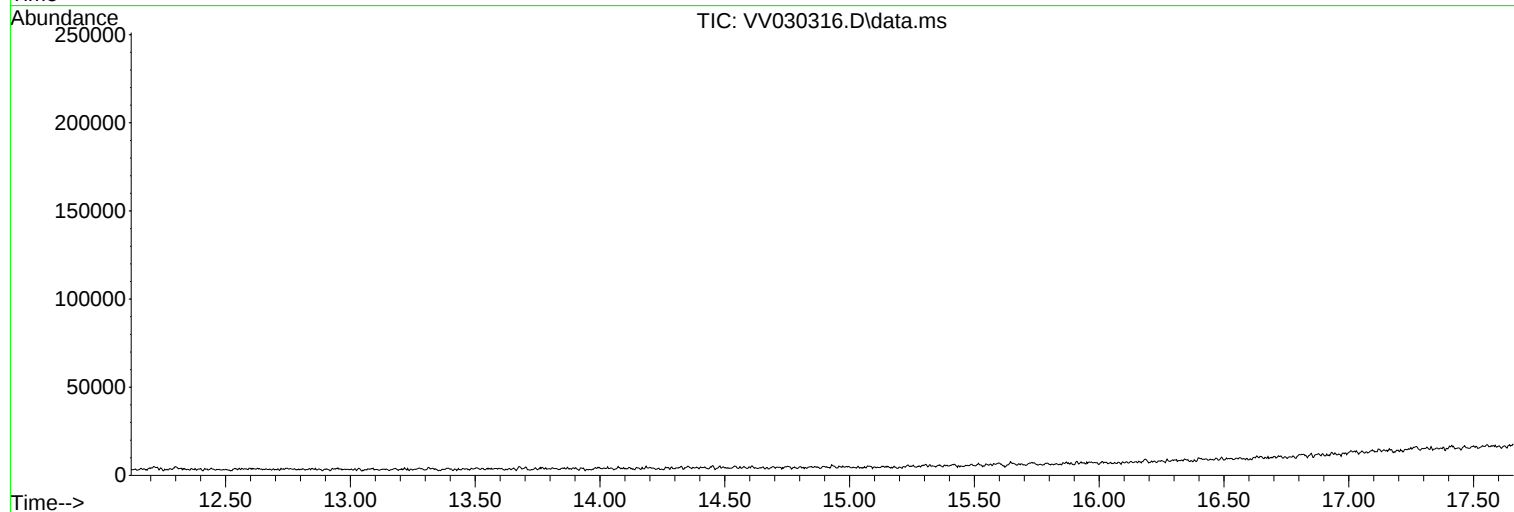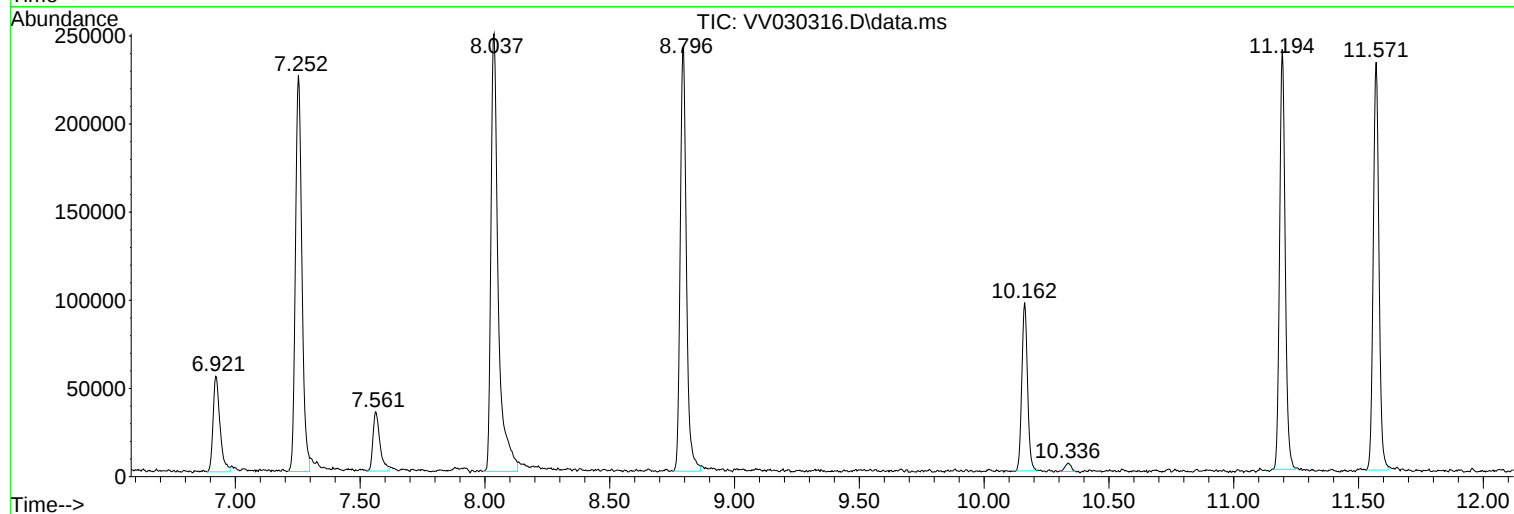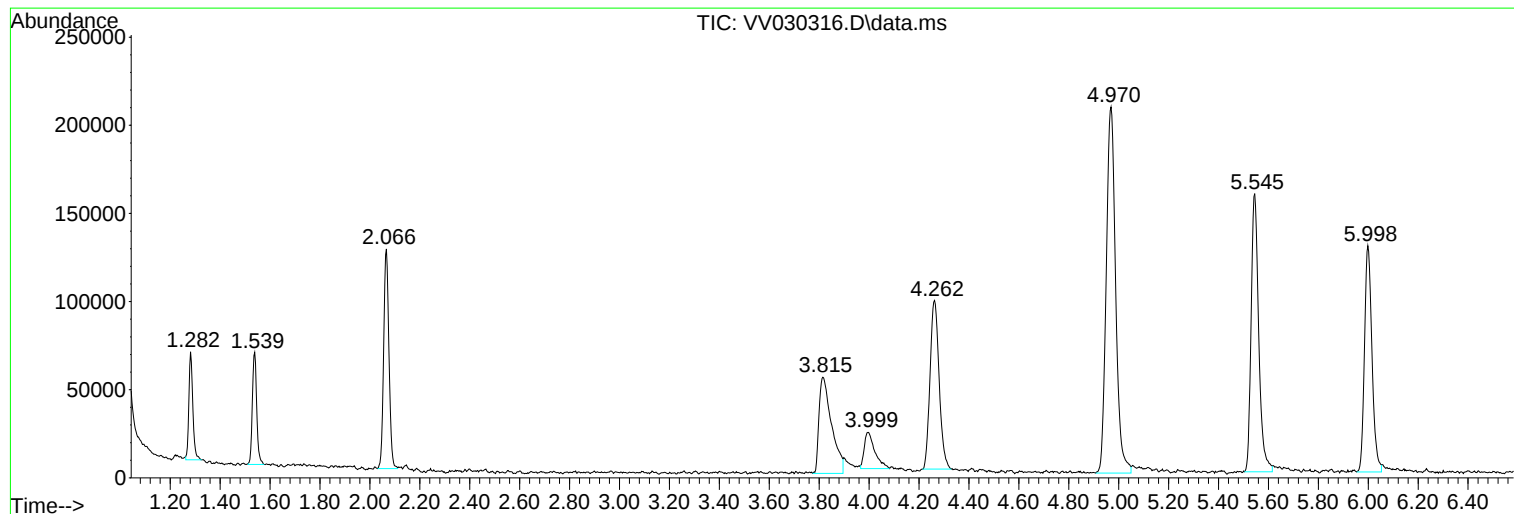

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030316.D
Acq On : 23 Mar 2023 17:22
Operator : SY/MD
Sample : 02053-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF73










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethyl Acetate Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.999	0.90 ug/L	60190	1,4-Difluorobenzene	5.545

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethyl Acetate	88	C4H8O2	000141-78-6	86
2			Ethyl Acetate	88	C4H8O2	000141-78-6	80
3			Ethyl Acetate	88	C4H8O2	000141-78-6	80
4			Ethyl Acetate	88	C4H8O2	000141-78-6	72
5			CH3C(O)CH2CH2OH	88	C4H8O2	000590-90-9	50

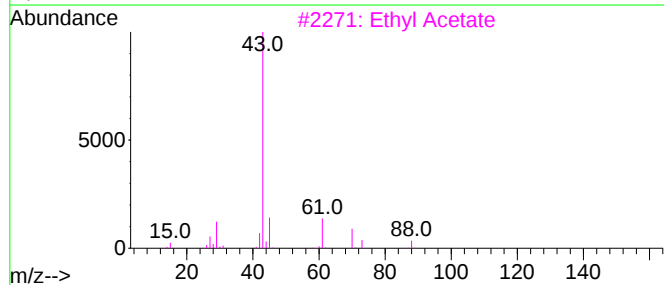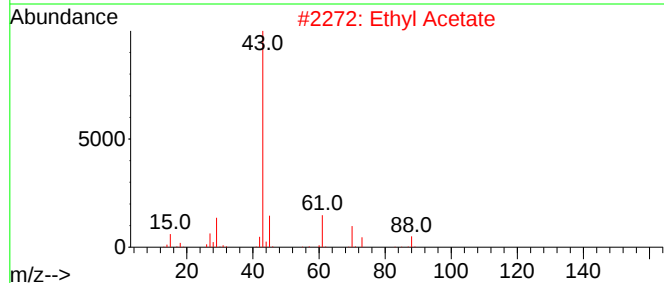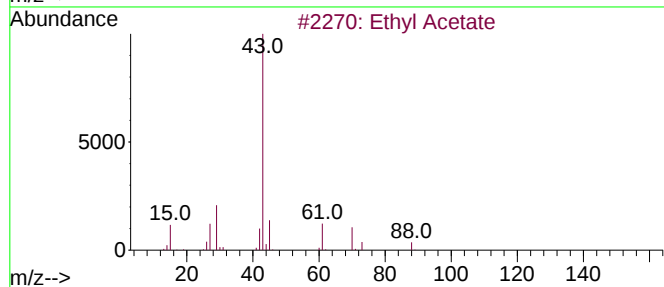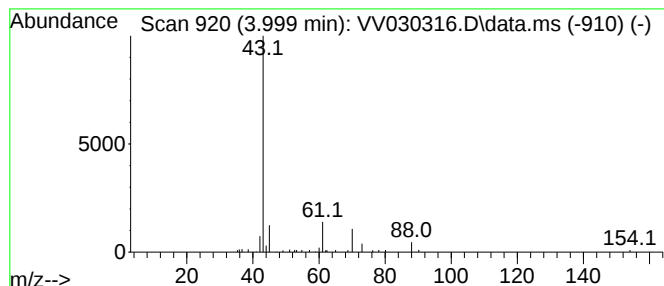

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030316.D
Acq On : 23 Mar 2023 17:22
Operator : SY/MD
Sample : 02053-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethyl Acetate	3.999	0.9	ug/L	60190	1	5.545	333485	5.0