
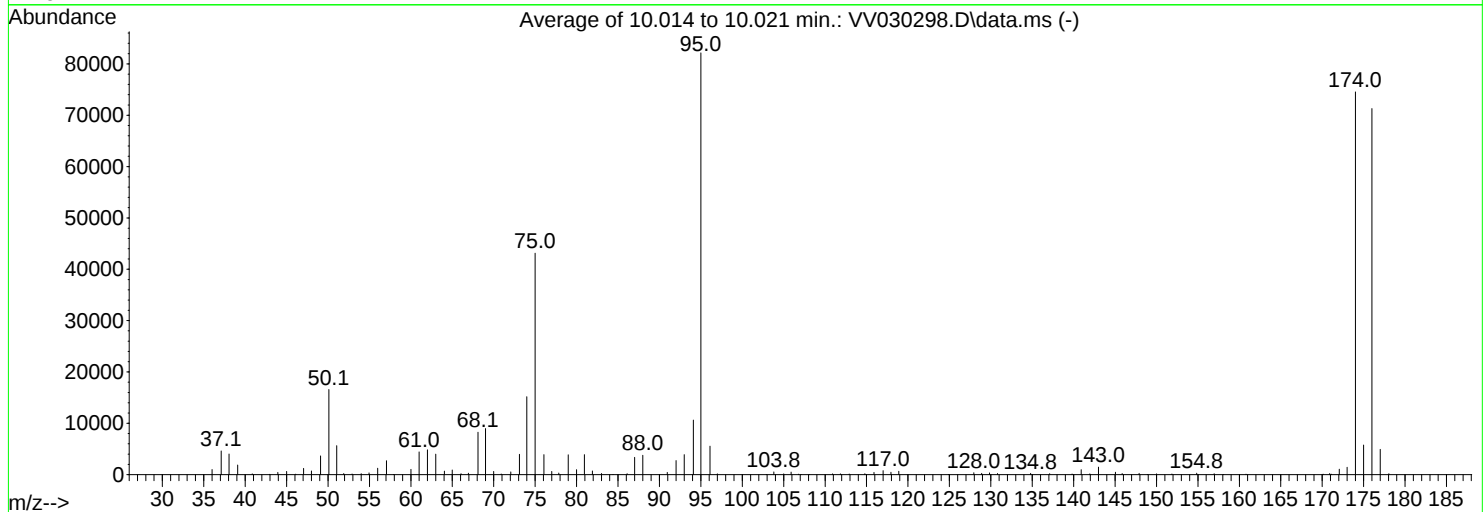


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032323\
Data File : VV030298.D
Acq On : 23 Mar 2023 09:17
Operator : SY/MD
Sample : BFB238
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB238

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 24 02:42:05 2023

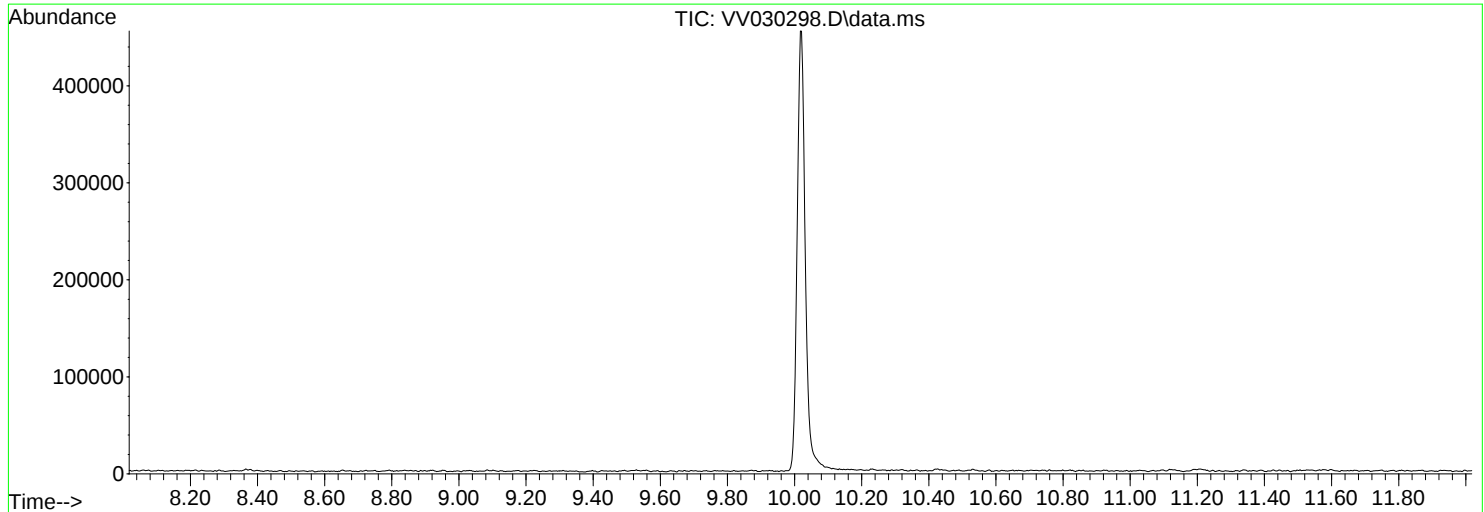

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	16569	PASS
75	95	30	80	52.5	43125	PASS
95	95	100	100	100.0	82149	PASS
96	95	5	9	6.8	5558	PASS
173	174	0.00	2	1.9	1436	PASS
174	95	50	120	90.8	74555	PASS
175	174	5	9	7.7	5770	PASS
176	174	95	105	95.6	71293	PASS
177	176	5	10	6.9	4932	PASS

m/z	Abundance
36.80	155.0
37.30	137.0
37.80	115.0
38.40	132.0
40.00	219.0
40.50	158.0
41.90	111.0
42.90	135.0
43.90	343.0
45.00	117.0
46.00	131.0
47.30	109.0
50.70	105.0
51.80	115.0
53.00	144.0
54.60	103.0
56.80	107.0
57.90	110.0
59.00	103.0
61.50	108.0
63.30	130.0
68.80	118.0
69.90	125.0
74.70	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
36.00	927.0
37.10	4386.0
38.10	3950.0
39.10	1750.0
40.00	248.0
40.90	169.0
43.00	182.0
44.00	772.0
45.00	651.0
46.20	254.0
47.10	1101.0
48.00	595.0
49.10	3452.0
50.10	15772.0
51.00	5391.0
52.00	346.0
52.90	243.0
54.00	210.0
55.00	295.0
56.00	1111.0
57.00	2606.0
57.90	145.0
59.20	114.0
60.00	1011.0
61.00	4081.0
62.00	4556.0
63.00	4000.0
64.00	704.0
65.00	802.0
66.10	165.0
66.90	299.0
68.10	7854.0
69.00	8535.0
70.10	690.0
70.90	122.0
72.10	449.0
73.10	3710.0
74.00	14333.0
75.00	40544.0
76.00	3846.0
77.00	572.0
77.80	253.0
79.00	3642.0
80.00	935.0
81.00	3786.0
81.90	703.0
83.00	211.0
84.40	111.0
86.00	202.0
87.00	3361.0
88.00	3667.0
90.90	393.0
92.00	2547.0
93.00	3711.0
94.10	9937.0
95.00	77688.0
96.10	5408.0
96.90	156.0
102.90	101.0
103.80	534.0
105.00	129.0
105.90	433.0
106.80	134.0
110.90	121.0
111.80	136.0
112.90	129.0
114.80	176.0
115.90	391.0
117.00	768.0
118.00	428.0
118.90	626.0
128.00	358.0
128.90	225.0
129.80	280.0
130.80	208.0
134.80	224.0
137.10	155.0
139.80	146.0
140.90	940.0
141.90	126.0
143.00	1377.0
145.10	444.0
145.90	232.0
147.80	231.0
150.00	136.0
151.90	143.0
154.90	261.0
157.00	180.0
170.90	340.0
172.10	987.0
173.00	1388.0
174.00	67512.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

175.00	5431.0
176.00	65544.0
177.00	4608.0
178.00	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
36.00	1043.0
37.10	4918.0
38.00	4149.0
39.10	1947.0
40.10	235.0
40.80	176.0
41.80	106.0
43.00	214.0
44.00	801.0
45.10	759.0
46.20	221.0
47.10	1282.0
48.00	733.0
49.10	3710.0
50.10	17168.0
51.10	5869.0
52.00	342.0
52.90	276.0
54.00	194.0
54.90	348.0
56.00	1269.0
57.10	2796.0
58.00	156.0
59.20	110.0
60.00	1047.0
61.00	4587.0
62.00	5091.0
63.00	4109.0
64.00	679.0
65.00	957.0
66.00	169.0
66.90	302.0
68.10	8446.0
69.00	9214.0
70.00	745.0
70.90	141.0
72.10	533.0
73.10	4093.0
74.00	15627.0
75.00	44488.0
76.10	3990.0
77.00	646.0
77.80	310.0
79.00	4034.0
80.00	1017.0
81.00	4091.0
81.90	744.0
83.00	213.0
86.10	203.0
87.00	3518.0
88.00	3941.0
90.90	419.0
92.00	2802.0
93.00	4039.0
94.10	10877.0
95.00	84776.0
96.10	5729.0
97.00	160.0
103.80	580.0
105.00	160.0
105.90	505.0
106.80	124.0
110.90	154.0
111.90	157.0
112.90	126.0
114.80	195.0
115.90	425.0
117.00	834.0
117.90	493.0
118.90	690.0
124.90	104.0
128.00	408.0
128.90	252.0
129.90	364.0
130.80	226.0
134.80	256.0
137.10	187.0
139.80	140.0
140.90	982.0
142.00	152.0
143.00	1547.0
145.00	461.0
145.80	207.0
147.90	257.0
148.90	101.0
150.00	161.0
151.80	137.0
154.90	292.0
157.00	209.0
160.80	127.0
170.10	136.0
170.90	312.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

172.00	1055.0
173.00	1497.0
174.00	77024.0
175.00	5931.0
176.00	73664.0
177.00	5128.0
178.00	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
36.00	1035.0
37.10	4945.0
38.10	4005.0
39.10	1885.0
40.30	268.0
40.80	175.0
41.70	114.0
43.00	218.0
44.00	790.0
45.10	825.0
46.20	195.0
47.00	1267.0
48.00	814.0
49.10	3773.0
50.10	16768.0
51.10	5646.0
52.00	307.0
52.90	279.0
54.00	162.0
54.90	398.0
56.00	1340.0
57.10	2722.0
58.00	160.0
60.00	997.0
61.00	4642.0
62.00	4895.0
63.00	3872.0
64.10	661.0
65.00	981.0
66.00	204.0
67.00	275.0
68.10	8491.0
69.00	9168.0
70.00	795.0
70.90	146.0
72.00	591.0
73.10	4076.0
74.00	15609.0
75.00	44344.0
76.00	3818.0
77.00	634.0
77.90	365.0
79.00	3920.0
80.00	989.0
80.90	3835.0
81.90	749.0
83.00	188.0
86.20	174.0
87.00	3247.0
88.00	3728.0
91.00	470.0
92.00	2837.0
93.00	3984.0
94.10	11026.0
95.00	83984.0
96.10	5537.0
97.10	153.0
103.80	522.0
105.00	176.0
105.90	540.0
107.10	125.0
108.10	106.0
110.90	158.0
111.90	149.0
112.90	143.0
114.80	185.0
115.90	460.0
117.00	767.0
117.90	518.0
118.90	693.0
127.90	394.0
128.90	243.0
129.90	411.0
130.80	242.0
134.80	262.0
137.10	223.0
139.80	133.0
140.90	947.0
142.00	181.0
143.00	1462.0
145.00	471.0
145.80	185.0
148.00	243.0
150.00	154.0
151.80	122.0
154.80	270.0
156.90	202.0
158.10	124.0
160.80	137.0
170.10	174.0
171.10	260.0
172.00	1115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

173.00	1422.0
174.00	79128.0
175.00	5947.0
176.00	74672.0
177.00	5061.0
178.10	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238