
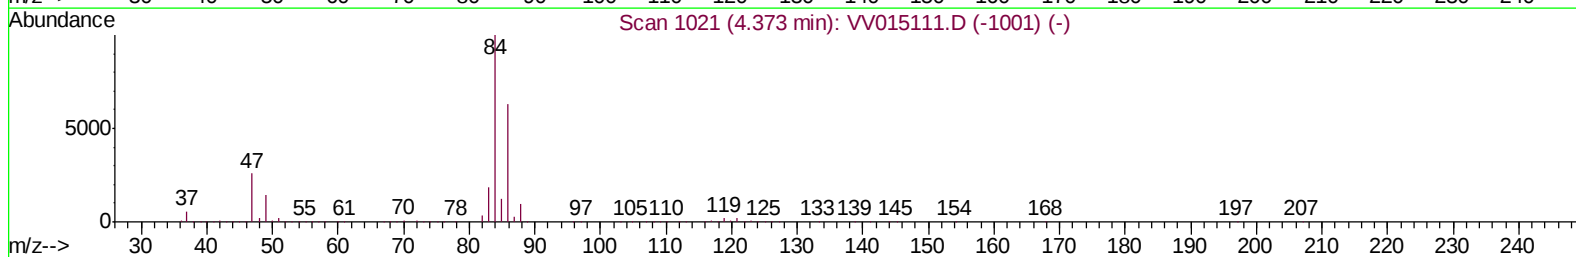
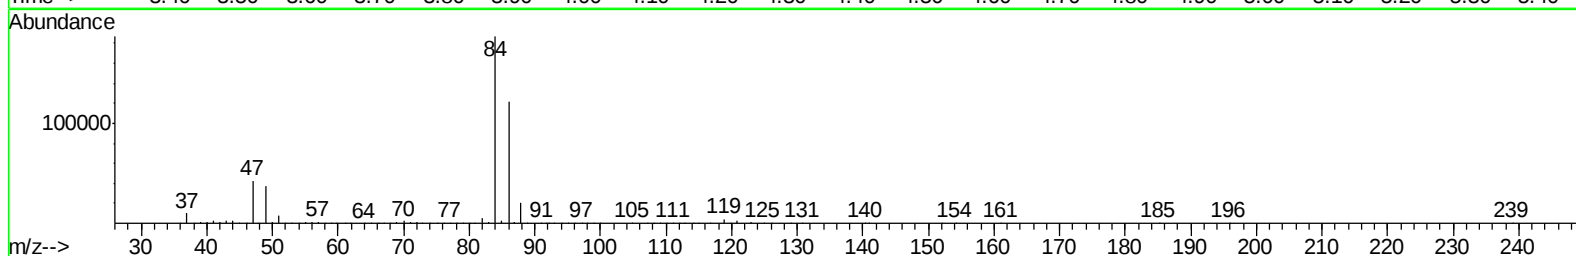


Data File : VV015115.D
Acq On : 24 Mar 2020 11:28
Operator : SY/MD
Sample : L1941-12DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 01:13:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 25 01:10:42 2020
Response via : Initial Calibration

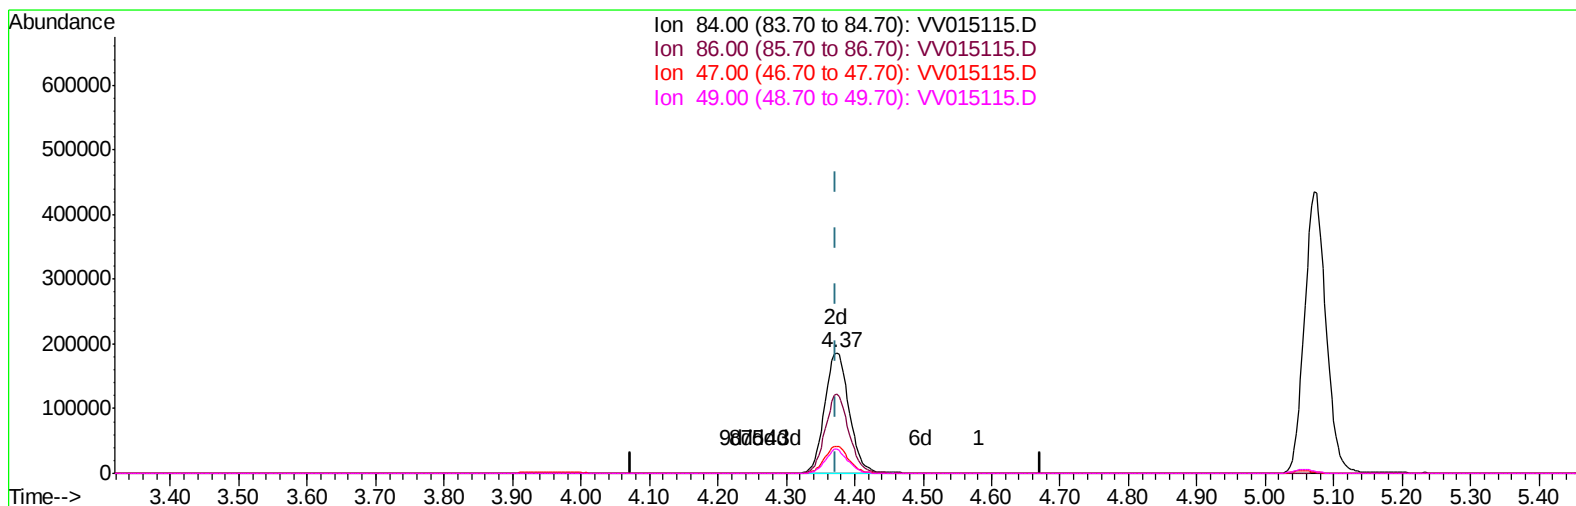

TIC: VV015115.D

(24) Chloroform-d (S)

4.373min (+0.000) 38.52ug/L m

response 460524

Ion	Exp%	Act%
84.00	100	100
86.00	62.30	0.05#
47.00	43.40	0.03#
49.00	26.10	0.01#