

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032420\
Quantitation Report (Qedit)




Data File : VV015112.D
Acq On : 24 Mar 2020 09:46
Operator : SY/MD
Sample : VV0324WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK91

Manual Integrations
APPROVED

apatel
3/25/2020 4:52:37 PM

Quant Time: Mar 25 01:12:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 25 01:10:42 2020
Response via : Initial Calibration

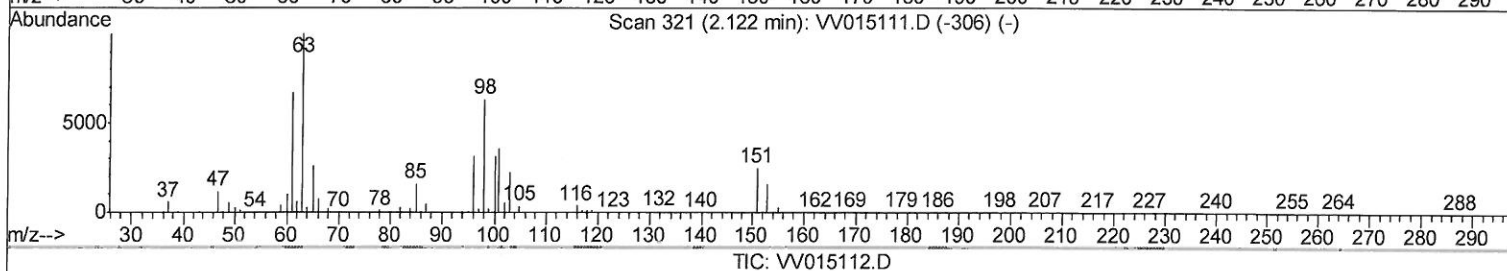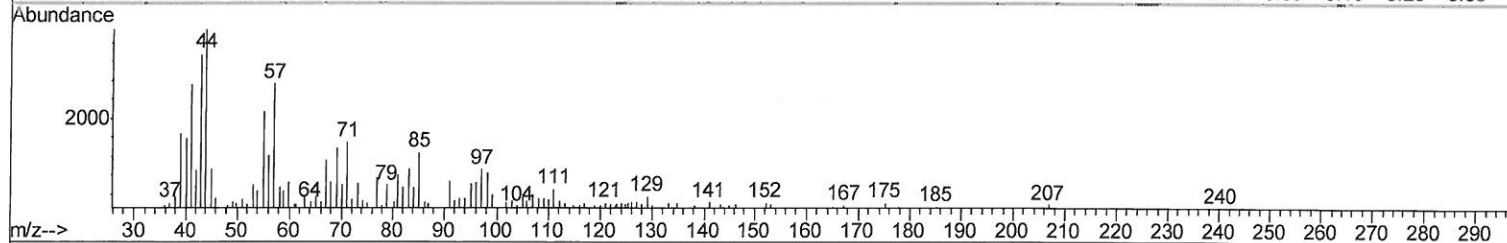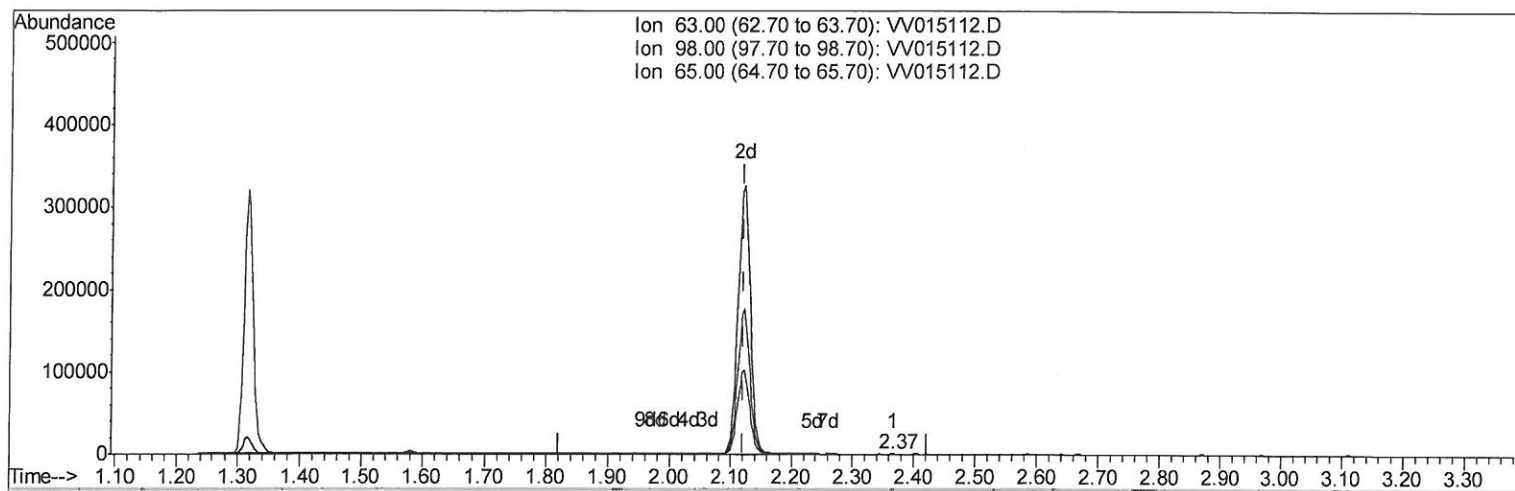

TIC: VV015112.D

(11) 1,1-Dichloroethene-d2 (S)

2.367min (+0.244) 0.04ug/L

response 428

Ion	Exp%	Act%
63.00	100	100
98.00	67.50	86.45
65.00	23.90	21.96
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032420\
Quantitation Report (Qedit)




Data File : VV015112.D
Acq On : 24 Mar 2020 09:46
Operator : SY/MD
Sample : VV0324WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK91

Manual Integrations
APPROVED

apatel
3/25/2020 4:52:37 PM

Quant Time: Mar 25 01:12:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 25 01:10:42 2020
Response via : Initial Calibration

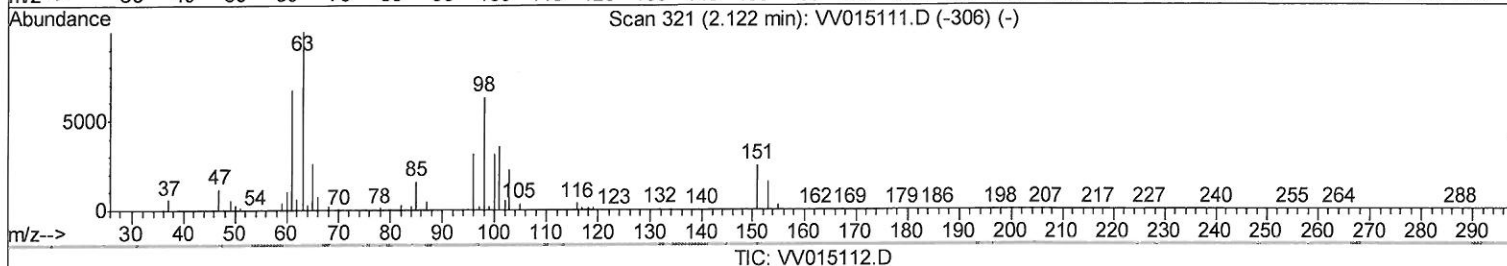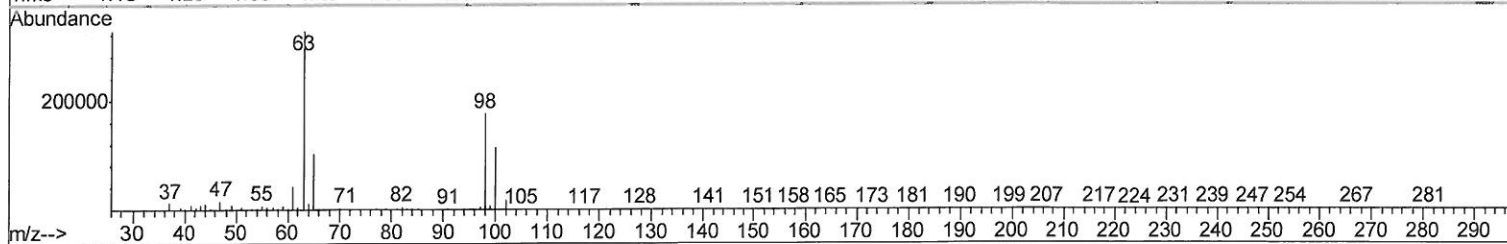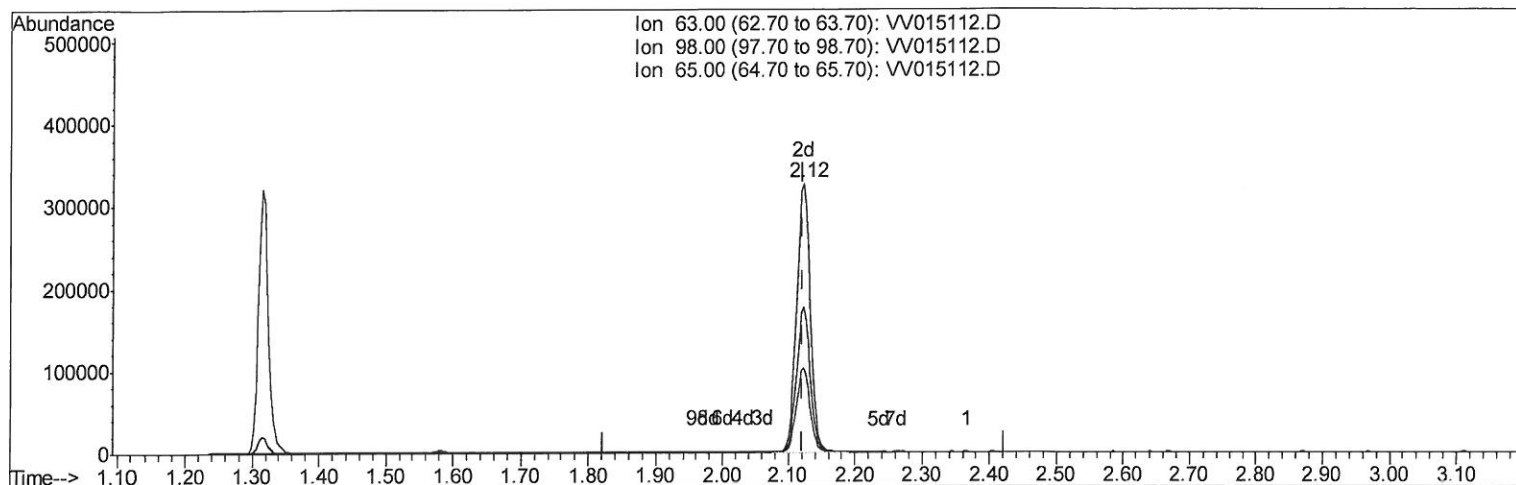

(11) 1,1-Dichloroethene-d2 (S)

2.122min (0.000) 38.60ug/L m

> 3/27/2024

response 470203

Ion	Exp%	Act%
63.00	100	100
98.00	67.50	0.08#
65.00	23.90	0.02#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032420\
 Quantitation Report (QT Reviewed)

Data File : VV015112.D
 Acq On : 24 Mar 2020 09:46
 Operator : SY/MD
 Sample : VV0324WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK91

Manual Integrations
 APPROVED

apatel
 3/25/2020 4:52:37 PM

Quant Time: Mar 25 01:28:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 25 01:10:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	789954	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	750996	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	349577	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	328628	45.04	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.08%		
7) Chloroethane-d5	1.58	69	288172	46.66	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.32%		
11) 1,1-Dichloroethene-d2	2.12	63	470203m	38.60	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.20%		
21) 2-Butanone-d5	3.94	46	411511	86.56	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	86.56%		
24) Chloroform-d	4.38	84	490513	44.47	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.94%		
26) 1,2-Dichloroethane-d4	5.06	65	319037	45.43	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.86%		
32) Benzene-d6	5.08	84	1038087	45.64	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.28%		
36) 1,2-Dichloropropane-d6	6.10	67	328663	44.15	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.30%		
41) Toluene-d8	7.34	98	995753	47.21	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.42%		
43) trans-1,3-Dichloropropene-	7.64	79	172624	43.91	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.82%		
47) 2-Hexanone-d5	8.11	63	326180	87.21	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.21%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	447636	42.88	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.76%		
64) 1,2-Dichlorobenzene-d4	11.65	152	362946	46.50	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.00%		

03/27/2020

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032420\
Quantitation Report (QT Reviewed)

Data File : VV015112.D
Acq On : 24 Mar 2020 09:46
Operator : SY/MD
Sample : VV0324WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK91

Manual Integrations
APPROVED

apatel
3/25/2020 4:52:37 PM

Quant Time: Mar 25 01:28:01 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 25 01:10:42 2020
Response via : Initial Calibration

