

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015115.D
 Acq On : 24 Mar 2020 11:28
 Operator : SY/MD
 Sample : L1941-12DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC3DL

Manual Integrations
 APPROVED

apatel
 3/25/2020 4:52:40 PM

Quant Time: Mar 25 01:51:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 25 01:10:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	856140	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	811035	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	384274	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	293062	37.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.12%
7) Chloroethane-d5	1.58	69	253056	37.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	75.62%
11) 1,1-Dichloroethene-d2	2.12	63	413731	31.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.68%
21) 2-Butanone-d5	3.93	46	371387	72.08	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	72.08%
24) Chloroform-d	4.37	84	460524m	38.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.04%
26) 1,2-Dichloroethane-d4	5.05	65	298425	39.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.42%
32) Benzene-d6	5.07	84	950241	38.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.36%
36) 1,2-Dichloropropane-d6	6.09	67	302812	37.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	75.34%
41) Toluene-d8	7.33	98	905462	39.75	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.50%#
43) trans-1,3-Dichloropropene-	7.64	79	162440	38.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.52%
47) 2-Hexanone-d5	8.11	63	284095	70.33	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	70.33%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	420396	37.29	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	74.58%
64) 1,2-Dichlorobenzene-d4	11.65	152	343114	39.99	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.98%#

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
51) Chlorobenzene	8.90	112	269554	16.015	ug/L	98
62) 1,3-Dichlorobenzene	11.21	146	21044	1.647	ug/L	96
63) 1,4-Dichlorobenzene	11.29	146	75489	5.846	ug/L	98
65) 1,2-Dichlorobenzene	11.67	146	705823	53.020	ug/L	99
68) 1,2,4-trichlorobenzene	13.29	180	82512	9.926	ug/L	99
70) 1,2,3-Trichlorobenzene	13.77	180	14530	1.697	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015115.D
Acq On : 24 Mar 2020 11:28
Operator : SY/MD
Sample : L1941-12DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0DC3DL

Manual Integrations
APPROVED

apatel
3/25/2020 4:52:40 PM

Quant Time: Mar 25 01:51:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 25 01:10:42 2020
Response via : Initial Calibration

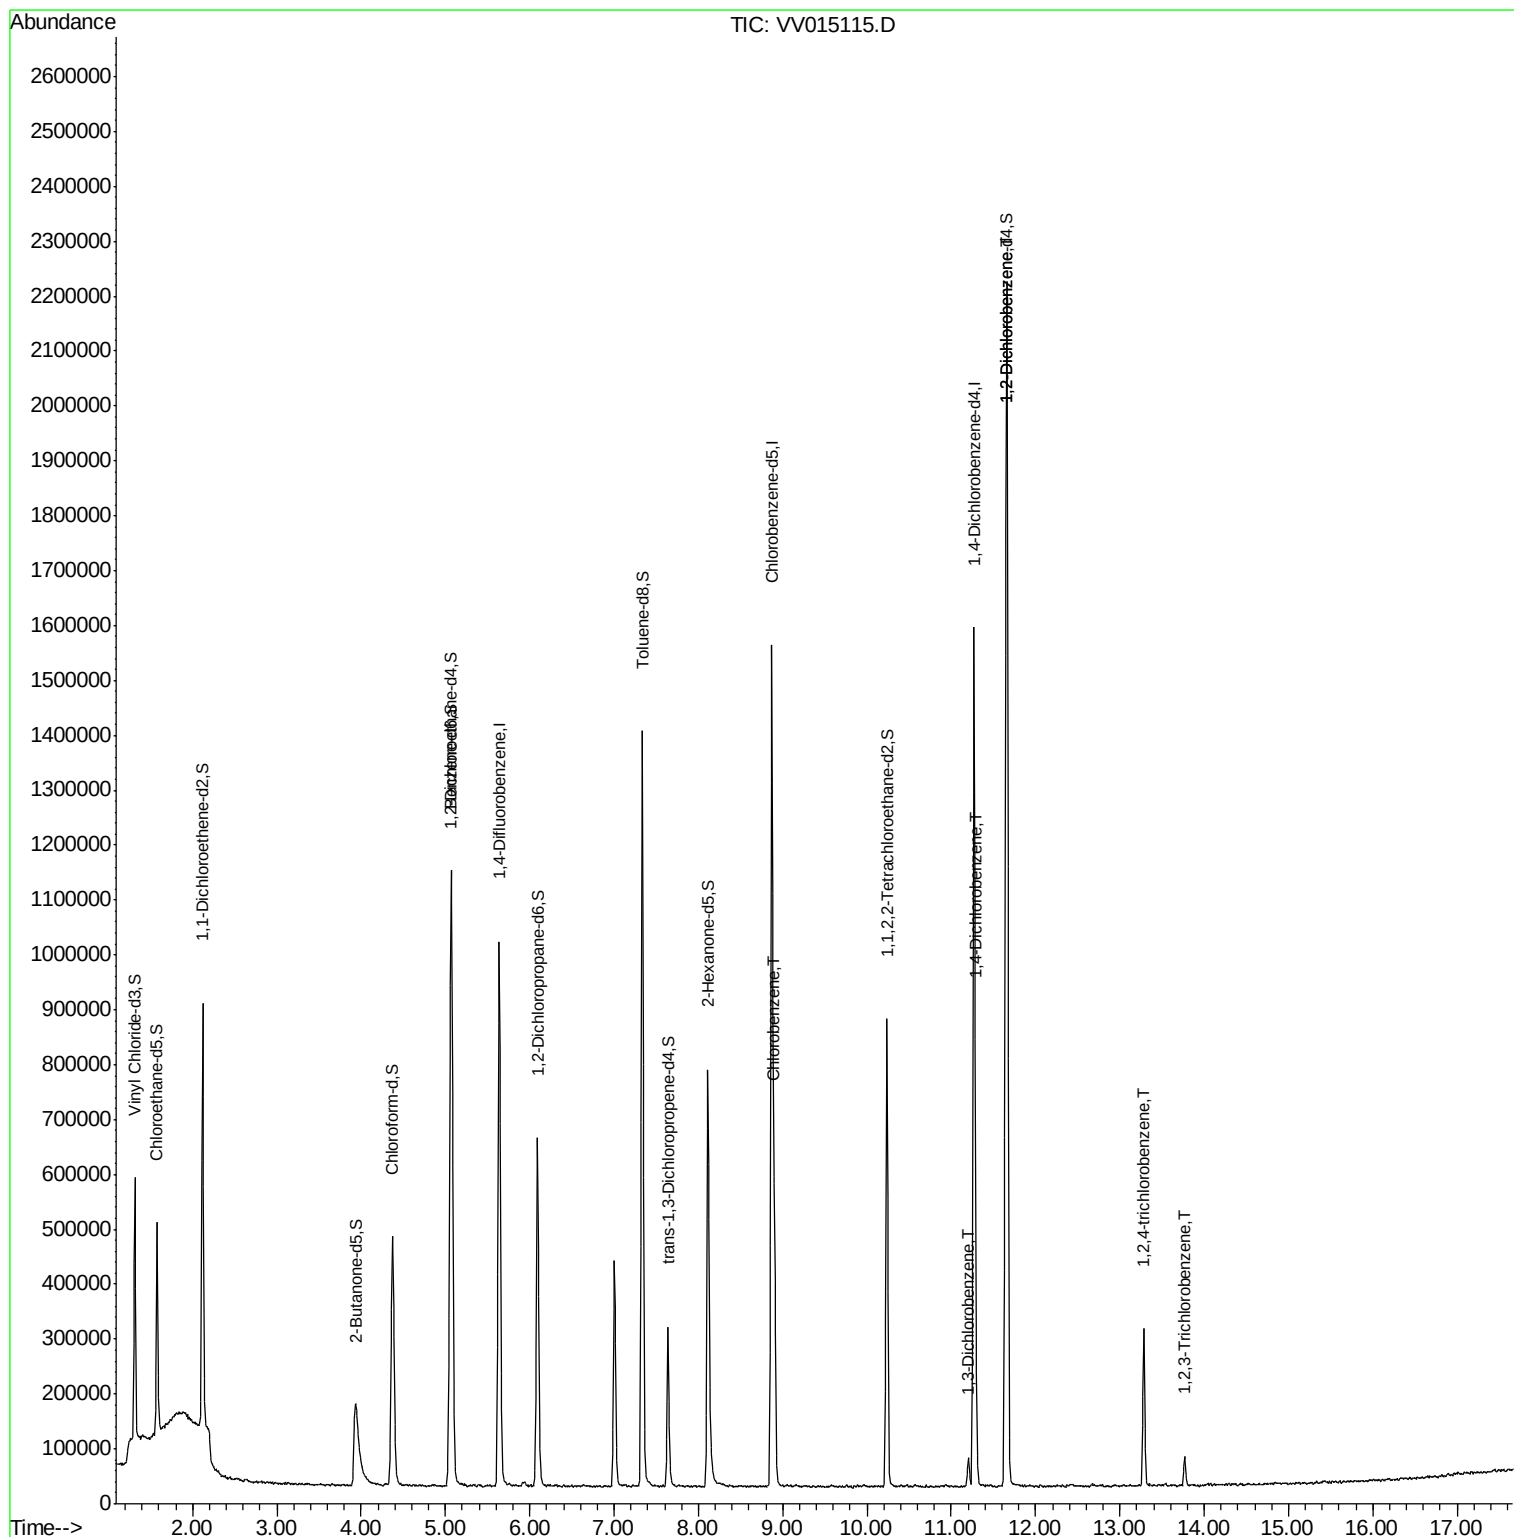

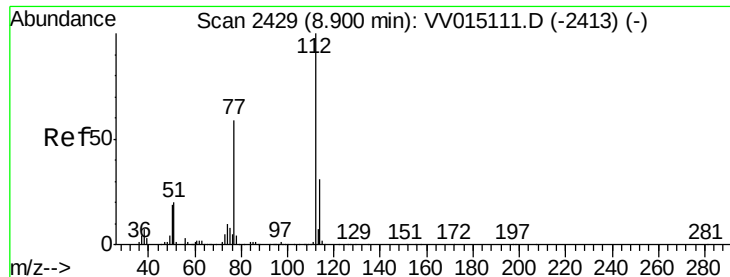

#51

Chlorobenzene

Concen: 16.015 ug/L

RT: 8.90 min Scan# 2429

Delta R.T. 0.00 min

Lab File: VV015115.D

Acq: 24 Mar 2020 11:28

Instrument :

MSVOA_V





ClientSampleId :

C0DC3DL

Tot Ion:	112	Resp:	269554
Ion Ratio		Lower	Upper
112	100		
114	31.3	22.3	41.3
77	57.8	48.1	72.1

Manual Integrations
APPROVED

apatel
3/25/2020 4:52:40 PM

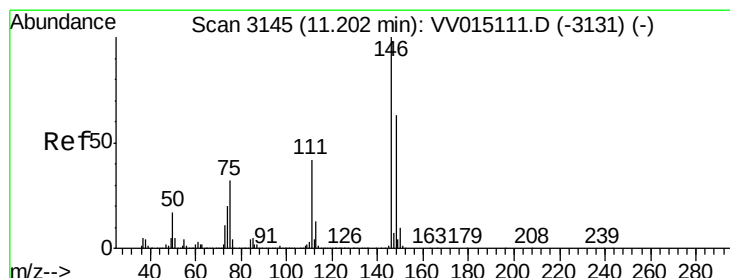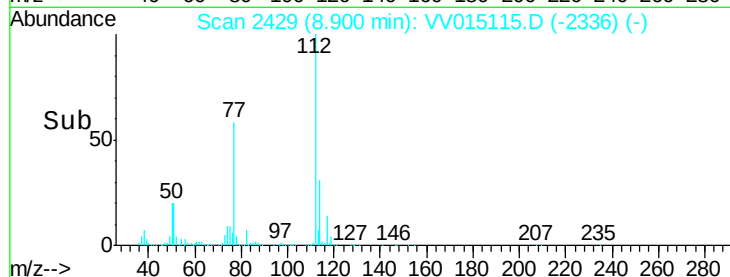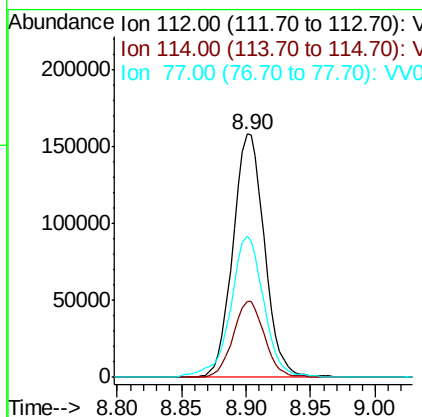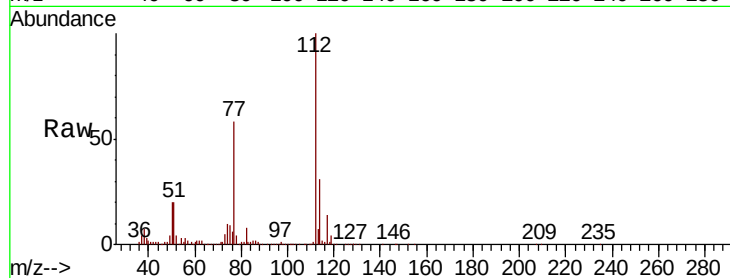

#62

1,3-Dichlorobenzene

Concen: 1.647 ug/L




RT: 11.21 min Scan# 3146


Delta R.T. 0.00 min

Lab File: VV015115.D

Acq: 24 Mar 2020 11:28

Tgt Ion:	146	Resp:	21044
Ion Ratio		Lower	Upper
146	100		
111	41.5	29.7	55.1
148	68.5	45.3	84.1

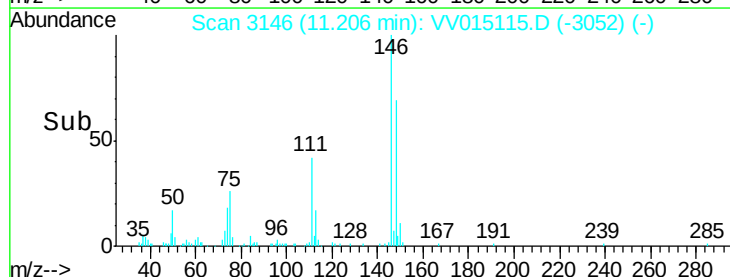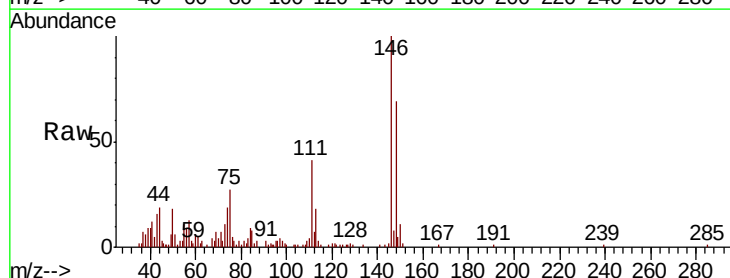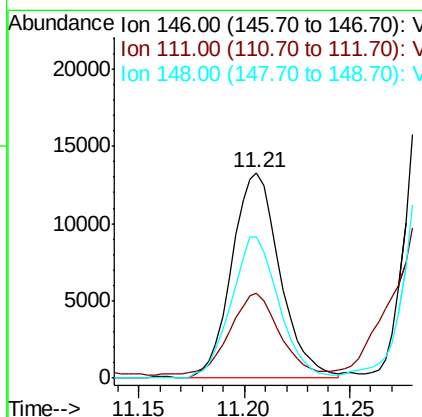

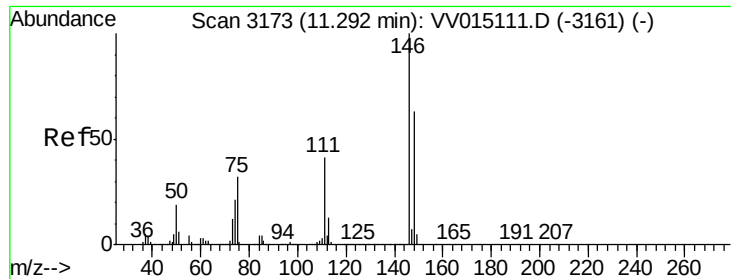





#63
 1,4-Dichlorobenzene
 Concen: 5.846 ug/L
 RT: 11.29 min Scan# 3173
 Delta R.T. 0.00 min
 Lab File: VV015115.D
 Acq: 24 Mar 2020 11:28

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC3DL

Tot Ion	Ratio	Lower	Upper
146	100		
111	39.5	28.2	52.4
148	62.6	44.9	83.5




Manual Integrations
 APPROVED


apatel
 3/25/2020 4:52:40 PM

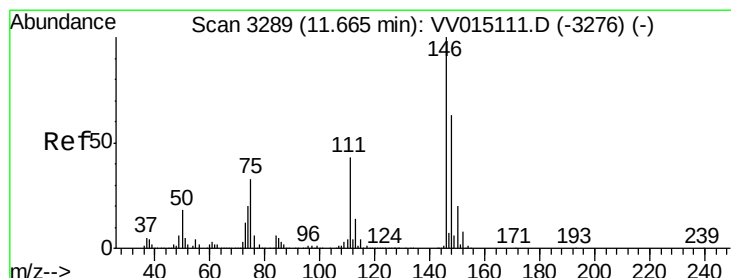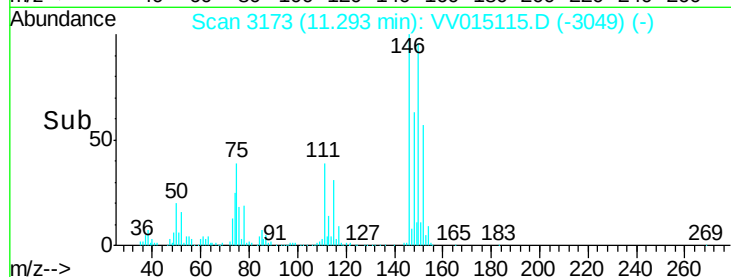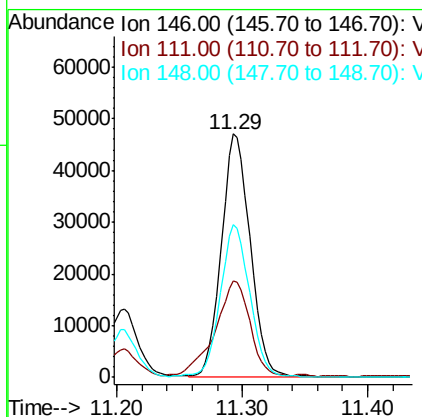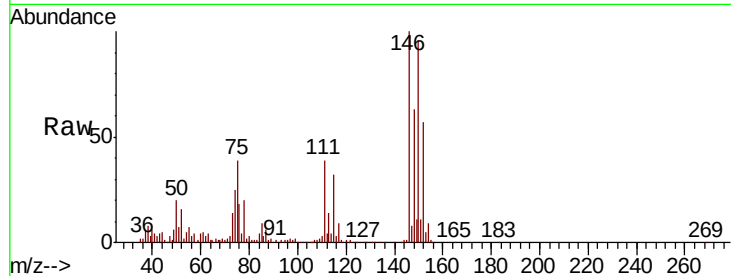

#65
 1,2-Dichlorobenzene
 Concen: 53.020 ug/L
 RT: 11.67 min Scan# 3289
 Delta R.T. 0.00 min
 Lab File: VV015115.D
 Acq: 24 Mar 2020 11:28

Tgt Ion	Ratio	Lower	Upper
146	100		
111	43.4	35.2	52.8
148	62.8	50.6	75.8

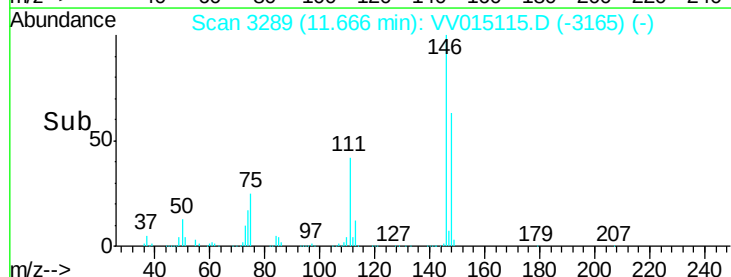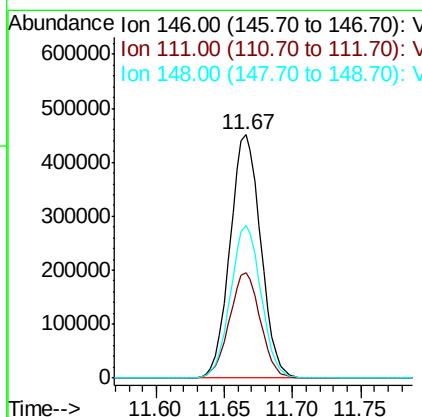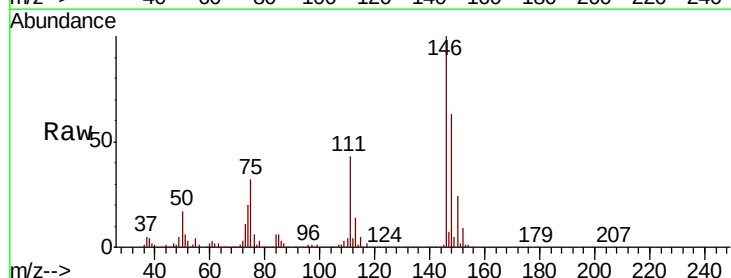

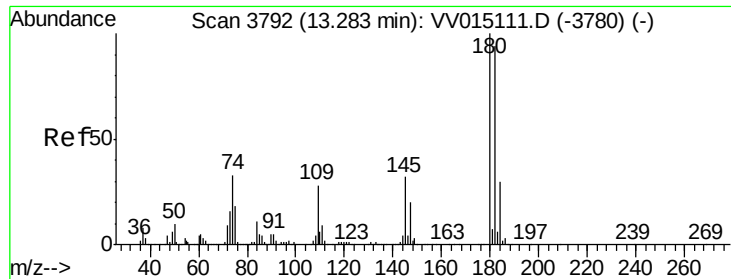





#68
 1,2,4-trichlorobenzene
 Concen: 9.926 ug/L
 RT: 13.29 min Scan# 3793
 Delta R.T. 0.00 min
 Lab File: VV015115.D
 Acq: 24 Mar 2020 11:28

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC3DL

Tot Ion	Ratio	Lower	Upper
180	100		
182	95.3	75.5	113.3
145	33.3	26.4	39.6

Manual Integrations
 APPROVED

apatel
 3/25/2020 4:52:40 PM

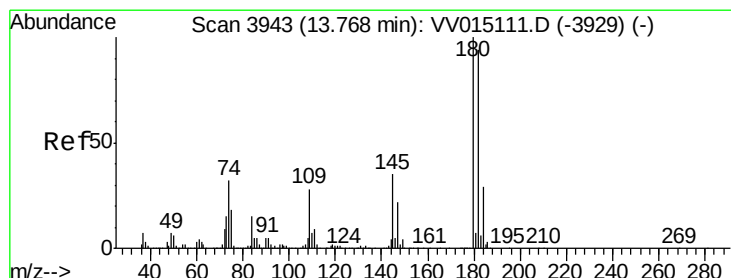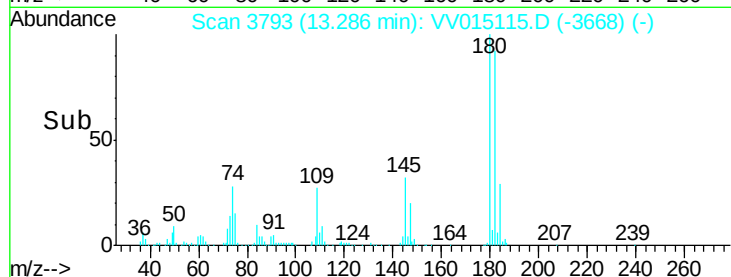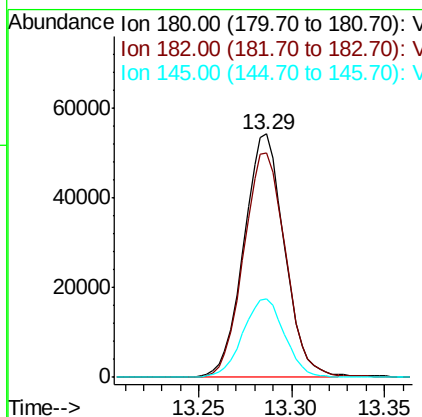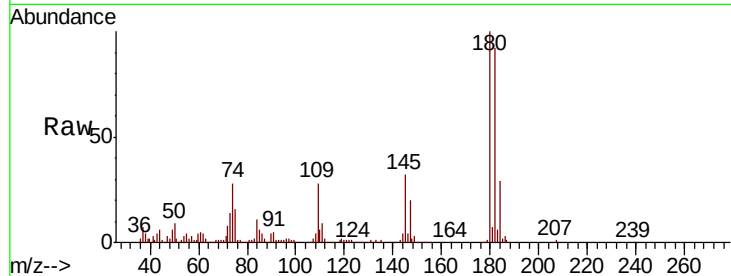

#70
 1,2,3-Trichlorobenzene
 Concen: 1.697 ug/L
 RT: 13.77 min Scan# 3943
 Delta R.T. 0.00 min
 Lab File: VV015115.D
 Acq: 24 Mar 2020 11:28

Tgt Ion	Ratio	Lower	Upper
180	100		
182	94.2	76.6	115.0
145	38.8	27.8	41.6

