

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015114.D
 Acq On : 24 Mar 2020 10:34
 Operator : SY/MD
 Sample : L1940-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	529303	521228	18.04%	2.161%
2	1.579	146	152	164	rBV	431780	488452	16.91%	2.025%
3	2.119	313	320	356	rVB	922753	1641099	56.81%	6.803%
4	3.688	804	808	811	rVB6	4186	3619	0.13%	0.015%
5	3.785	834	838	842	rBV7	2302	2099	0.07%	0.009%
6	3.939	873	886	936	rVV	160013	688195	23.82%	2.853%
7	4.380	1006	1023	1043	rBV	458898	1116978	38.67%	4.630%
8	4.518	1062	1066	1069	rVB5	3240	2573	0.09%	0.011%
9	4.537	1069	1072	1076	rVB5	3846	2778	0.10%	0.012%
10	4.563	1076	1080	1083	rVB4	3214	2218	0.08%	0.009%
11	4.595	1087	1090	1093	rBV5	3306	2287	0.08%	0.009%
12	4.749	1136	1138	1143	rVB6	2960	2076	0.07%	0.009%
13	4.913	1184	1189	1190	rBV4	2668	2344	0.08%	0.010%
14	5.074	1222	1239	1268	rVV2	1163382	2888759	100.00%	11.975%
15	5.286	1301	1305	1310	rBV8	2968	2725	0.09%	0.011%
16	5.312	1310	1313	1314	rBV2	3039	2025	0.07%	0.008%
17	5.479	1360	1365	1368	rBV6	2351	2454	0.08%	0.010%
18	5.499	1368	1371	1375	rVB5	3818	3167	0.11%	0.013%
19	5.643	1400	1416	1440	rBV	890528	1779646	61.61%	7.377%
20	5.811	1464	1468	1471	rBV6	3504	2911	0.10%	0.012%
21	5.878	1485	1489	1492	rBV5	2726	2540	0.09%	0.011%
22	5.907	1492	1498	1499	rVV6	3271	2942	0.10%	0.012%
23	5.930	1499	1505	1515	rVB6	7725	14980	0.52%	0.062%
24	5.997	1522	1526	1527	rBV3	3930	2942	0.10%	0.012%
25	6.097	1541	1557	1583	rVV2	644437	1323969	45.83%	5.488%
26	6.299	1616	1620	1624	rBV6	4322	3507	0.12%	0.015%
27	6.322	1624	1627	1631	rVV6	4530	3475	0.12%	0.014%
28	6.344	1631	1634	1636	rVV4	2787	2198	0.08%	0.009%
29	6.357	1636	1638	1643	rVB5	4296	2834	0.10%	0.012%
30	6.393	1643	1649	1650	rBV6	2364	2252	0.08%	0.009%
31	6.421	1654	1658	1661	rBV5	2352	2393	0.08%	0.010%
32	6.499	1677	1682	1685	rBV6	3393	3872	0.13%	0.016%
33	6.737	1751	1756	1757	rBV5	2701	2335	0.08%	0.010%
34	6.865	1791	1796	1800	rVB8	3963	4011	0.14%	0.017%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015114.D
 Acq On : 24 Mar 2020 10:34
 Operator : SY/MD
 Sample : L1940-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

35	6.894	1800	1805	1807	rBV6	3952	3319	0.11%	0.014%
36	6.968	1820	1828	1829	rBV9	2870	2735	0.09%	0.011%
37	7.007	1829	1840	1862	rVV	416302	755213	26.14%	3.131%
38	7.177	1891	1893	1898	rBV5	2327	2370	0.08%	0.010%
39	7.338	1930	1943	1968	rBV	1443102	2501198	86.58%	10.369%
40	7.582	2015	2019	2021	rBV5	3249	2139	0.07%	0.009%
41	7.643	2027	2038	2053	rBV	305340	511267	17.70%	2.119%
42	7.753	2070	2072	2077	rVB6	3594	2209	0.08%	0.009%
43	7.788	2077	2083	2085	rBV6	3136	2063	0.07%	0.009%
44	7.804	2085	2088	2090	rBV3	2751	1973	0.07%	0.008%
45	7.843	2097	2100	2103	rVB5	3961	2936	0.10%	0.012%
46	7.894	2110	2116	2118	rBV7	3585	3064	0.11%	0.013%
47	7.910	2118	2121	2124	rBV4	2618	2076	0.07%	0.009%
48	8.045	2159	2163	2166	rVB5	4499	3691	0.13%	0.015%
49	8.068	2166	2170	2172	rBV5	4623	3644	0.13%	0.015%
50	8.116	2173	2185	2214	rVV	841919	1663204	57.58%	6.895%
51	8.698	2357	2366	2368	rBV9	3054	3824	0.13%	0.016%
52	8.875	2409	2421	2441	rVV	1352964	2214462	76.66%	9.180%
53	8.984	2451	2455	2456	rBV4	3619	2629	0.09%	0.011%
54	9.026	2464	2468	2471	rBV5	4545	3437	0.12%	0.014%
55	9.338	2561	2565	2569	rBV7	2838	2415	0.08%	0.010%
56	9.383	2575	2579	2581	rBV5	3336	2744	0.09%	0.011%
57	9.743	2688	2691	2695	rVB5	3872	2647	0.09%	0.011%
58	9.833	2717	2719	2723	rVB5	3314	2217	0.08%	0.009%
59	9.855	2723	2726	2730	rBV5	3129	2377	0.08%	0.010%
60	9.897	2733	2739	2744	rBV9	6109	8558	0.30%	0.035%
61	9.958	2754	2758	2761	rBV7	3841	3449	0.12%	0.014%
62	10.097	2796	2801	2804	rBV6	2898	2164	0.07%	0.009%
63	10.167	2815	2823	2824	rVV7	2844	2877	0.10%	0.012%
64	10.238	2827	2845	2863	rBV	907522	1429649	49.49%	5.927%
65	10.389	2888	2892	2895	rVV6	2831	1990	0.07%	0.008%
66	10.569	2938	2948	2951	rBV6	3957	5689	0.20%	0.024%
67	10.617	2960	2963	2969	rVB7	3259	2988	0.10%	0.012%
68	10.743	2997	3002	3005	rBV7	2892	3148	0.11%	0.013%
69	10.804	3017	3021	3025	rBV7	2450	2048	0.07%	0.008%
70	11.000	3078	3082	3086	rBV7	2799	2299	0.08%	0.010%
71	11.071	3100	3104	3109	rVB7	2978	2691	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015114.D
 Acq On : 24 Mar 2020 10:34
 Operator : SY/MD
 Sample : L1940-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

72	11.187	3137	3140	3142	rBV4	3732	2755	0.10%	0.011%
73	11.270	3154	3166	3183	rBV	1392765	2132706	73.83%	8.841%
74	11.424	3210	3214	3216	rBV4	2605	1923	0.07%	0.008%
75	11.441	3216	3219	3222	rVB5	4527	2716	0.09%	0.011%
76	11.476	3227	3230	3234	rBV6	3401	2609	0.09%	0.011%
77	11.527	3243	3246	3250	rVB6	2705	2116	0.07%	0.009%
78	11.556	3250	3255	3257	rBV6	3003	2920	0.10%	0.012%
79	11.646	3269	3283	3299	rVV	1432537	2200371	76.17%	9.122%
80	11.884	3353	3357	3358	rBV4	2858	2089	0.07%	0.009%
81	11.900	3360	3362	3370	rVB8	4733	4331	0.15%	0.018%
82	12.048	3405	3408	3412	rVB6	2629	2091	0.07%	0.009%
83	12.084	3412	3419	3422	rBV8	4169	4268	0.15%	0.018%
84	12.228	3460	3464	3466	rBV5	3061	2467	0.09%	0.010%
85	12.277	3472	3479	3483	rBV9	4990	6422	0.22%	0.027%
86	12.383	3507	3512	3518	rBV9	3338	4276	0.15%	0.018%
87	12.495	3546	3547	3551	rVB4	3589	1933	0.07%	0.008%
88	12.621	3581	3586	3588	rVV6	2216	1903	0.07%	0.008%
89	12.704	3609	3612	3616	rVB6	2917	2112	0.07%	0.009%
90	12.849	3650	3657	3659	rBV7	2390	3048	0.11%	0.013%
91	13.103	3731	3736	3739	rBV6	2696	2790	0.10%	0.012%
92	13.222	3771	3773	3779	rVB6	2824	2672	0.09%	0.011%
93	13.289	3784	3794	3801	rBV6	10594	18470	0.64%	0.077%
94	13.418	3831	3834	3836	rBV4	2751	1984	0.07%	0.008%
95	13.672	3910	3913	3918	rBV6	2704	2554	0.09%	0.011%
96	13.765	3939	3942	3943	rBV3	3574	2095	0.07%	0.009%
97	13.910	3984	3987	3992	rVB7	2698	2351	0.08%	0.010%
98	14.039	4022	4027	4029	rBV5	3138	3475	0.12%	0.014%
99	14.231	4084	4087	4090	rBV5	3473	2006	0.07%	0.008%
100	14.514	4172	4175	4177	rBV4	3342	1965	0.07%	0.008%


Sum of corrected areas: 24122704

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015114.D
Acq On : 24 Mar 2020 10:34
Operator : SY/MD
Sample : L1940-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

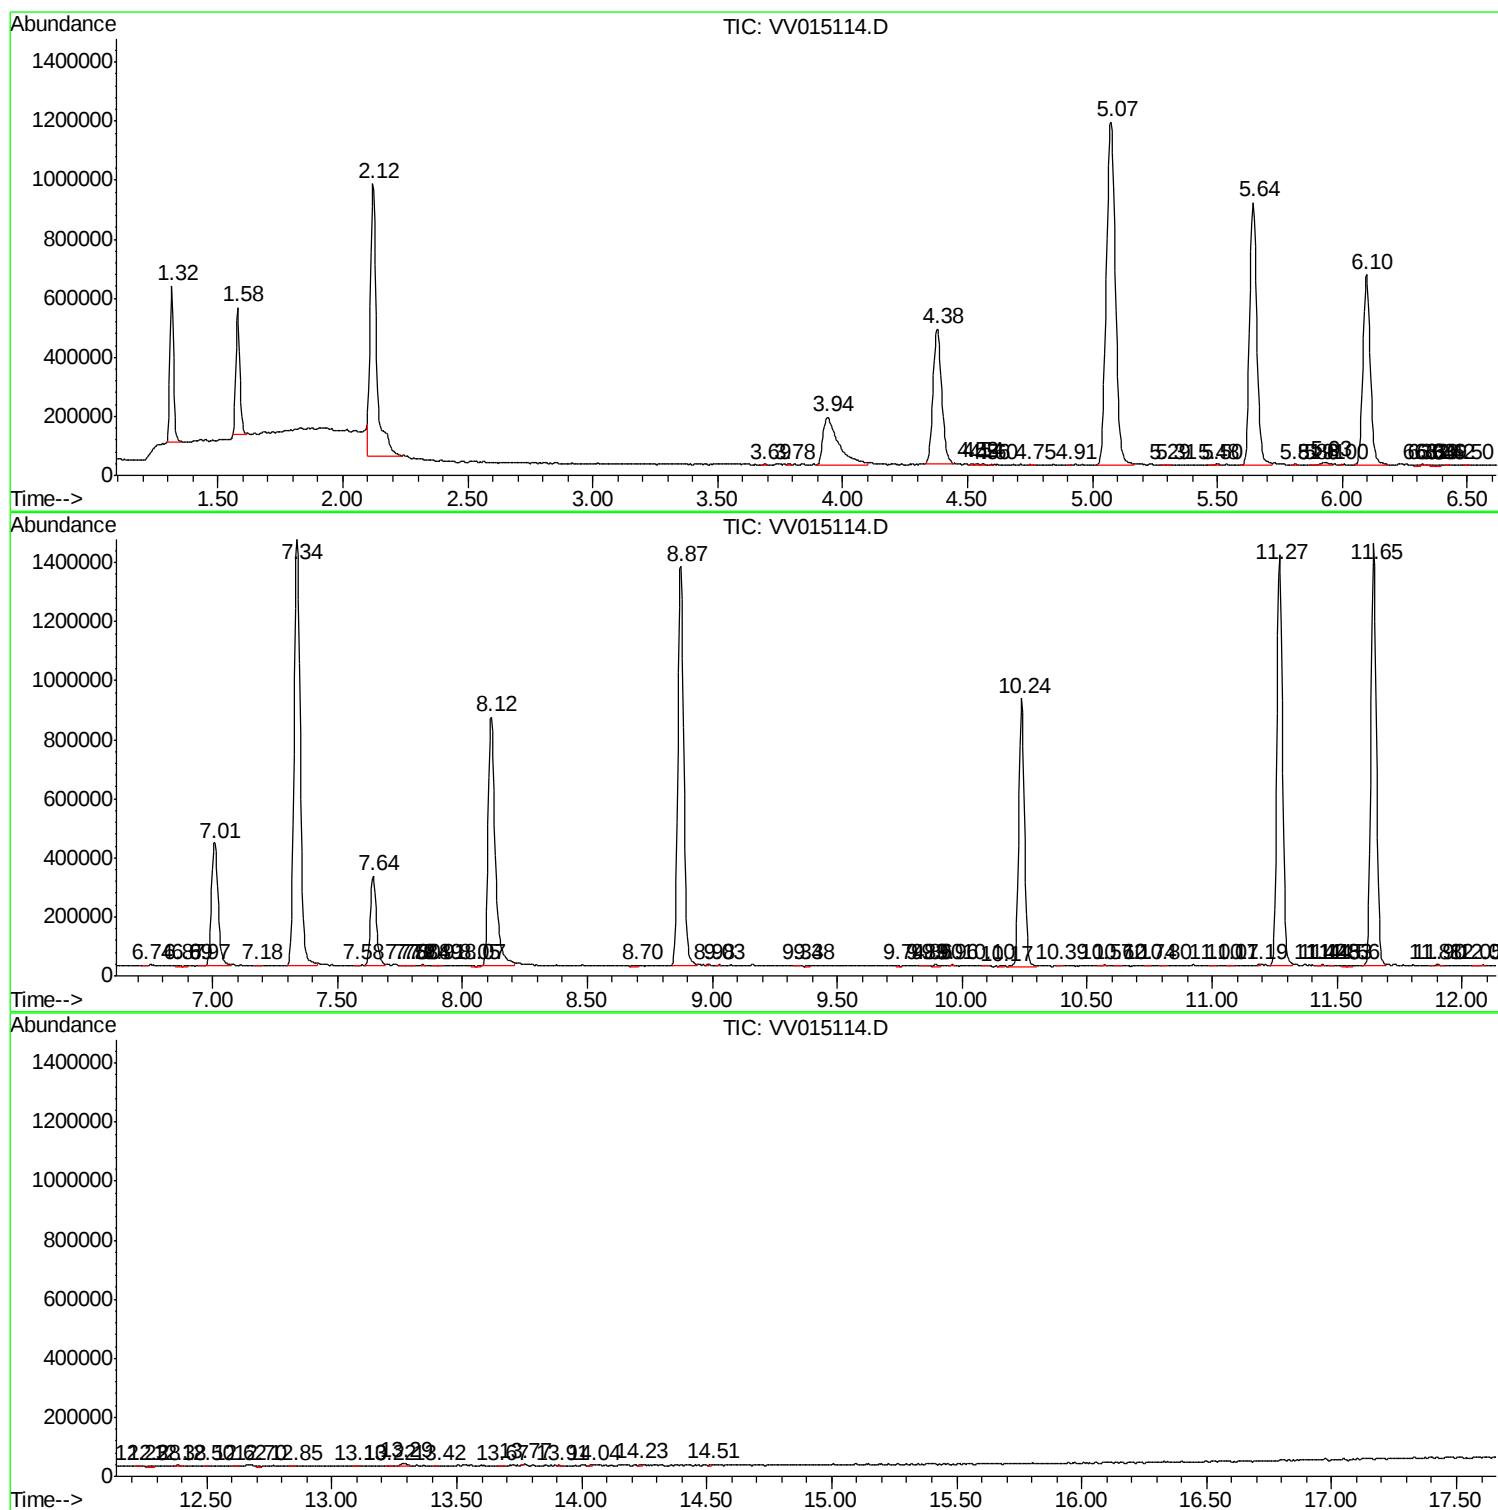

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032420\
Data File : VV015114.D
Acq On : 24 Mar 2020 10:34
Operator : SY/MD
Sample : L1940-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032420\
Data File : VV015114.D
Acq On : 24 Mar 2020 10:34
Operator : SY/MD
Sample : L1940-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc