

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015115.D
 Acq On : 24 Mar 2020 11:28
 Operator : SY/MD
 Sample : L1941-12DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	80	rVB	470871	473531	9.53%	1.685%
2	1.579	146	152	165	rVB	377916	457819	9.21%	1.630%
3	2.119	312	320	341	rVB	776876	1122414	22.59%	3.995%
4	3.132	632	635	639	rBV6	3806	3166	0.06%	0.011%
5	3.222	659	663	667	rVB7	3577	3047	0.06%	0.011%
6	3.743	822	825	828	rBV5	2929	2253	0.05%	0.008%
7	3.824	847	850	854	rBV5	3265	2881	0.06%	0.010%
8	3.936	871	885	927	rVV2	148060	652008	13.12%	2.321%
9	4.283	987	993	995	rBV6	4099	4426	0.09%	0.016%
10	4.373	1004	1021	1047	rBV	452179	1102930	22.20%	3.926%
11	4.531	1065	1070	1077	rBV10	4029	5306	0.11%	0.019%
12	4.569	1080	1082	1087	rBV5	3073	2429	0.05%	0.009%
13	4.611	1091	1095	1098	rBV6	2840	2613	0.05%	0.009%
14	4.653	1105	1108	1112	rBV5	2470	2063	0.04%	0.007%
15	4.762	1140	1142	1146	rVB4	4075	2775	0.06%	0.010%
16	4.782	1146	1148	1151	rBV4	4025	2954	0.06%	0.011%
17	4.846	1160	1168	1172	rBV10	3372	5058	0.10%	0.018%
18	5.068	1217	1237	1262	rBV2	1121542	2786217	56.08%	9.917%
19	5.229	1284	1287	1290	rBV5	3036	2047	0.04%	0.007%
20	5.637	1400	1414	1432	rBV	992486	1961915	39.49%	6.983%
21	5.917	1494	1501	1503	rBV7	5852	6389	0.13%	0.023%
22	6.090	1542	1555	1576	rBV	634135	1265825	25.48%	4.506%
23	6.216	1588	1594	1596	rBV7	3490	3594	0.07%	0.013%
24	6.402	1648	1652	1653	rBV4	3325	2168	0.04%	0.008%
25	6.441	1660	1664	1666	rBV4	3006	1990	0.04%	0.007%
26	6.486	1674	1678	1680	rBV4	2430	1995	0.04%	0.007%
27	6.499	1680	1682	1686	rVB5	4924	3094	0.06%	0.011%
28	6.531	1686	1692	1695	rBV7	3391	3869	0.08%	0.014%
29	6.753	1756	1761	1765	rVB8	2747	2053	0.04%	0.007%
30	6.798	1769	1775	1777	rBV6	3213	3192	0.06%	0.011%
31	6.875	1793	1799	1802	rBV7	3105	3706	0.07%	0.013%
32	7.007	1829	1840	1857	rVV	409459	724438	14.58%	2.579%
33	7.225	1903	1908	1912	rBV7	2747	3045	0.06%	0.011%
34	7.335	1929	1942	1964	rBV	1375432	2380764	47.92%	8.474%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015115.D
 Acq On : 24 Mar 2020 11:28
 Operator : SY/MD
 Sample : L1941-12DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

35	7.582	2016	2019	2024	rVB7	2836	2290	0.05%	0.008%
36	7.640	2024	2037	2049	rBV	291417	492732	9.92%	1.754%
37	7.814	2088	2091	2096	rVB7	2280	2051	0.04%	0.007%
38	7.955	2130	2135	2138	rVV7	2792	3398	0.07%	0.012%
39	8.113	2170	2184	2218	rBV	760240	1542225	31.04%	5.489%
40	8.338	2252	2254	2259	rVB6	2660	2562	0.05%	0.009%
41	8.367	2259	2263	2265	rBV4	3578	2658	0.05%	0.009%
42	8.418	2275	2279	2282	rBV5	2146	2102	0.04%	0.007%
43	8.544	2316	2318	2326	rVB8	2914	2671	0.05%	0.010%
44	8.601	2333	2336	2341	rVB7	2187	2212	0.04%	0.008%
45	8.720	2368	2373	2376	rBV8	2829	3127	0.06%	0.011%
46	8.791	2392	2395	2399	rVB6	3009	2543	0.05%	0.009%
47	8.814	2399	2402	2403	rBV3	3578	2308	0.05%	0.008%
48	8.872	2408	2420	2449	rVV2	1533061	3257059	65.55%	11.593%
49	9.100	2489	2491	2495	rVB5	3703	2199	0.04%	0.008%
50	9.135	2498	2502	2505	rBV5	3829	3898	0.08%	0.014%
51	9.158	2507	2509	2513	rVB5	3364	1918	0.04%	0.007%
52	9.302	2552	2554	2564	rVB10	3319	3886	0.08%	0.014%
53	9.415	2585	2589	2590	rBV3	2450	1905	0.04%	0.007%
54	9.756	2685	2695	2697	rBV10	3901	4693	0.09%	0.017%
55	9.823	2714	2716	2719	rVB4	3040	1876	0.04%	0.007%
56	9.839	2719	2721	2723	rBV3	3365	2132	0.04%	0.008%
57	9.888	2732	2736	2739	rBV4	3669	2576	0.05%	0.009%
58	9.962	2755	2759	2761	rBV5	2489	1781	0.04%	0.006%
59	10.013	2771	2775	2778	rVB5	3194	2527	0.05%	0.009%
60	10.132	2809	2812	2818	rVB7	1970	1847	0.04%	0.007%
61	10.238	2833	2845	2864	rVV	852360	1364857	27.47%	4.858%
62	10.402	2894	2896	2903	rVB8	2886	2717	0.05%	0.010%
63	10.505	2926	2928	2933	rBV6	3160	2060	0.04%	0.007%
64	10.553	2939	2943	2944	rBV3	3779	2745	0.06%	0.010%
65	10.653	2971	2974	2977	rBV4	2815	1875	0.04%	0.007%
66	10.701	2985	2989	2996	rVB8	4894	4350	0.09%	0.015%
67	10.749	3000	3004	3008	rVV7	2966	2372	0.05%	0.008%
68	11.113	3114	3117	3120	rBV4	2567	1813	0.04%	0.006%
69	11.203	3135	3145	3155	rVV	52579	86283	1.74%	0.307%
70	11.270	3155	3166	3192	rVB	1563129	2678029	53.90%	9.532%
71	11.408	3206	3209	3213	rBV5	2572	2066	0.04%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015115.D
 Acq On : 24 Mar 2020 11:28
 Operator : SY/MD
 Sample : L1941-12DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

72	11.553	3249	3254	3257	rBV7	2596	2484	0.05%	0.009%
73	11.659	3270	3287	3310	rBV2	2194346	4968498	100.00%	17.685%
74	11.842	3342	3344	3348	rVB5	3303	2107	0.04%	0.007%
75	11.868	3348	3352	3356	rBV6	3536	3303	0.07%	0.012%
76	12.045	3404	3407	3410	rBV5	3485	2570	0.05%	0.009%
77	12.061	3410	3412	3418	rVB7	4272	3847	0.08%	0.014%
78	12.100	3421	3424	3431	rVB8	3184	3921	0.08%	0.014%
79	12.142	3431	3437	3440	rBV7	3125	3190	0.06%	0.011%
80	12.167	3440	3445	3448	rBV6	3408	2472	0.05%	0.009%
81	12.183	3448	3450	3455	rBV5	2562	2124	0.04%	0.008%
82	12.212	3455	3459	3466	rVB9	2575	2558	0.05%	0.009%
83	12.257	3470	3473	3476	rBV4	2204	1939	0.04%	0.007%
84	12.315	3488	3491	3494	rBV4	3209	2408	0.05%	0.009%
85	12.370	3503	3508	3510	rBV5	3423	2950	0.06%	0.011%
86	12.592	3573	3577	3581	rVV7	2636	2177	0.04%	0.008%
87	12.624	3581	3587	3590	rVB8	2938	2838	0.06%	0.010%
88	12.662	3590	3599	3600	rBV9	5363	5648	0.11%	0.020%
89	12.791	3636	3639	3645	rVB8	3391	3423	0.07%	0.012%
90	12.910	3670	3676	3677	rBV5	2114	1990	0.04%	0.007%
91	13.035	3712	3715	3717	rBV4	3026	2146	0.04%	0.008%
92	13.283	3778	3792	3812	rBV	286744	457434	9.21%	1.628%
93	13.354	3812	3814	3822	rVB8	4038	3253	0.07%	0.012%
94	13.521	3864	3866	3870	rBV5	2203	2273	0.05%	0.008%
95	13.768	3934	3943	3955	rBV2	54534	89842	1.81%	0.320%
96	13.842	3963	3966	3970	rBV6	2790	2528	0.05%	0.009%
97	14.106	4044	4048	4051	rBV6	2532	2377	0.05%	0.008%
98	14.331	4112	4118	4123	rBV9	3361	4716	0.09%	0.017%
99	14.482	4163	4165	4168	rBV4	2778	1835	0.04%	0.007%
100	15.154	4371	4374	4377	rBV4	4620	3889	0.08%	0.014%


Sum of corrected areas: 28095057

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015115.D
Acq On : 24 Mar 2020 11:28
Operator : SY/MD
Sample : L1941-12DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0DC3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

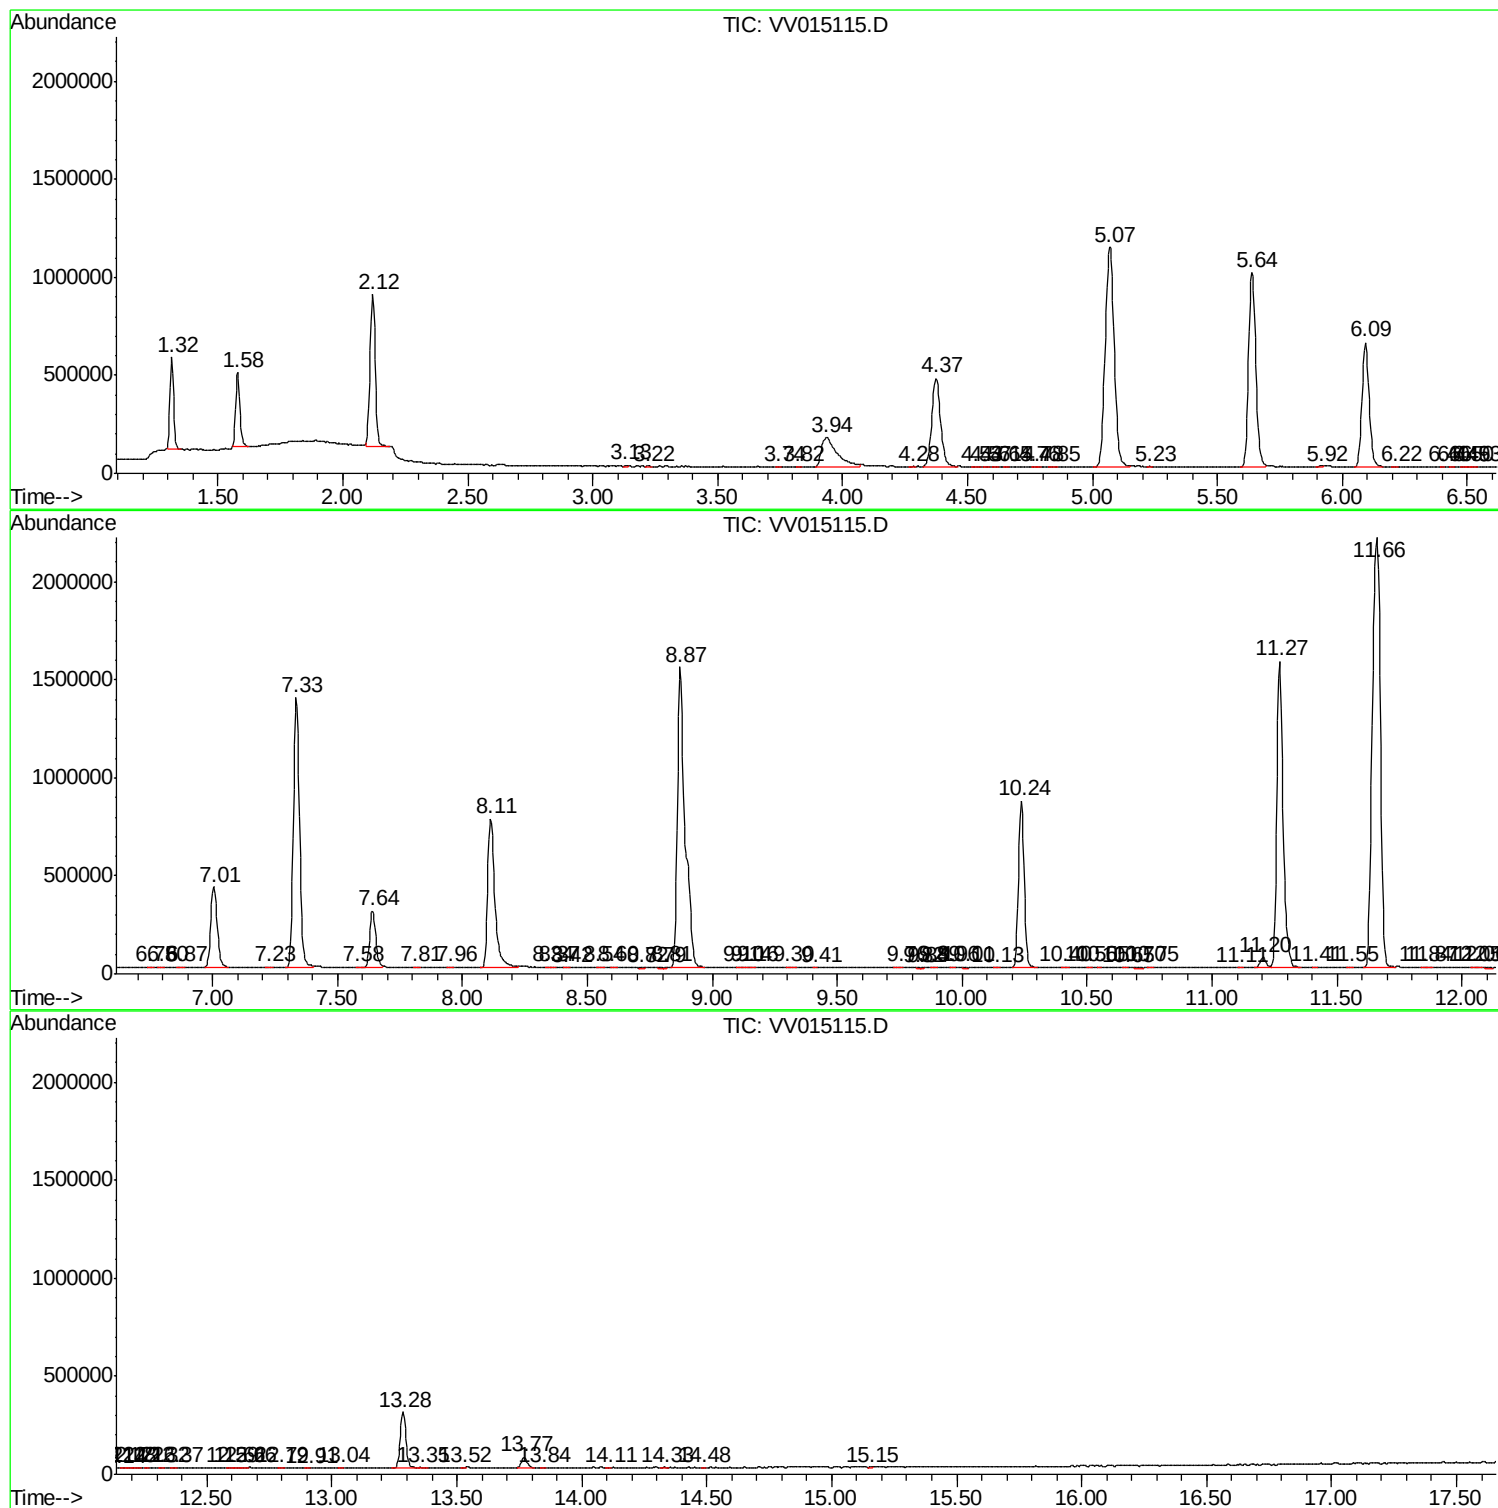

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032420\
Data File : VV015115.D
Acq On : 24 Mar 2020 11:28
Operator : SY/MD
Sample : L1941-12DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032420\
Data File : VV015115.D
Acq On : 24 Mar 2020 11:28
Operator : SY/MD
Sample : L1941-12DL 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DC3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
