

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015117.D
 Acq On : 24 Mar 2020 12:35
 Operator : SY/MD
 Sample : L1941-17DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	83	rVB	495021	476207	4.18%	1.200%
2	1.579	147	152	164	rVB	411367	463153	4.06%	1.167%
3	3.936	873	885	922	rBV2	161463	640354	5.62%	1.613%
4	4.261	983	986	990	rBV5	3922	2746	0.02%	0.007%
5	4.380	1009	1023	1046	rVB	457954	1114531	9.78%	2.808%
6	4.544	1071	1074	1080	rBV8	2999	2873	0.03%	0.007%
7	5.074	1222	1239	1249	rBV2	1150723	2911810	25.55%	7.336%
8	5.360	1326	1328	1330	rBV3	1857	893	0.01%	0.002%
9	5.434	1347	1351	1353	rBV4	2216	1802	0.02%	0.005%
10	5.447	1353	1355	1359	rBV4	2752	2458	0.02%	0.006%
11	5.643	1403	1416	1438	rBV	882659	1738473	15.25%	4.380%
12	6.010	1527	1530	1533	rBV5	3600	2784	0.02%	0.007%
13	6.097	1544	1557	1580	rVB	658682	1302284	11.43%	3.281%
14	6.402	1650	1652	1657	rVB5	2382	1796	0.02%	0.005%
15	6.434	1660	1662	1667	rBV7	2218	1441	0.01%	0.004%
16	6.466	1669	1672	1674	rBV4	2145	1397	0.01%	0.004%
17	6.550	1694	1698	1703	rBV7	3008	3180	0.03%	0.008%
18	6.579	1705	1707	1709	rVB3	1466	477	0.00%	0.001%
19	6.595	1709	1712	1713	rBV3	1857	1059	0.01%	0.003%
20	6.778	1766	1769	1770	rBV3	1852	866	0.01%	0.002%
21	6.788	1770	1772	1775	rVV4	2364	1518	0.01%	0.004%
22	7.006	1828	1840	1863	rBV	426552	765598	6.72%	1.929%
23	7.338	1928	1943	1966	rBV	1436786	2514409	22.06%	6.335%
24	7.489	1985	1990	1992	rBV5	3032	2738	0.02%	0.007%
25	7.543	2004	2007	2008	rBV3	2477	1505	0.01%	0.004%
26	7.643	2028	2038	2061	rVB	299359	512544	4.50%	1.291%
27	7.862	2104	2106	2107	rBV2	1921	925	0.01%	0.002%
28	8.113	2174	2184	2213	rBV	827726	1629304	14.29%	4.105%
29	8.534	2310	2315	2317	rVB5	2282	1743	0.02%	0.004%
30	8.810	2399	2401	2405	rBV5	2404	1698	0.01%	0.004%
31	8.875	2407	2421	2423	rBV	1477075	1879429	16.49%	4.735%
32	9.257	2538	2540	2541	rBV2	1923	706	0.01%	0.002%
33	9.363	2571	2573	2576	rVB4	1987	953	0.01%	0.002%
34	9.421	2590	2591	2594	rVB3	1944	898	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015117.D
 Acq On : 24 Mar 2020 12:35
 Operator : SY/MD
 Sample : L1941-17DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

35	9.437	2594	2596	2597	rBV2	1789	761	0.01%	0.002%
36	9.511	2616	2619	2620	rBV3	2758	1377	0.01%	0.003%
37	9.643	2657	2660	2663	rVB5	2047	1303	0.01%	0.003%
38	9.688	2671	2674	2676	rBV4	2868	2156	0.02%	0.005%
39	9.739	2687	2690	2694	rVB6	4045	2870	0.03%	0.007%
40	9.772	2697	2700	2702	rBV3	2708	1681	0.01%	0.004%
41	9.810	2706	2712	2715	rBV8	3293	4029	0.04%	0.010%
42	9.829	2715	2718	2720	rBV4	2288	1611	0.01%	0.004%
43	9.874	2730	2732	2734	rVB3	1185	428	0.00%	0.001%
44	9.916	2743	2745	2749	rVB5	2617	1517	0.01%	0.004%
45	9.955	2754	2757	2762	rBV7	3006	2526	0.02%	0.006%
46	10.003	2767	2772	2775	rBV7	3212	2718	0.02%	0.007%
47	10.026	2777	2779	2784	rVB5	1896	1309	0.01%	0.003%
48	10.080	2793	2796	2800	rVB5	2449	1806	0.02%	0.005%
49	10.141	2814	2815	2817	rBV2	1230	442	0.00%	0.001%
50	10.196	2828	2832	2833	rBV4	2560	1772	0.02%	0.004%
51	10.238	2834	2845	2861	rVV	931760	1438438	12.62%	3.624%
52	10.366	2882	2885	2888	rBV4	1577	1201	0.01%	0.003%
53	10.431	2902	2905	2908	rVB4	1992	1001	0.01%	0.003%
54	10.456	2908	2913	2916	rBV7	3799	4144	0.04%	0.010%
55	10.643	2968	2971	2973	rBV4	1434	1007	0.01%	0.003%
56	10.704	2984	2990	2993	rBV7	4076	4374	0.04%	0.011%
57	10.720	2993	2995	2996	rBV2	2176	964	0.01%	0.002%
58	10.974	3072	3074	3076	rBV3	2883	1570	0.01%	0.004%
59	11.067	3100	3103	3105	rBV4	2422	1694	0.01%	0.004%
60	11.138	3123	3125	3127	rBV3	2034	1217	0.01%	0.003%
61	11.202	3135	3145	3155	rBV	295670	458126	4.02%	1.154%
62	11.292	3156	3173	3197	rVB2	4009472	8088157	70.96%	20.377%
63	11.665	3272	3289	3310	rBV2	6239363	11398280	100.00%	28.716%
64	12.029	3399	3402	3405	rBV4	2690	1983	0.02%	0.005%
65	12.087	3418	3420	3425	rBV5	2736	2359	0.02%	0.006%
66	12.190	3448	3452	3456	rBV7	2849	2481	0.02%	0.006%
67	12.354	3494	3503	3506	rBV8	4014	4965	0.04%	0.013%
68	12.460	3534	3536	3537	rBV2	1994	941	0.01%	0.002%
69	12.932	3681	3683	3686	rBV3	2153	974	0.01%	0.002%
70	12.958	3688	3691	3695	rVB5	3237	1989	0.02%	0.005%
71	13.122	3740	3742	3745	rBV4	2156	1152	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015117.D
Acq On : 24 Mar 2020 12:35
Operator : SY/MD
Sample : L1941-17DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL7DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Title : VOC Analysis

72	13.228	3774	3775	3776	rBV	1266	403	0.00%	0.001%
73	13.283	3776	3792	3815	rVV	1178451	1840367	16.15%	4.636%
74	13.768	3933	3943	3956	rBV	273696	422545	3.71%	1.065%


Sum of corrected areas: 39693190

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015117.D
Acq On : 24 Mar 2020 12:35
Operator : SY/MD
Sample : L1941-17DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

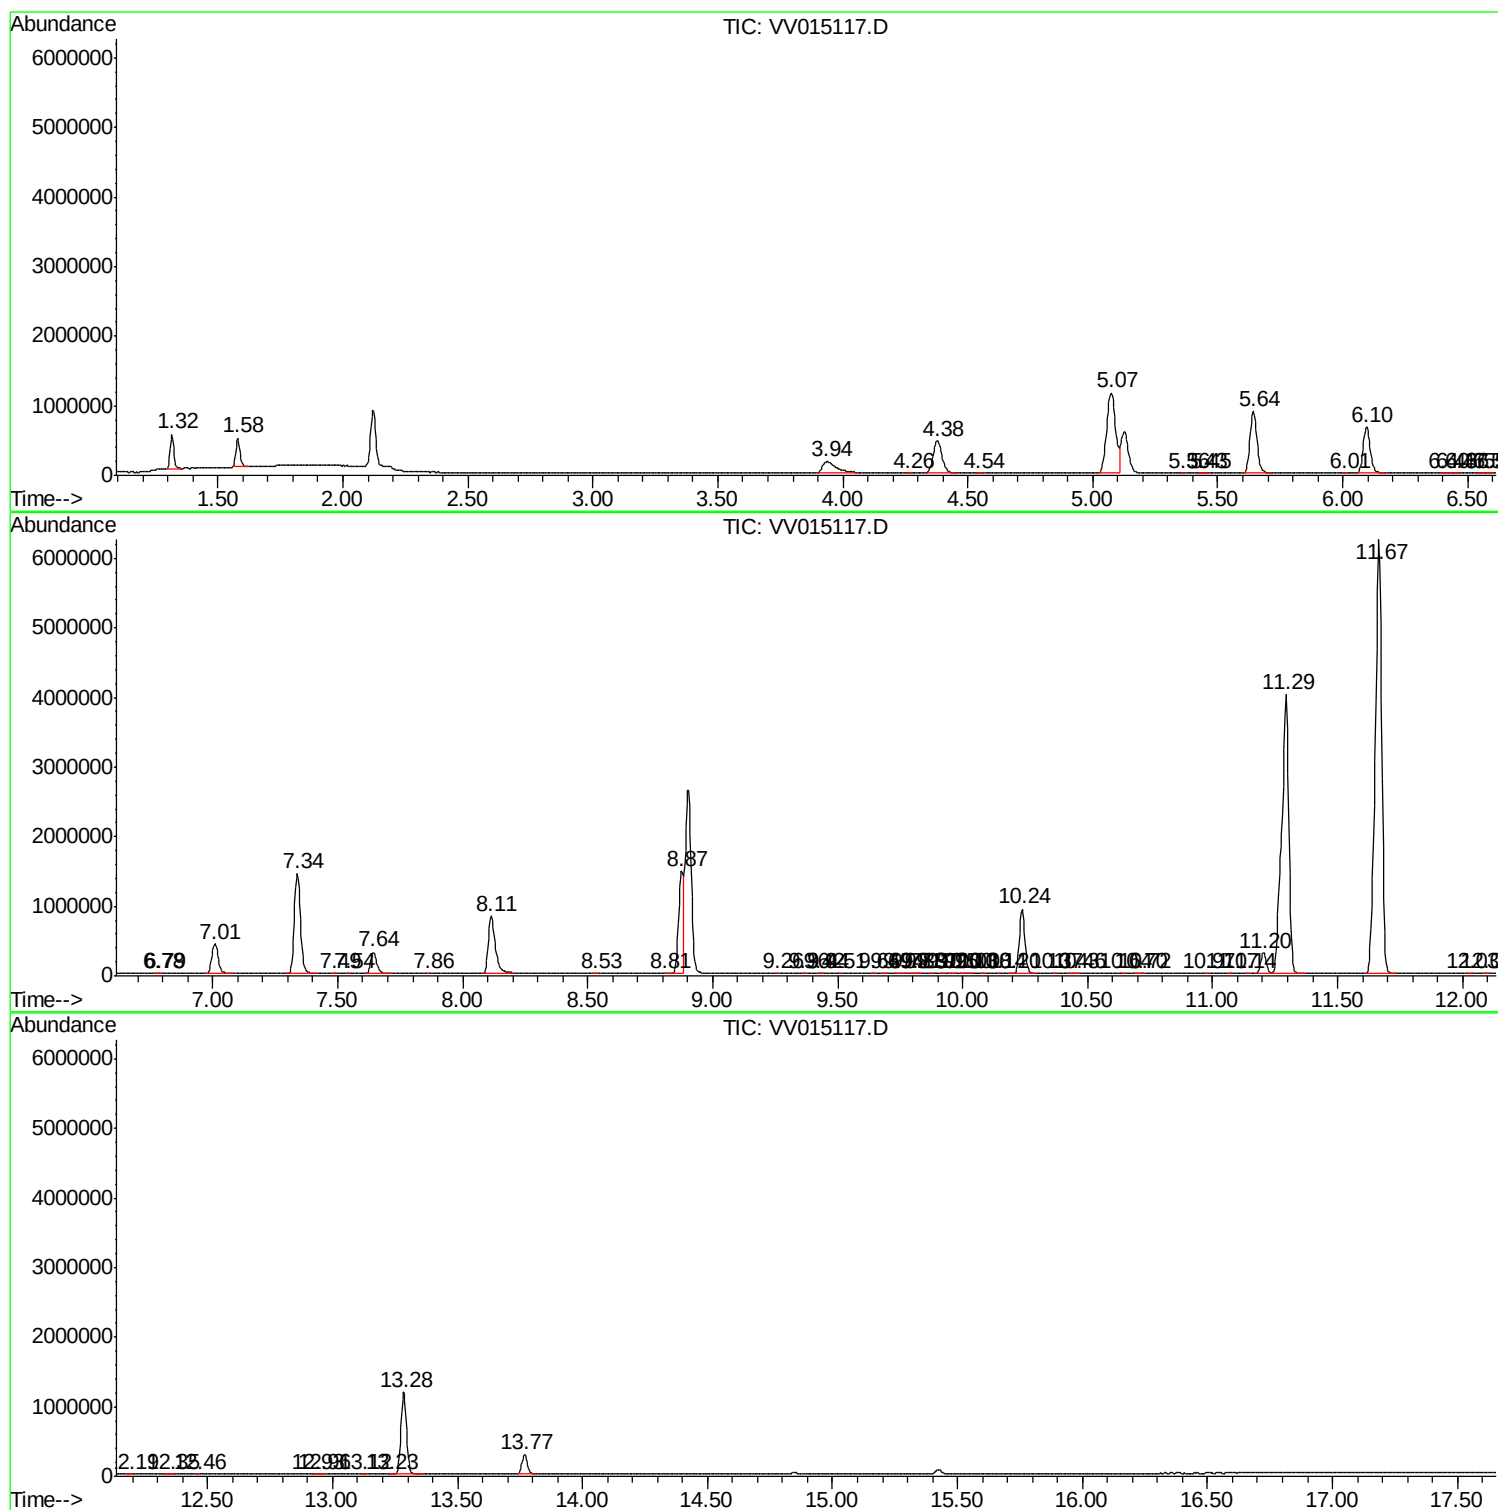

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032420\
Data File : VV015117.D
Acq On : 24 Mar 2020 12:35
Operator : SY/MD
Sample : L1941-17DL 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DL7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032420\
Data File : VV015117.D
Acq On : 24 Mar 2020 12:35
Operator : SY/MD
Sample : L1941-17DL 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DL7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc