

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015118.D
 Acq On : 24 Mar 2020 12:59
 Operator : SY/MD
 Sample : L1941-19DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	65	70	85	rVB	452279	454298	4.10%	1.128%
2	1.579	147	152	164	rVB	379516	418485	3.78%	1.039%
3	3.759	827	830	832	rBV4	2742	1809	0.02%	0.004%
4	3.939	873	886	922	rBV2	157042	647669	5.85%	1.608%
5	4.206	964	969	977	rBV10	4238	6493	0.06%	0.016%
6	4.377	1006	1022	1047	rBV	445965	1131274	10.22%	2.809%
7	4.618	1091	1097	1101	rBV9	3061	4370	0.04%	0.011%
8	4.811	1153	1157	1159	rBV4	2726	2058	0.02%	0.005%
9	4.823	1159	1161	1163	rBV3	2983	1653	0.01%	0.004%
10	4.913	1186	1189	1193	rBV6	2302	1842	0.02%	0.005%
11	4.949	1196	1200	1203	rBV5	2796	2109	0.02%	0.005%
12	5.071	1221	1238	1247	rBV2	1104415	2703901	24.42%	6.713%
13	5.251	1291	1294	1297	rBV4	3635	2447	0.02%	0.006%
14	5.328	1315	1318	1322	rBV6	3461	3321	0.03%	0.008%
15	5.508	1370	1374	1376	rBV5	2763	2363	0.02%	0.006%
16	5.640	1402	1415	1438	rBV	891679	1767176	15.96%	4.387%
17	6.093	1544	1556	1580	rVB	615395	1245991	11.25%	3.093%
18	6.357	1634	1638	1641	rBV5	2580	2168	0.02%	0.005%
19	6.479	1674	1676	1678	rBV3	2596	1315	0.01%	0.003%
20	6.553	1692	1699	1703	rVB9	3697	4122	0.04%	0.010%
21	6.605	1713	1715	1718	rVB4	2329	1194	0.01%	0.003%
22	6.630	1718	1723	1725	rBV5	3487	2463	0.02%	0.006%
23	6.643	1725	1727	1728	rBV2	2415	898	0.01%	0.002%
24	6.778	1766	1769	1771	rBV4	1287	1042	0.01%	0.003%
25	6.804	1774	1777	1779	rBV4	2241	1372	0.01%	0.003%
26	6.836	1784	1787	1790	rBV5	2623	1869	0.02%	0.005%
27	6.901	1804	1807	1809	rVB4	1755	1117	0.01%	0.003%
28	7.007	1829	1840	1862	rBV	403277	722809	6.53%	1.794%
29	7.338	1931	1943	1967	rVV	1378227	2379211	21.48%	5.907%
30	7.585	2017	2020	2023	rBV4	2729	1719	0.02%	0.004%
31	7.643	2028	2038	2056	rVV	287468	490200	4.43%	1.217%
32	7.910	2119	2121	2127	rVB7	3619	3097	0.03%	0.008%
33	7.997	2146	2148	2153	rBV5	2340	1785	0.02%	0.004%
34	8.052	2162	2165	2168	rBV4	3171	2643	0.02%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015118.D
 Acq On : 24 Mar 2020 12:59
 Operator : SY/MD
 Sample : L1941-19DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

35	8.116	2174	2185	2212	rBV	811068	1590551	14.36%	3.949%
36	8.373	2263	2265	2268	rBV4	1649	962	0.01%	0.002%
37	8.479	2291	2298	2304	rBV4	3782	5930	0.05%	0.015%
38	8.563	2320	2324	2325	rBV4	2540	1865	0.02%	0.005%
39	8.605	2332	2337	2341	rVB7	1976	2238	0.02%	0.006%
40	8.627	2341	2344	2346	rBV3	2197	1533	0.01%	0.004%
41	8.720	2370	2373	2379	rVB7	3398	2839	0.03%	0.007%
42	8.753	2379	2383	2386	rBV6	1902	1813	0.02%	0.005%
43	8.804	2396	2399	2402	rBV5	2244	1626	0.01%	0.004%
44	8.823	2402	2405	2406	rBV3	2258	1328	0.01%	0.003%
45	8.904	2409	2430	2451	rVV2	5552310	11074472	100.00%	27.494%
46	9.248	2533	2537	2540	rBV5	3526	2281	0.02%	0.006%
47	9.402	2583	2585	2587	rBV3	2872	1656	0.01%	0.004%
48	9.463	2596	2604	2608	rBV3	4819	6295	0.06%	0.016%
49	9.553	2627	2632	2633	rBV5	1800	1505	0.01%	0.004%
50	9.624	2651	2654	2655	rBV3	1382	922	0.01%	0.002%
51	9.727	2683	2686	2688	rBV4	1645	952	0.01%	0.002%
52	9.772	2697	2700	2704	rBV6	3935	3721	0.03%	0.009%
53	9.791	2704	2706	2709	rVB4	2559	1387	0.01%	0.003%
54	9.814	2709	2713	2716	rBV6	3275	2145	0.02%	0.005%
55	9.871	2728	2731	2735	rVB6	2790	2244	0.02%	0.006%
56	9.891	2735	2737	2742	rBV5	1995	1703	0.02%	0.004%
57	9.952	2752	2756	2759	rBV6	2553	2175	0.02%	0.005%
58	10.000	2768	2771	2776	rBV6	3025	2399	0.02%	0.006%
59	10.055	2786	2788	2793	rVB6	3209	1950	0.02%	0.005%
60	10.103	2798	2803	2805	rBV5	3442	3186	0.03%	0.008%
61	10.151	2816	2818	2819	rBV2	1597	856	0.01%	0.002%
62	10.196	2826	2832	2834	rBV7	3056	3710	0.03%	0.009%
63	10.238	2834	2845	2859	rVV	880684	1386611	12.52%	3.442%
64	10.383	2887	2890	2893	rBV4	2102	1660	0.01%	0.004%
65	10.402	2893	2896	2901	rVB6	2991	2387	0.02%	0.006%
66	10.434	2901	2906	2911	rBV9	3196	3475	0.03%	0.009%
67	10.476	2916	2919	2922	rBV5	2930	2049	0.02%	0.005%
68	10.495	2922	2925	2928	rBV5	2815	2267	0.02%	0.006%
69	10.659	2973	2976	2981	rVB6	2553	2355	0.02%	0.006%
70	10.685	2981	2984	2986	rVB4	1439	925	0.01%	0.002%
71	10.704	2986	2990	2993	rBV5	3814	3259	0.03%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015118.D
 Acq On : 24 Mar 2020 12:59
 Operator : SY/MD
 Sample : L1941-19DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

72	10.769	3006	3010	3015	rVB8	2895	2782	0.03%	0.007%
73	10.797	3015	3019	3022	rBV5	2562	2608	0.02%	0.006%
74	10.833	3028	3030	3032	rBV3	2248	1366	0.01%	0.003%
75	10.916	3053	3056	3058	rBV3	2954	1938	0.02%	0.005%
76	11.029	3087	3091	3092	rBV4	1761	1466	0.01%	0.004%
77	11.058	3097	3100	3102	rBV4	1875	1272	0.01%	0.003%
78	11.087	3106	3109	3113	rVB6	2595	1652	0.01%	0.004%
79	11.109	3113	3116	3117	rBV2	1752	988	0.01%	0.002%
80	11.142	3122	3126	3127	rBV4	1512	1129	0.01%	0.003%
81	11.203	3135	3145	3155	rBV	264948	406436	3.67%	1.009%
82	11.293	3156	3173	3192	rVB2	2549075	5822804	52.58%	14.456%
83	11.588	3262	3265	3269	rVB5	3676	2526	0.02%	0.006%
84	11.662	3272	3288	3304	rVV2	3206686	6623182	59.81%	16.443%
85	11.958	3378	3380	3384	rBV5	2091	1333	0.01%	0.003%
86	12.029	3400	3402	3404	rBV3	2147	987	0.01%	0.002%
87	12.055	3407	3410	3411	rBV3	1846	1207	0.01%	0.003%
88	12.209	3455	3458	3461	rBV4	2838	1797	0.02%	0.004%
89	12.360	3500	3505	3507	rBV5	2923	2735	0.02%	0.007%
90	12.418	3518	3523	3528	rBV8	6518	8252	0.07%	0.020%
91	12.492	3542	3546	3547	rBV3	2855	2038	0.02%	0.005%
92	12.598	3576	3579	3581	rBV4	3854	2799	0.03%	0.007%
93	12.736	3618	3622	3627	rBV7	3027	3330	0.03%	0.008%
94	12.871	3663	3664	3668	rBV4	1480	1104	0.01%	0.003%
95	13.116	3737	3740	3743	rBV4	3286	2121	0.02%	0.005%
96	13.193	3762	3764	3765	rBV2	2105	978	0.01%	0.002%
97	13.283	3781	3792	3807	rBV	594300	931187	8.41%	2.312%
98	13.768	3934	3943	3959	rVB	182167	282518	2.55%	0.701%
99	14.257	4093	4095	4098	rBV4	2702	2203	0.02%	0.005%
100	15.100	4354	4357	4361	rBV	34142	19354	0.17%	0.048%


Sum of corrected areas: 40279607

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015118.D
Acq On : 24 Mar 2020 12:59
Operator : SY/MD
Sample : L1941-19DL 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

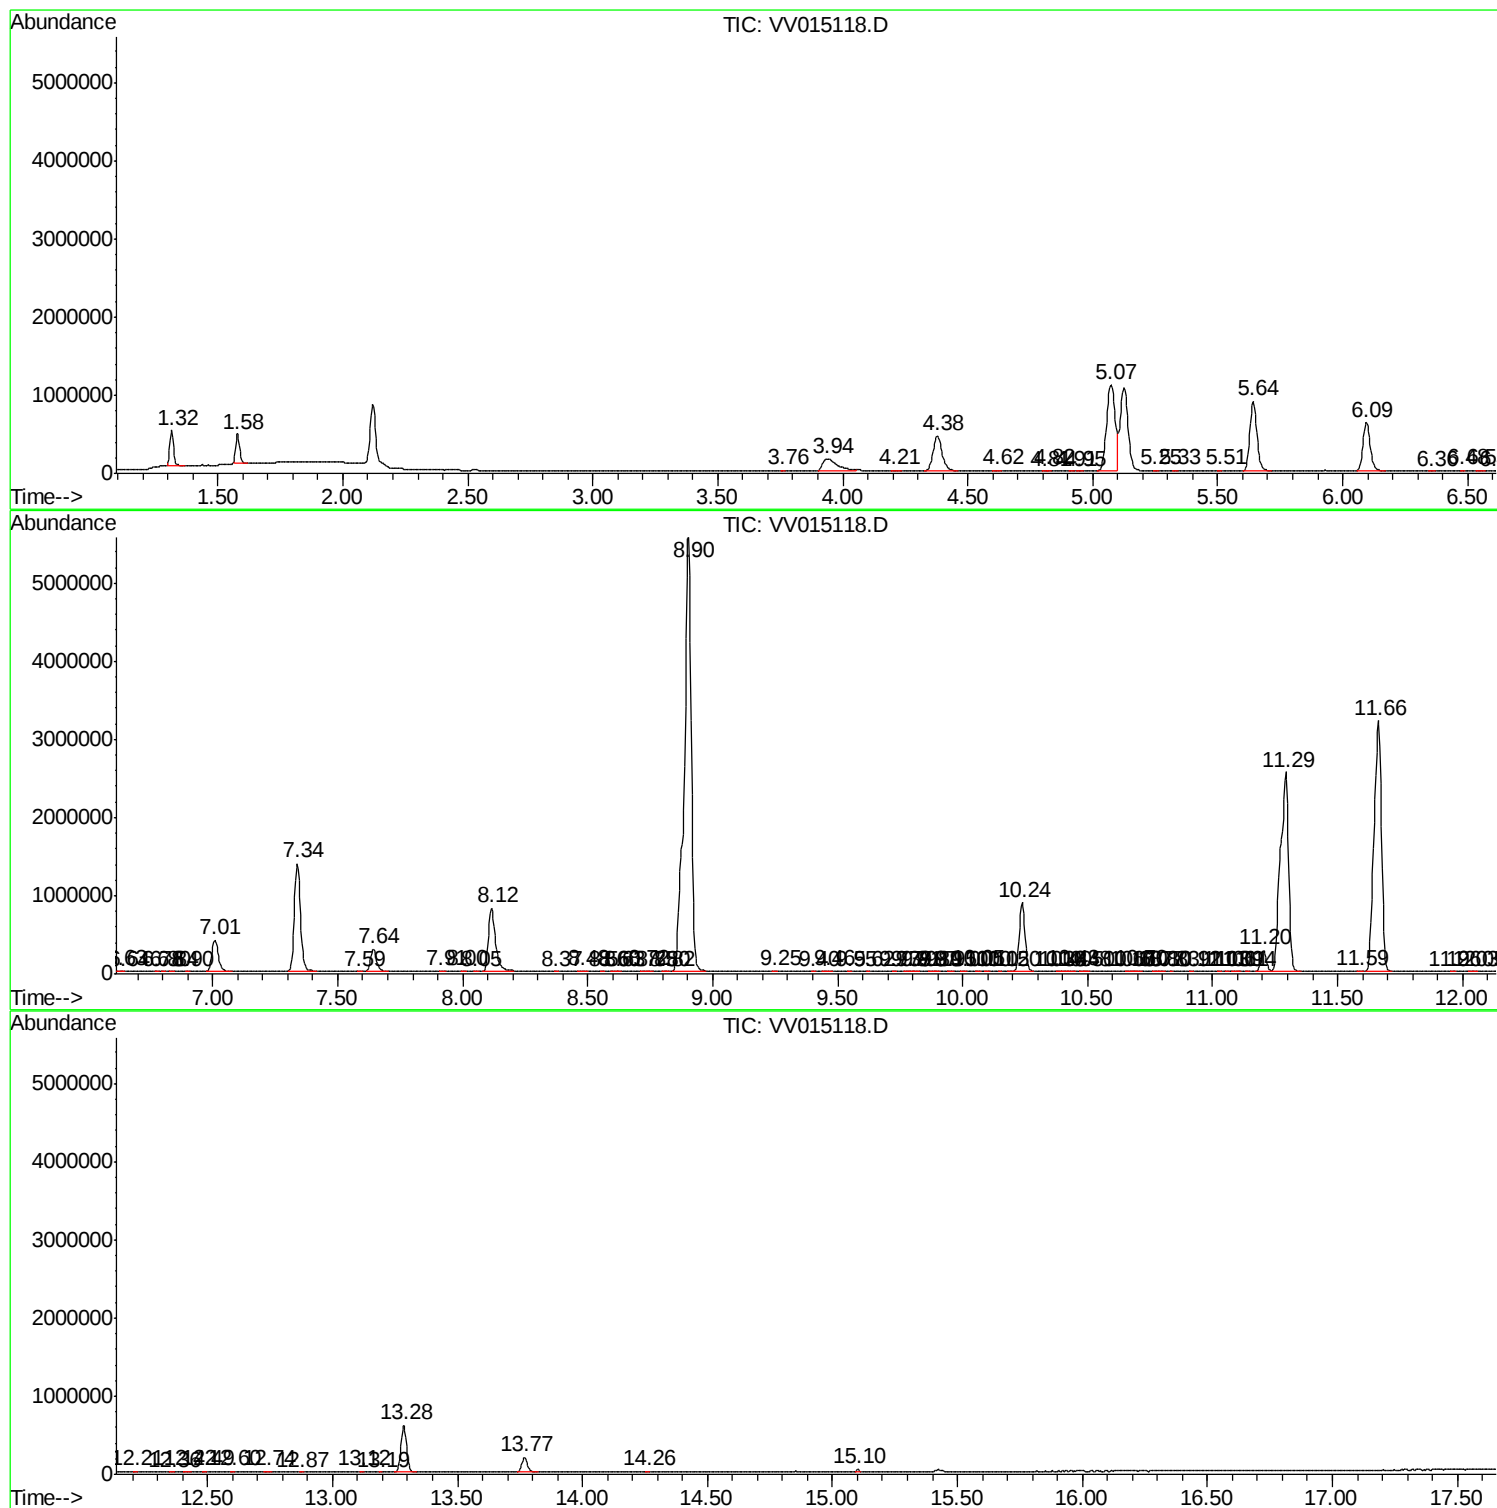

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032420\
Data File : VV015118.D
Acq On : 24 Mar 2020 12:59
Operator : SY/MD
Sample : L1941-19DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032420\
Data File : VV015118.D
Acq On : 24 Mar 2020 12:59
Operator : SY/MD
Sample : L1941-19DL 200X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DL9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc