

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015121.D
 Acq On : 24 Mar 2020 14:12
 Operator : SY/MD
 Sample : L1968-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	87	rVB	437142	449853	7.17%	1.651%
2	3.778	833	836	838	rBV3	3179	1977	0.03%	0.007%
3	3.933	871	884	923	rBV2	164049	622303	9.91%	2.284%
4	4.376	1008	1022	1045	rVB	419918	1023300	16.30%	3.756%
5	4.627	1097	1100	1104	rBV6	3614	3272	0.05%	0.012%
6	4.878	1177	1178	1180	rBV2	1290	450	0.01%	0.002%
7	4.917	1188	1190	1193	rBV4	3463	1802	0.03%	0.007%
8	4.936	1193	1196	1197	rBV2	2326	1260	0.02%	0.005%
9	4.994	1206	1214	1217	rBV8	4408	6270	0.10%	0.023%
10	5.071	1221	1238	1250	rBV2	1055548	2641689	42.08%	9.696%
11	5.640	1403	1415	1444	rBV	866925	1715026	27.32%	6.295%
12	5.823	1470	1472	1476	rBV5	2746	1464	0.02%	0.005%
13	6.045	1538	1541	1542	rBV3	2295	1518	0.02%	0.006%
14	6.093	1544	1556	1580	rVV	590852	1202210	19.15%	4.413%
15	6.454	1664	1668	1669	rBV4	1911	1436	0.02%	0.005%
16	6.585	1706	1709	1712	rBV5	3347	2704	0.04%	0.010%
17	6.756	1757	1762	1766	rBV8	3183	3201	0.05%	0.012%
18	6.810	1775	1779	1782	rBV6	2605	2112	0.03%	0.008%
19	6.872	1796	1798	1800	rBV3	3137	1608	0.03%	0.006%
20	6.936	1816	1818	1821	rBV4	1582	755	0.01%	0.003%
21	6.955	1821	1824	1826	rVB4	2647	1491	0.02%	0.005%
22	7.007	1829	1840	1862	rVV	389853	695982	11.09%	2.555%
23	7.158	1884	1887	1890	rBV4	3473	2666	0.04%	0.010%
24	7.222	1904	1907	1910	rBV4	2982	1975	0.03%	0.007%
25	7.270	1920	1922	1926	rBV5	2200	1786	0.03%	0.007%
26	7.338	1931	1943	1967	rBV	1311485	2275075	36.24%	8.350%
27	7.605	2022	2026	2027	rBV4	3882	2556	0.04%	0.009%
28	7.643	2028	2038	2056	rVV	273643	463466	7.38%	1.701%
29	7.846	2095	2101	2103	rBV6	2469	2268	0.04%	0.008%
30	7.961	2127	2137	2145	rBV2	22943	41408	0.66%	0.152%
31	8.039	2159	2161	2163	rBV3	2081	986	0.02%	0.004%
32	8.113	2174	2184	2217	rBV	777921	1519749	24.21%	5.578%
33	8.367	2260	2263	2266	rBV4	2940	2533	0.04%	0.009%
34	8.453	2288	2290	2291	rBV2	2003	868	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015121.D
 Acq On : 24 Mar 2020 14:12
 Operator : SY/MD
 Sample : L1968-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

35	8.511	2304	2308	2313	rBV7	3255	4298	0.07%	0.016%
36	8.560	2321	2323	2325	rVB3	2352	907	0.01%	0.003%
37	8.643	2346	2349	2353	rBV6	4448	4368	0.07%	0.016%
38	8.678	2358	2360	2362	rBV3	2071	961	0.02%	0.004%
39	8.749	2378	2382	2383	rBV4	3219	2206	0.04%	0.008%
40	8.823	2402	2405	2408	rBV5	2715	1662	0.03%	0.006%
41	8.875	2408	2421	2423	rBV	1428575	1852769	29.52%	6.800%
42	9.080	2481	2485	2492	rBV8	3438	4529	0.07%	0.017%
43	9.148	2502	2506	2507	rBV4	2696	1753	0.03%	0.006%
44	9.228	2529	2531	2533	rBV3	2043	1076	0.02%	0.004%
45	9.283	2546	2548	2555	rBV8	3379	2510	0.04%	0.009%
46	9.354	2568	2570	2575	rBV6	2053	1407	0.02%	0.005%
47	9.379	2575	2578	2583	rVB7	3684	2740	0.04%	0.010%
48	9.489	2610	2612	2618	rBV8	1515	1148	0.02%	0.004%
49	9.695	2673	2676	2682	rVB8	2909	2863	0.05%	0.011%
50	9.727	2682	2686	2688	rBV4	3067	2644	0.04%	0.010%
51	9.740	2688	2690	2694	rVB6	3307	1595	0.03%	0.006%
52	9.759	2694	2696	2698	rBV3	1375	810	0.01%	0.003%
53	9.785	2702	2704	2707	rBV4	2292	1497	0.02%	0.005%
54	9.974	2760	2763	2767	rBV5	3866	2805	0.04%	0.010%
55	10.013	2772	2775	2778	rVB5	2375	1452	0.02%	0.005%
56	10.039	2780	2783	2785	rBV4	3008	1952	0.03%	0.007%
57	10.113	2803	2806	2808	rBV4	2217	1511	0.02%	0.006%
58	10.238	2832	2845	2861	rBV	855812	1349150	21.49%	4.952%
59	10.627	2963	2966	2968	rBV4	2159	1335	0.02%	0.005%
60	10.662	2974	2977	2978	rBV3	1652	974	0.02%	0.004%
61	10.691	2983	2986	2989	rVB5	2895	1786	0.03%	0.007%
62	10.746	2997	3003	3004	rVB5	2812	2476	0.04%	0.009%
63	10.852	3033	3036	3040	rVB6	3030	2388	0.04%	0.009%
64	10.878	3040	3044	3049	rBV8	5192	4272	0.07%	0.016%
65	10.907	3050	3053	3057	rBV6	2167	2029	0.03%	0.007%
66	10.987	3076	3078	3081	rVB4	2695	1122	0.02%	0.004%
67	11.084	3105	3108	3109	rBV3	2158	1283	0.02%	0.005%
68	11.203	3133	3145	3156	rBV	692034	1060262	16.89%	3.892%
69	11.293	3156	3173	3189	rVB2	2827064	6277322	100.00%	23.040%
70	11.649	3272	3284	3302	rBV3	1523147	3257275	51.89%	11.955%
71	11.990	3386	3390	3395	rVB8	4725	4211	0.07%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015121.D
Acq On : 24 Mar 2020 14:12
Operator : SY/MD
Sample : L1968-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD5

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Title : VOC Analysis

72	12.064	3410	3413	3414	rBV2	2418	1405	0.02%	0.005%
73	12.129	3430	3433	3435	rBV4	2146	1337	0.02%	0.005%
74	12.177	3446	3448	3451	rBV4	1387	788	0.01%	0.003%
75	12.251	3468	3471	3472	rBV3	3524	1800	0.03%	0.007%
76	12.527	3555	3557	3561	rVB5	2352	1359	0.02%	0.005%
77	12.881	3665	3667	3670	rBV3	3005	1577	0.03%	0.006%
78	13.074	3722	3727	3729	rBV6	2782	2411	0.04%	0.009%
79	13.286	3780	3793	3805	rBV	392868	614662	9.79%	2.256%
80	13.768	3936	3943	3954	rVB3	37703	57490	0.92%	0.211%


Sum of corrected areas: 27245196

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015121.D
Acq On : 24 Mar 2020 14:12
Operator : SY/MD
Sample : L1968-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

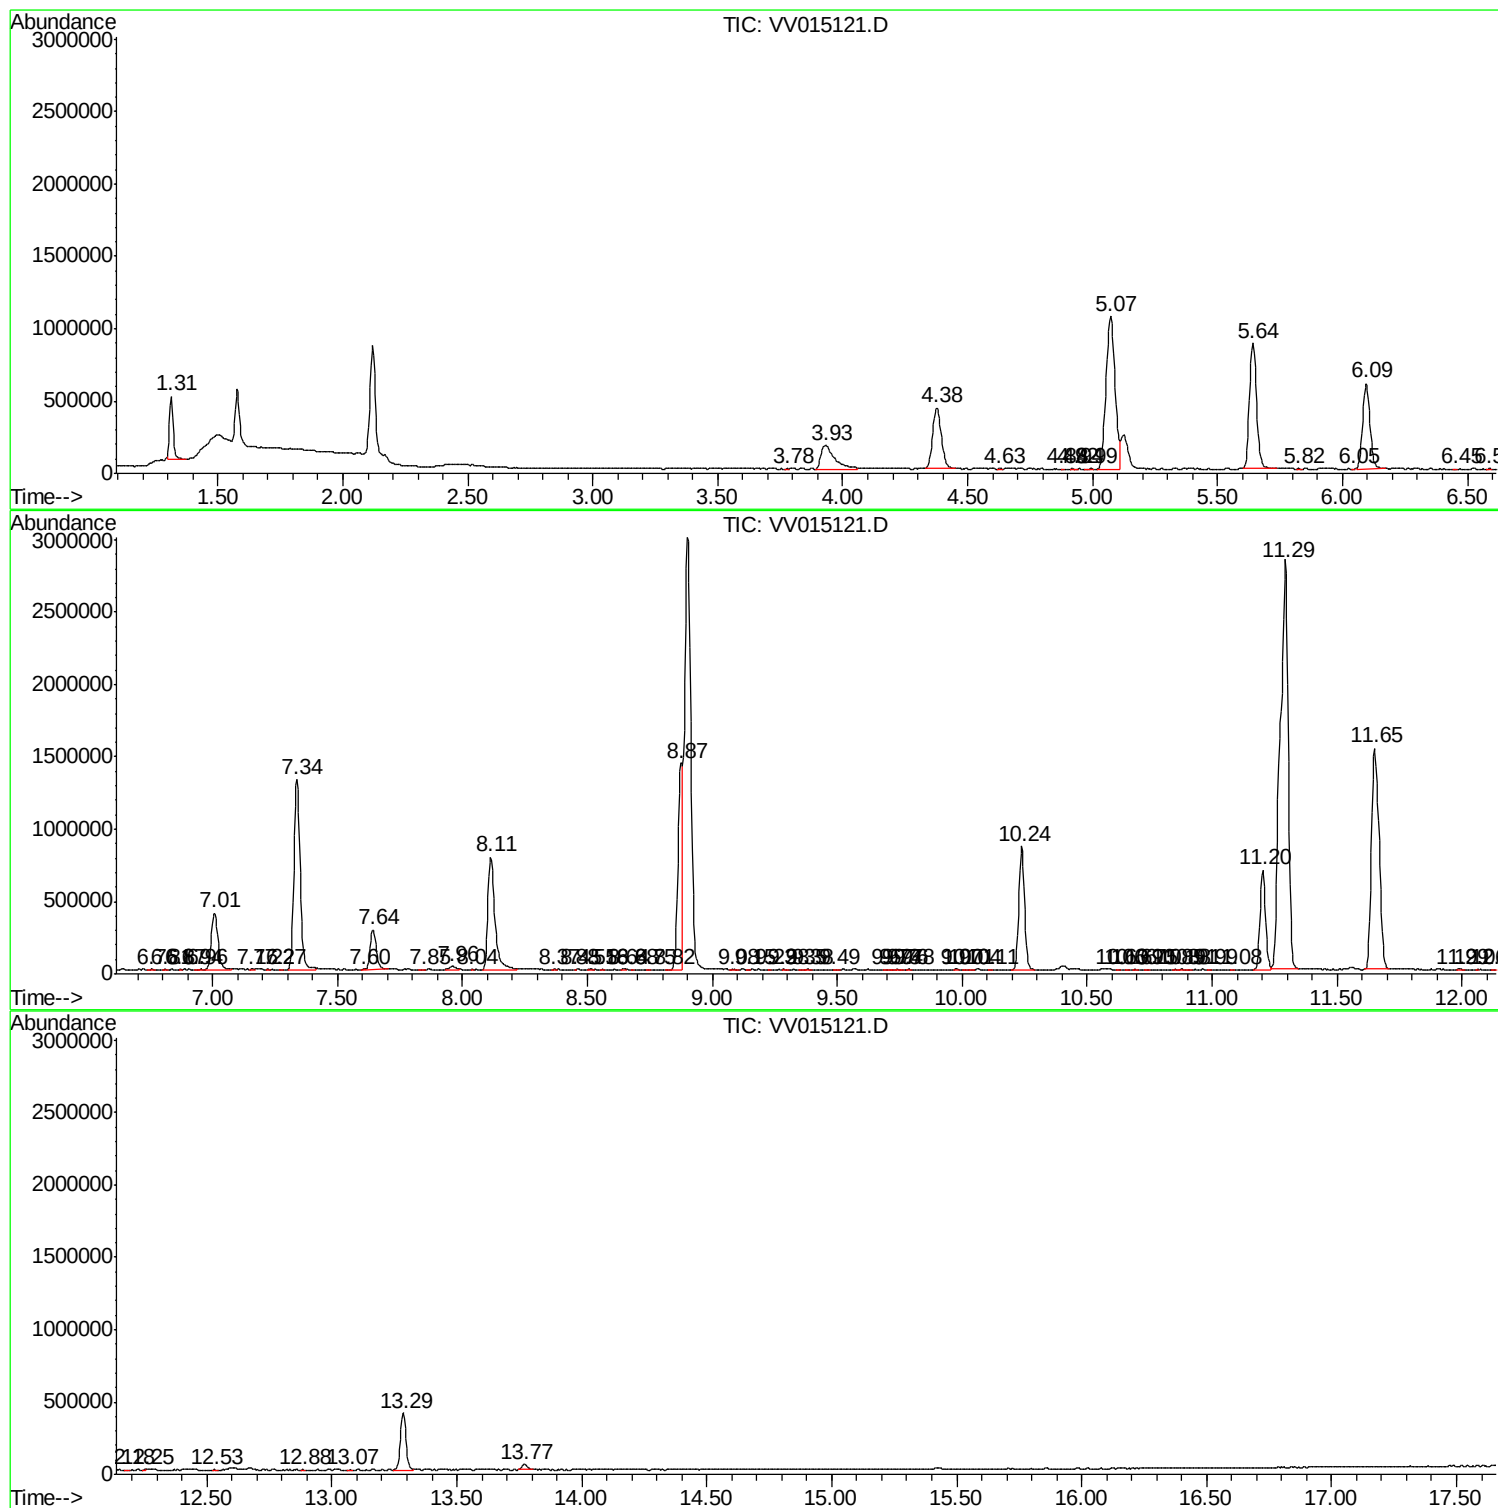

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032420\
Data File : VV015121.D
Acq On : 24 Mar 2020 14:12
Operator : SY/MD
Sample : L1968-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DD5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032420\
Data File : VV015121.D
Acq On : 24 Mar 2020 14:12
Operator : SY/MD
Sample : L1968-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DD5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc