

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015122.D
 Acq On : 24 Mar 2020 14:36
 Operator : SY/MD
 Sample : L1968-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	65	70	80	rVB	423739	424735	10.65%	1.631%
2	3.766	828	832	837	rBV6	3487	3932	0.10%	0.015%
3	3.962	873	893	929	rBV4	317907	1681817	42.16%	6.458%
4	4.380	1010	1023	1046	rVB	425458	1058870	26.54%	4.066%
5	4.811	1155	1157	1159	rBV3	3126	1585	0.04%	0.006%
6	5.074	1223	1239	1274	rVB2	1080253	2683057	67.26%	10.303%
7	5.502	1367	1372	1378	rBV10	3832	4942	0.12%	0.019%
8	5.643	1403	1416	1441	rBV	866934	1724943	43.24%	6.624%
9	5.817	1467	1470	1471	rBV3	3925	1813	0.05%	0.007%
10	5.901	1489	1496	1497	rBV7	4469	4784	0.12%	0.018%
11	6.097	1542	1557	1580	rBV	602112	1243571	31.17%	4.775%
12	6.364	1638	1640	1643	rVB3	3537	1946	0.05%	0.007%
13	6.383	1643	1646	1649	rBV5	2939	2079	0.05%	0.008%
14	6.573	1702	1705	1707	rBV3	2415	1605	0.04%	0.006%
15	6.675	1735	1737	1743	rBV7	1842	1201	0.03%	0.005%
16	6.791	1769	1773	1777	rBV7	3385	3236	0.08%	0.012%
17	6.814	1777	1780	1781	rBV3	1814	1004	0.03%	0.004%
18	6.907	1803	1809	1810	rBV6	2112	2211	0.06%	0.008%
19	6.949	1820	1822	1825	rVB4	3571	2103	0.05%	0.008%
20	7.010	1825	1841	1859	rBV	393335	715402	17.93%	2.747%
21	7.338	1931	1943	1961	rBV	1314928	2292904	57.48%	8.805%
22	7.643	2028	2038	2059	rVB	273626	458874	11.50%	1.762%
23	7.798	2085	2086	2087	rBV	1577	597	0.01%	0.002%
24	7.865	2104	2107	2109	rBV4	3460	2165	0.05%	0.008%
25	7.904	2114	2119	2121	rBV5	2821	2821	0.07%	0.011%
26	8.113	2174	2184	2217	rBV	816030	1586459	39.77%	6.092%
27	8.415	2275	2278	2282	rBV6	2334	1795	0.04%	0.007%
28	8.521	2309	2311	2314	rBV4	2418	1353	0.03%	0.005%
29	8.563	2321	2324	2327	rVB4	2424	1643	0.04%	0.006%
30	8.579	2327	2329	2331	rBV3	1924	1166	0.03%	0.004%
31	8.627	2341	2344	2348	rVB6	2394	1712	0.04%	0.007%
32	8.656	2348	2353	2357	rBV7	2652	3469	0.09%	0.013%
33	8.688	2360	2363	2366	rVB5	2433	1599	0.04%	0.006%
34	8.807	2397	2400	2402	rBV4	2573	1326	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
 Data File : VV015122.D
 Acq On : 24 Mar 2020 14:36
 Operator : SY/MD
 Sample : L1968-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
 Title : VOC Analysis

35	8.875	2408	2421	2448	rBV2	1321632	2561487	64.21%	9.836%
36	9.151	2503	2507	2509	rBV4	2434	1768	0.04%	0.007%
37	9.299	2549	2553	2558	rBV8	2254	2605	0.07%	0.010%
38	9.460	2599	2603	2604	rBV4	1953	1466	0.04%	0.006%
39	9.486	2607	2611	2612	rBV4	972	540	0.01%	0.002%
40	9.505	2613	2617	2618	rBV3	2567	1665	0.04%	0.006%
41	9.576	2636	2639	2640	rBV3	1381	740	0.02%	0.003%
42	9.624	2653	2654	2655	rBV	1408	390	0.01%	0.001%
43	9.682	2667	2672	2675	rBV6	2275	2324	0.06%	0.009%
44	9.717	2681	2683	2687	rBV5	1397	992	0.02%	0.004%
45	9.817	2708	2714	2716	rBV6	3145	2558	0.06%	0.010%
46	9.830	2716	2718	2719	rBV2	774	277	0.01%	0.001%
47	9.865	2724	2729	2732	rBV7	4556	3383	0.08%	0.013%
48	9.900	2738	2740	2742	rBV3	1326	663	0.02%	0.003%
49	9.936	2748	2751	2753	rBV4	1862	1208	0.03%	0.005%
50	9.978	2761	2764	2769	rVB7	3249	2450	0.06%	0.009%
51	10.000	2769	2771	2772	rBV2	2182	743	0.02%	0.003%
52	10.119	2802	2808	2810	rBV6	2248	2299	0.06%	0.009%
53	10.238	2832	2845	2861	rBV	878130	1369011	34.32%	5.257%
54	10.476	2914	2919	2921	rBV6	2493	2009	0.05%	0.008%
55	10.662	2974	2977	2979	rBV3	2362	1419	0.04%	0.005%
56	10.688	2983	2985	2986	rBV2	1944	849	0.02%	0.003%
57	10.769	3006	3010	3013	rBV5	1684	1283	0.03%	0.005%
58	10.785	3013	3015	3018	rBV4	2532	1606	0.04%	0.006%
59	10.833	3027	3030	3032	rBV4	2534	1876	0.05%	0.007%
60	11.074	3101	3105	3111	rBV9	2845	3464	0.09%	0.013%
61	11.203	3135	3145	3155	rBV	196116	309197	7.75%	1.187%
62	11.270	3156	3166	3188	rVB	1420717	2373921	59.51%	9.116%
63	11.505	3236	3239	3240	rBV3	2880	1661	0.04%	0.006%
64	11.608	3267	3271	3272	rBV4	2736	2056	0.05%	0.008%
65	11.656	3272	3286	3308	rVV2	1700642	3989360	100.00%	15.319%
66	11.923	3366	3369	3372	rVB5	3275	1764	0.04%	0.007%
67	12.035	3402	3404	3406	rVB3	1611	488	0.01%	0.002%
68	12.051	3407	3409	3413	rVB5	2706	1771	0.04%	0.007%
69	12.116	3426	3429	3430	rBV3	3015	1901	0.05%	0.007%
70	12.206	3454	3457	3463	rBV8	2633	2659	0.07%	0.010%
71	12.305	3485	3488	3495	rBV8	2925	2274	0.06%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015122.D
Acq On : 24 Mar 2020 14:36
Operator : SY/MD
Sample : L1968-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Title : VOC Analysis

72	12.508	3549	3551	3552	rBV2	1238	351	0.01%	0.001%
73	12.537	3556	3560	3561	rBV4	2380	1829	0.05%	0.007%
74	12.932	3682	3683	3685	rBV2	2090	1014	0.03%	0.004%
75	13.283	3781	3792	3806	rBV	664298	1020811	25.59%	3.920%
76	13.768	3933	3943	3954	rBV2	285037	438737	11.00%	1.685%


Sum of corrected areas: 26041588

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032420\
Data File : VV015122.D
Acq On : 24 Mar 2020 14:36
Operator : SY/MD
Sample : L1968-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

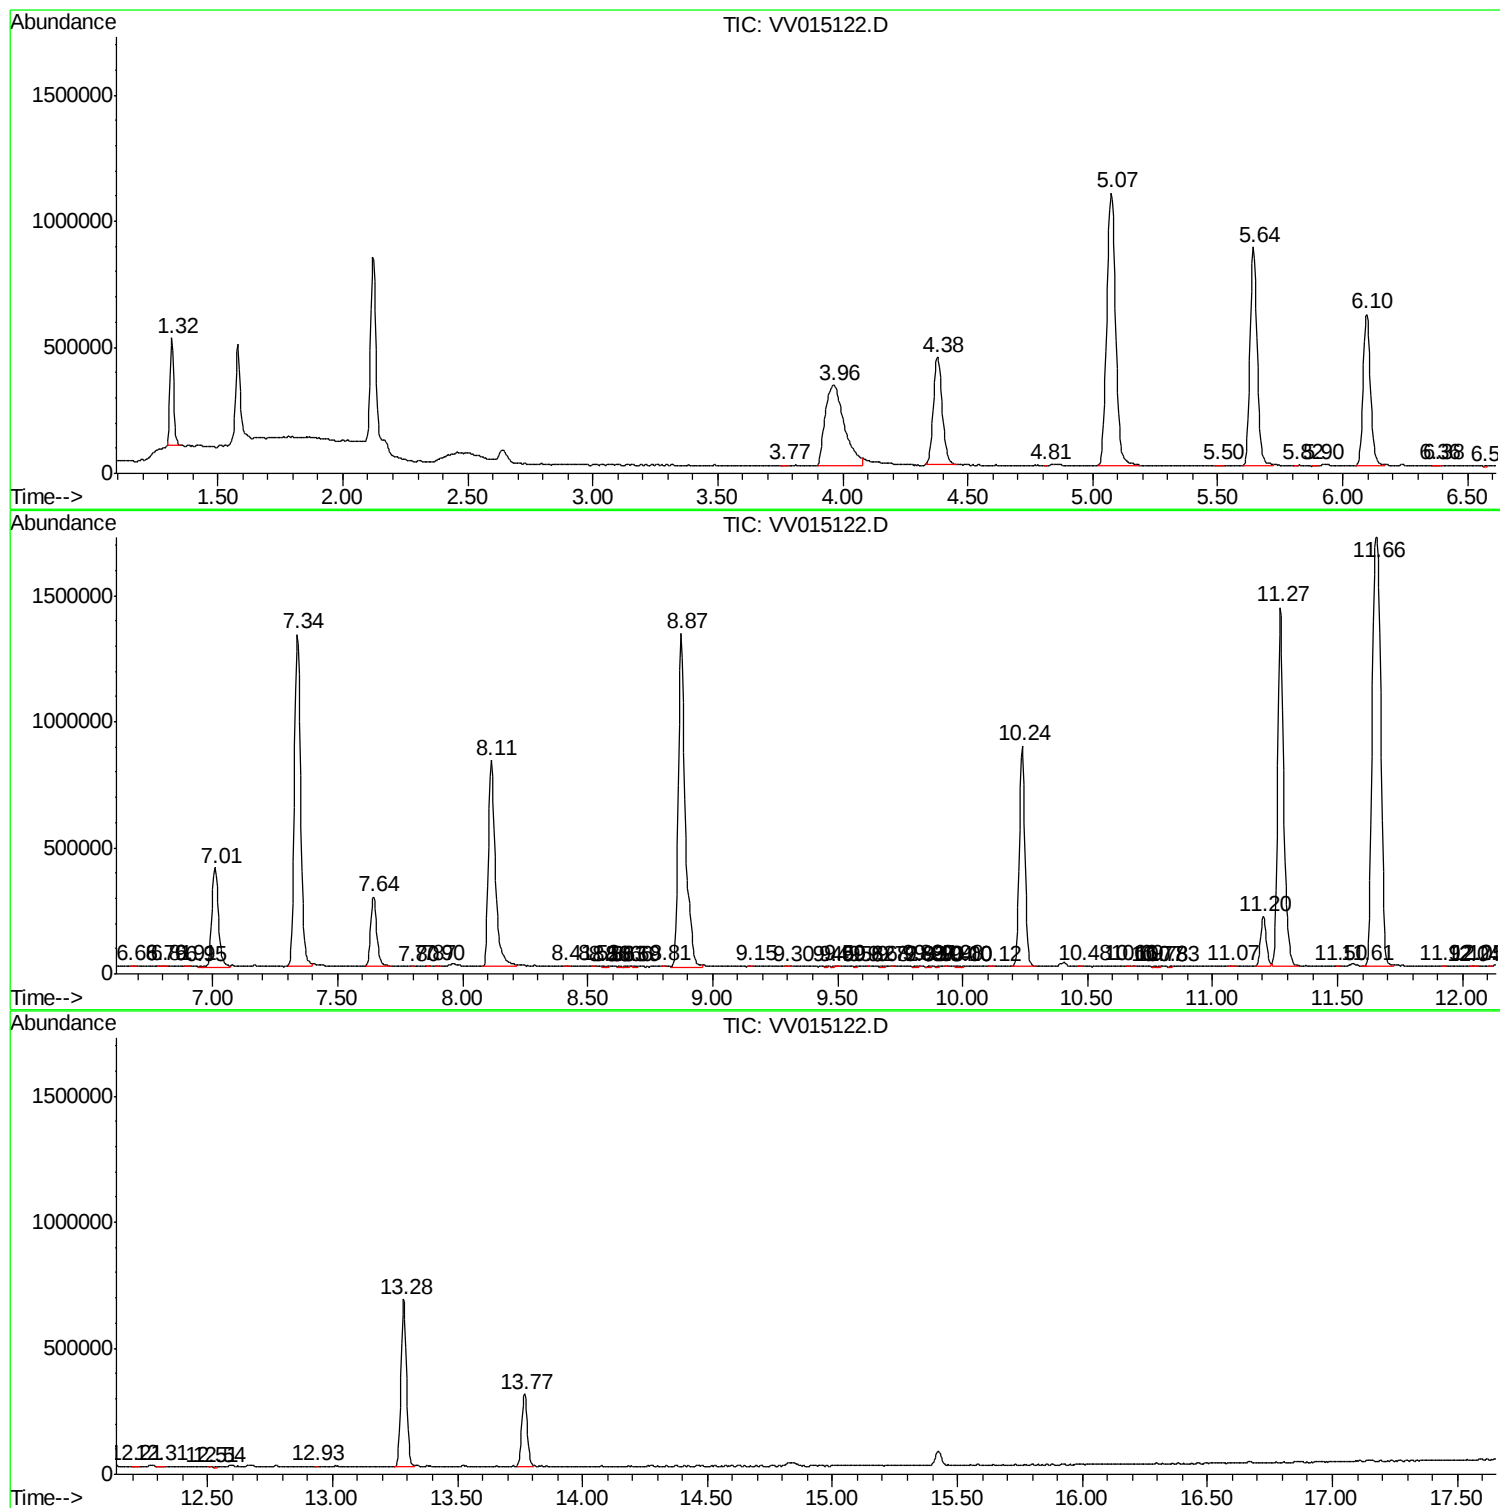

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032420\
Data File : VV015122.D
Acq On : 24 Mar 2020 14:36
Operator : SY/MD
Sample : L1968-07
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DD6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032420\
Data File : VV015122.D
Acq On : 24 Mar 2020 14:36
Operator : SY/MD
Sample : L1968-07
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DD6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc