

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020725.D
 Acq On : 24 Mar 2021 10:30
 Operator : SY/MD
 Sample : VV0324WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Quant Time: Mar 25 03:11:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 25 03:10:36 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	729537	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	715114	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	348202	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	238759	46.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.20%
7) Chloroethane-d5	1.571	69	183175	46.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.56%
11) 1,1-Dichloroethene-d2	2.108	63	361014	36.94	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.88%
21) 2-Butanone-d5	3.896	46	326901	97.01	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.01%
24) Chloroform-d	4.352	84	485483	47.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.32%
26) 1,2-Dichloroethane-d4	5.037	65	331414	48.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.74%
32) Benzene-d6	5.053	84	929952	48.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.58%
36) 1,2-Dichloropropane-d6	6.072	67	287121	49.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.12%
41) Toluene-d8	7.320	98	845812	47.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.34%
43) trans-1,3-Dichloroprop...	7.625	79	144959	46.56	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.12%
47) 2-Hexanone-d5	8.092	63	251543	102.52	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.52%
57) 1,1,2,2-Tetrachloroeth...	10.220	84	394320	46.26	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.52%
64) 1,2-Dichlorobenzene-d4	11.632	152	344883	51.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.06%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.108	101	4139	0.90	ug/L	Qvalue # 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020725.D
Acq On : 24 Mar 2021 10:30
Operator : SY/MD
Sample : VV0324WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78


Quant Time: Mar 25 03:11:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 25 03:10:36 2021
Response via : Initial Calibration

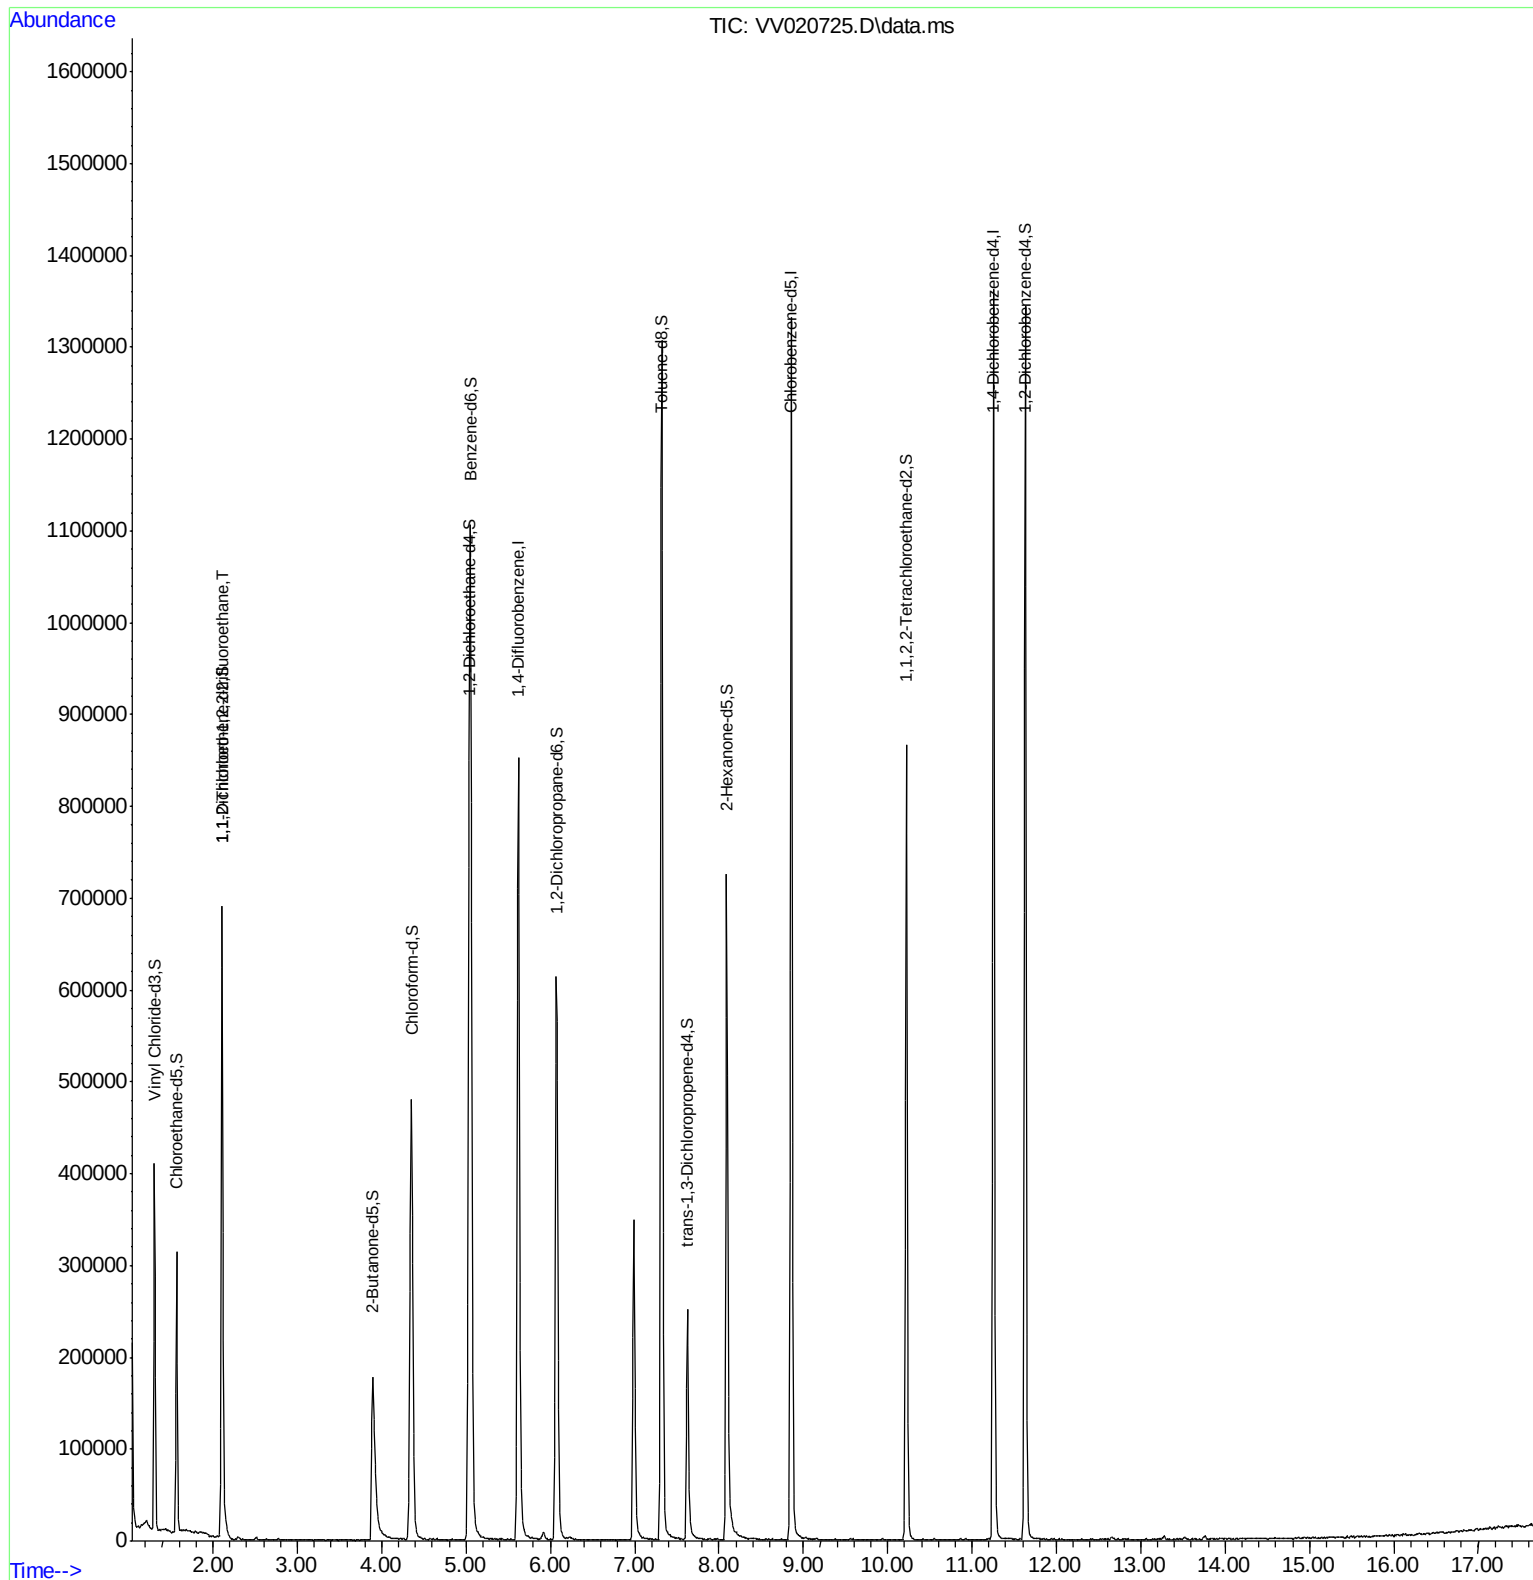

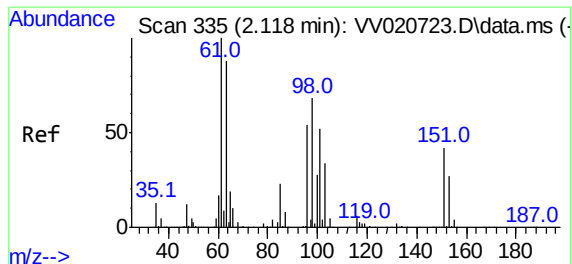

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.90 ug/L
 RT: 2.108 min Scan# 332
 Delta R.T. -0.010 min
 Lab File: VV020725.D
 Acq: 24 Mar 2021 10:30

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

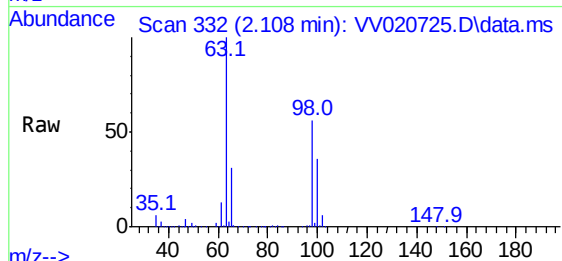

Tgt Ion:101 Resp: 4139
 Ion Ratio Lower Upper
 101 100
 85 8.1 35.4 53.0#
 151 4.5 63.5 95.3#

