

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032421\
 Data File : VW020737.D
 Acq On : 24 Mar 2021 15:17
 Operator : SY/MD
 Sample : M1783-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Mar 25 03:14:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 25 03:10:36 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	600018	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	592135	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	283318	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	225316	52.89	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.78%
7) Chloroethane-d5	1.571	69	178155	55.32	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	110.64%
11) 1,1-Dichloroethene-d2	2.108	63	348707	43.39	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.78%
21) 2-Butanone-d5	3.889	46	330037	119.09	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	119.09%
24) Chloroform-d	4.352	84	483038	57.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	114.10%
26) 1,2-Dichloroethane-d4	5.034	65	333081	59.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	119.44%
32) Benzene-d6	5.053	84	917954	58.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	116.32%
36) 1,2-Dichloropropane-d6	6.076	67	286737	59.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	118.34%
41) Toluene-d8	7.320	98	834514	56.80	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.60%
43) trans-1,3-Dichloroprop...	7.625	79	145800	56.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	113.10%
47) 2-Hexanone-d5	8.092	63	251261	123.68	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	123.68%
57) 1,1,2,2-Tetrachloroeth...	10.220	84	391584	55.48	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	110.96%
64) 1,2-Dichlorobenzene-d4	11.632	152	343243	62.42	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	124.84%#
Target Compounds						
12) 1,1-Dichloroethene	2.108	96	2997	0.86	ug/L	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020737.D
Acq On : 24 Mar 2021 15:17
Operator : SY/MD
Sample : M1783-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Mar 25 03:14:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 25 03:10:36 2021
Response via : Initial Calibration

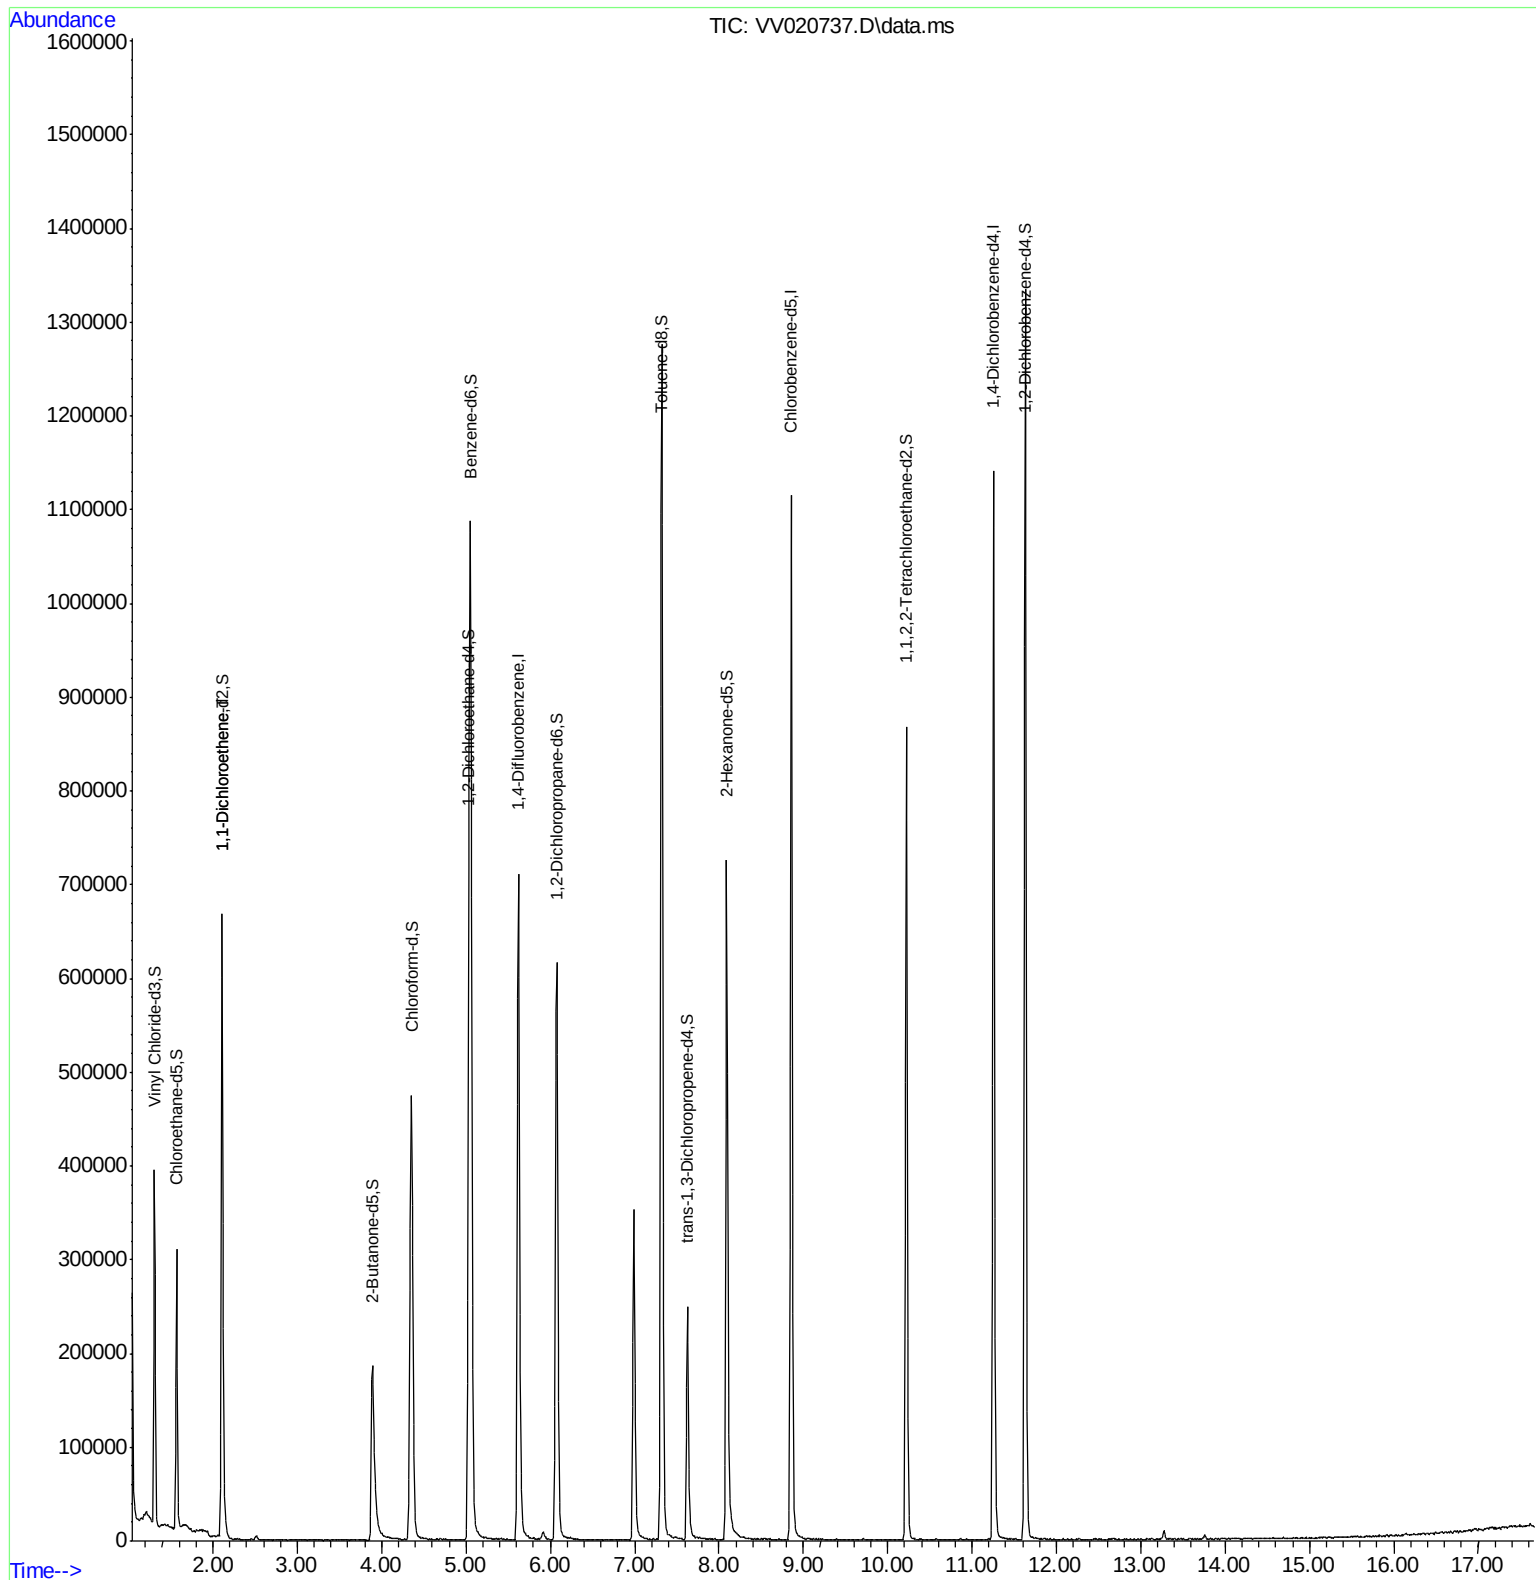

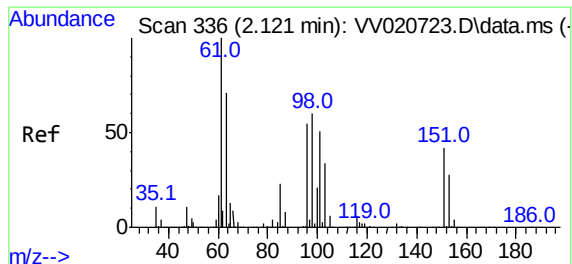

#12
 1,1-Dichloroethene
 Concen: 0.86 ug/L
 RT: 2.108 min Scan# 332
 Delta R.T. -0.013 min
 Lab File: VV020737.D
 Acq: 24 Mar 2021 15:17

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tgt Ion: 96 Resp: 2997
 Ion Ratio Lower Upper
 96 100
 61 1558.0 126.3 234.6#
 63 12136.9 100.2 186.2#

