

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032421\
 Data File : VW020730.D
 Acq On : 24 Mar 2021 12:33
 Operator : SY/MD
 Sample : M1783-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 25 03:12:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 25 03:10:36 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	700225	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	678305	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	334452	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	217242	43.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.40%
7) Chloroethane-d5	1.571	69	171457	45.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.24%
11) 1,1-Dichloroethene-d2	2.108	63	339691	36.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.44%
21) 2-Butanone-d5	3.892	46	329834	101.98	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.98%
24) Chloroform-d	4.352	84	458516	46.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.80%
26) 1,2-Dichloroethane-d4	5.037	65	315122	48.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.82%
32) Benzene-d6	5.053	84	869872	48.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.22%
36) 1,2-Dichloropropane-d6	6.072	67	266682	48.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.08%
41) Toluene-d8	7.320	98	799401	47.50	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.00%
43) trans-1,3-Dichloroprop...	7.625	79	136300	46.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.30%
47) 2-Hexanone-d5	8.091	63	240649	103.41	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.41%
57) 1,1,2,2-Tetrachloroeth...	10.220	84	368333	45.55	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.10%
64) 1,2-Dichlorobenzene-d4	11.628	152	329571	50.77	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.54%
Target Compounds						
25) Chloroform	4.384	83	11882m	1.28	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020730.D
Acq On : 24 Mar 2021 12:33
Operator : SY/MD
Sample : M1783-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 25 03:12:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 25 03:10:36 2021
Response via : Initial Calibration

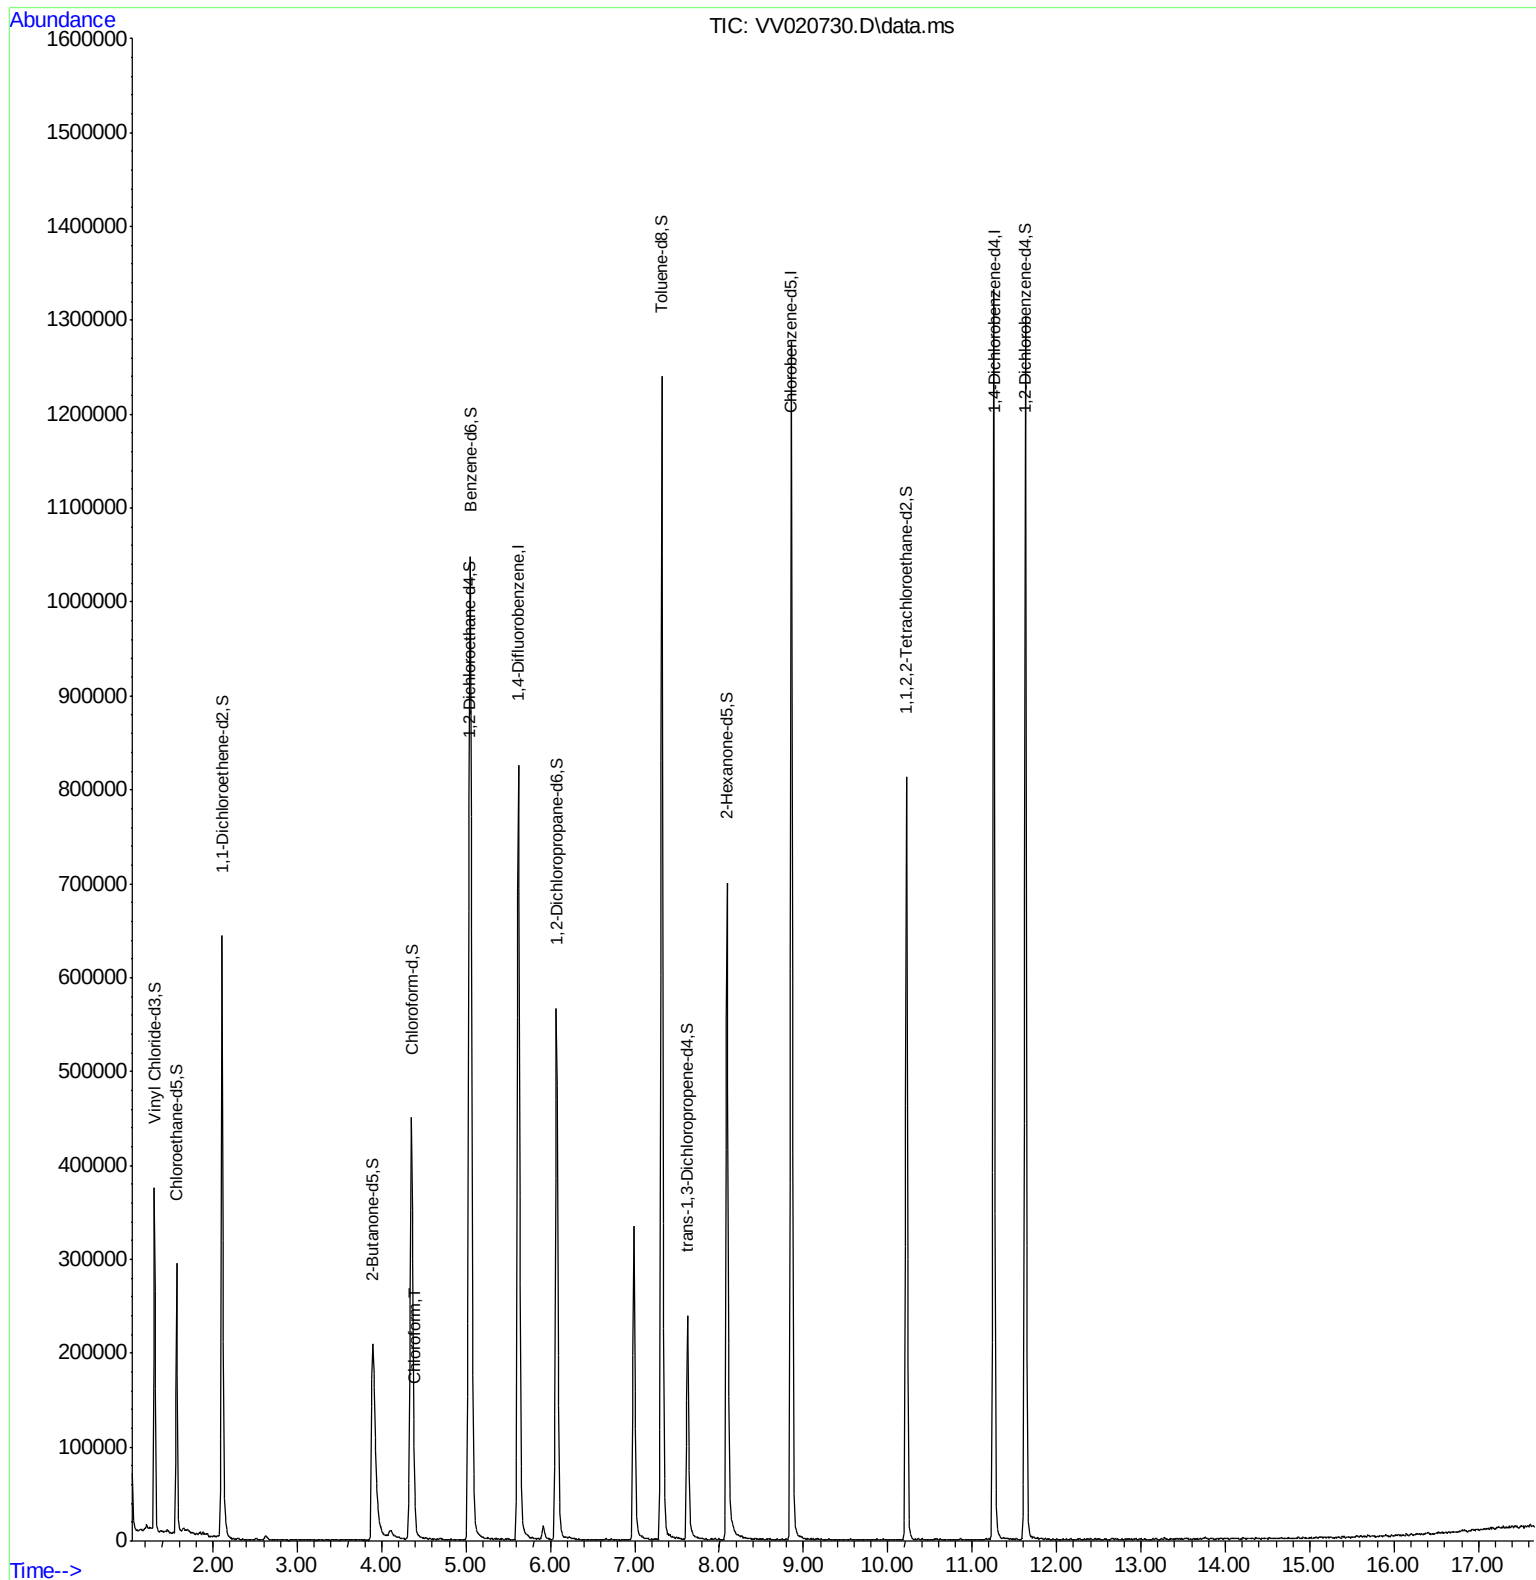

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020730.D
Acq On : 24 Mar 2021 12:33
Operator : SY/MD
Sample : M1783-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 25 03:12:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 25 03:10:36 2021
Response via : Initial Calibration

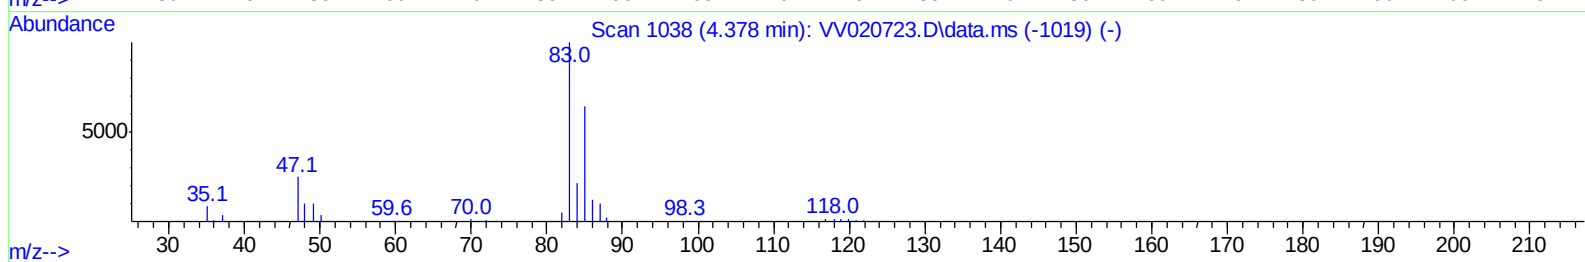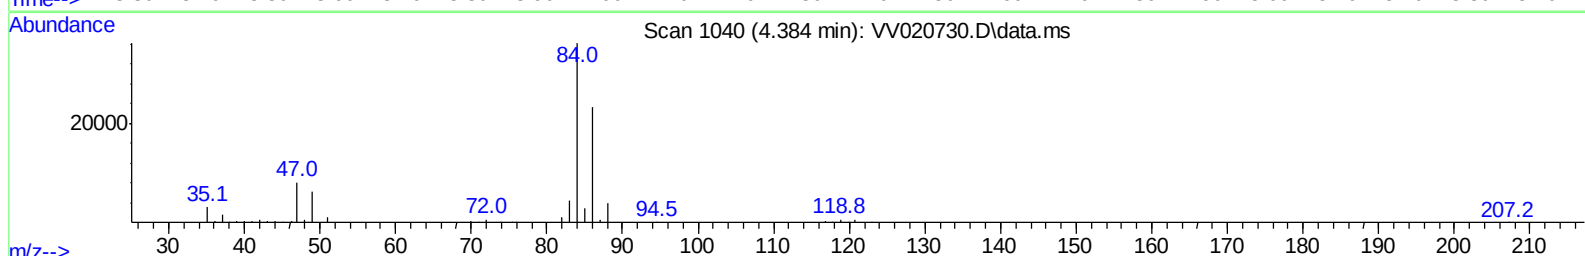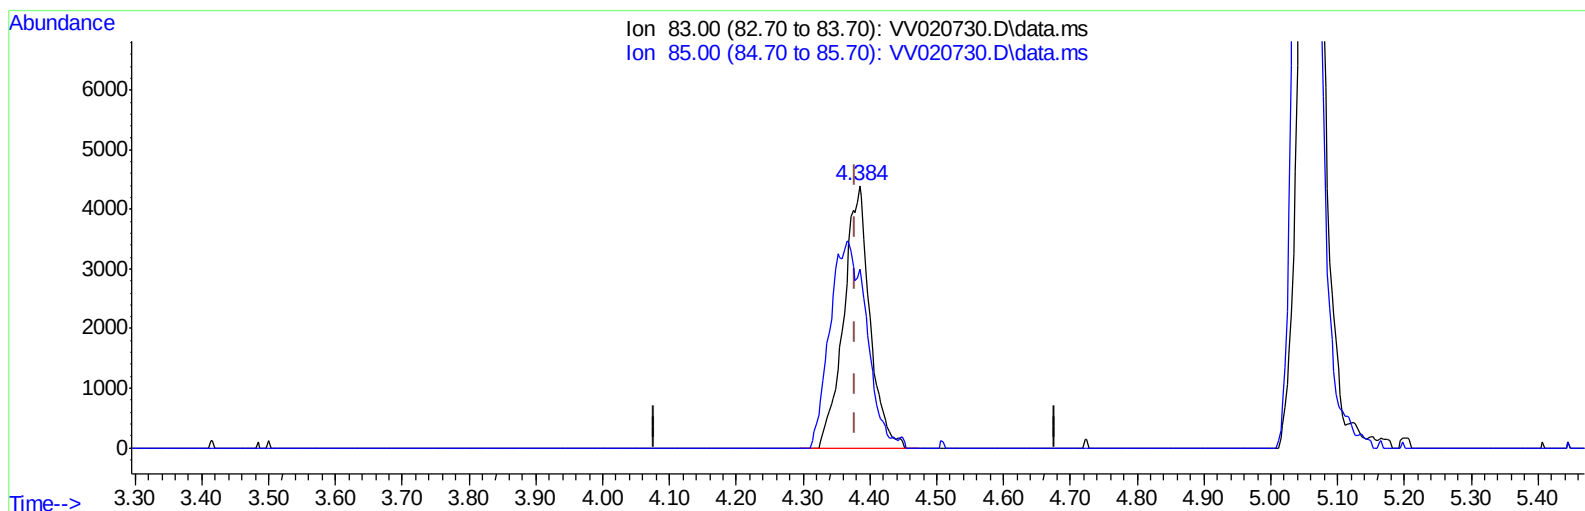

TIC: VV020730.D\data.ms

(25) Chloroform (T)




4.384min (+ 0.006) 1.28 ug/L m

response 11882

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	66.70	67.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020730.D
 Acq On : 24 Mar 2021 12:33
 Operator : SY/MD
 Sample : M1783-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 25 03:12:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 25 03:10:36 2021
 Response via : Initial Calibration

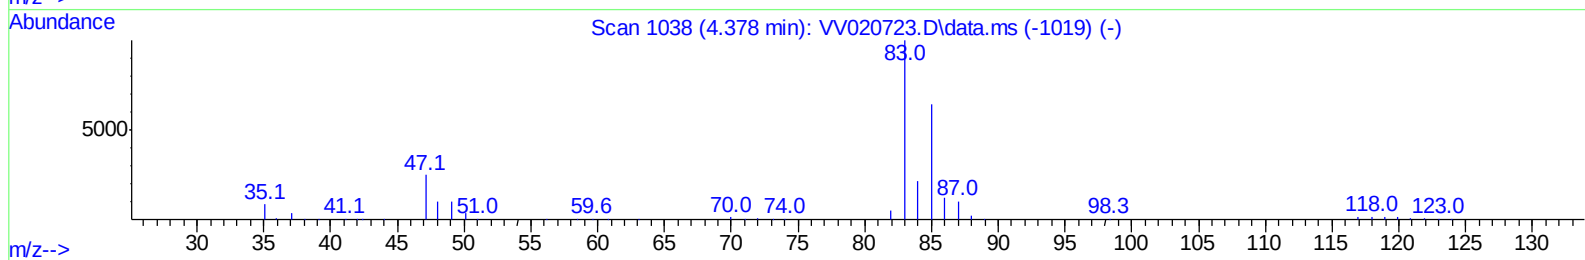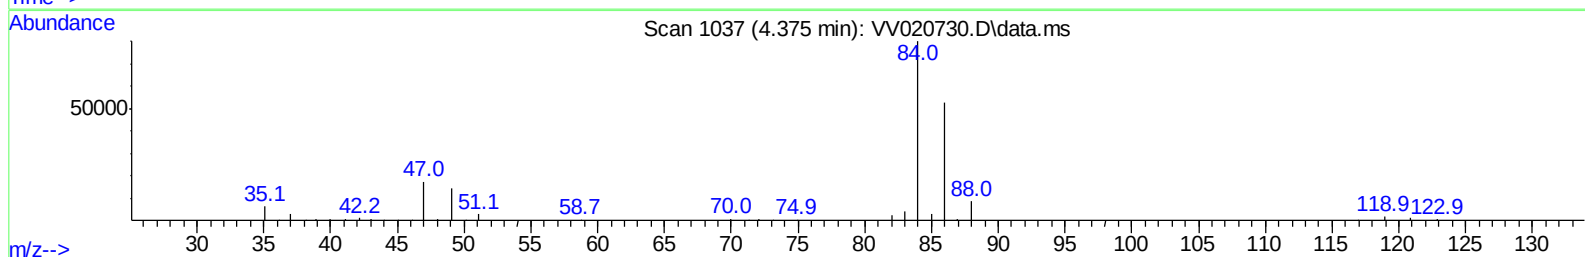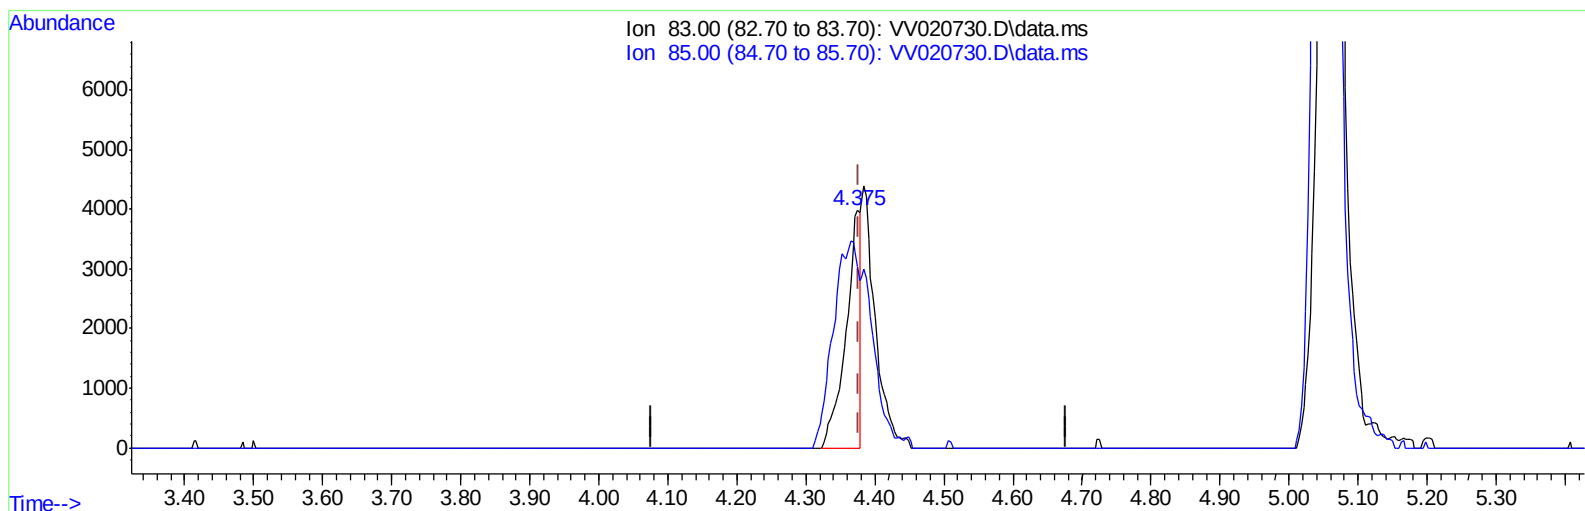

TIC: VV020730.D\data.ms

(25) Chloroform (T)

4.375min (-0.003) 0.62 ug/L

response 5701

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	66.70	76.53
0.00	0.00	0.00
0.00	0.00	0.00