

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020726.D
 Acq On : 24 Mar 2021 10:59
 Operator : SY/MD
 Sample : M1781-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3F9

Quant Time: Mar 25 03:11:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 25 03:10:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	721911	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	700641	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.256	152	351832	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	190301	37.13	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.26%		
7) Chloroethane-d5	1.568	69	158785	40.98	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.96%		
11) 1,1-Dichloroethene-d2	2.108	63	309012	31.96	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.92%		
21) 2-Butanone-d5	3.892	46	278552	83.54	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	83.54%		
24) Chloroform-d	4.349	84	442436	43.43	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.86%		
26) 1,2-Dichloroethane-d4	5.034	65	305416	45.51	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.02%		
32) Benzene-d6	5.050	84	830836	44.49	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.98%		
36) 1,2-Dichloropropane-d6	6.072	67	260352	45.41	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.82%		
41) Toluene-d8	7.317	98	755168	43.44	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.88%		
43) trans-1,3-Dichloroprop...	7.625	79	131280	43.03	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.06%		
47) 2-Hexanone-d5	8.092	63	206020	85.70	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.70%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	346245	41.46	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	82.92%		
64) 1,2-Dichlorobenzene-d4	11.628	152	315277	46.17	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.34%		
Target Compounds					Qvalue	
13) Acetone	2.182	43	29072	12.23	ug/L	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020726.D
Acq On : 24 Mar 2021 10:59
Operator : SY/MD
Sample : M1781-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3F9

Quant Time: Mar 25 03:11:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 25 03:10:36 2021
Response via : Initial Calibration

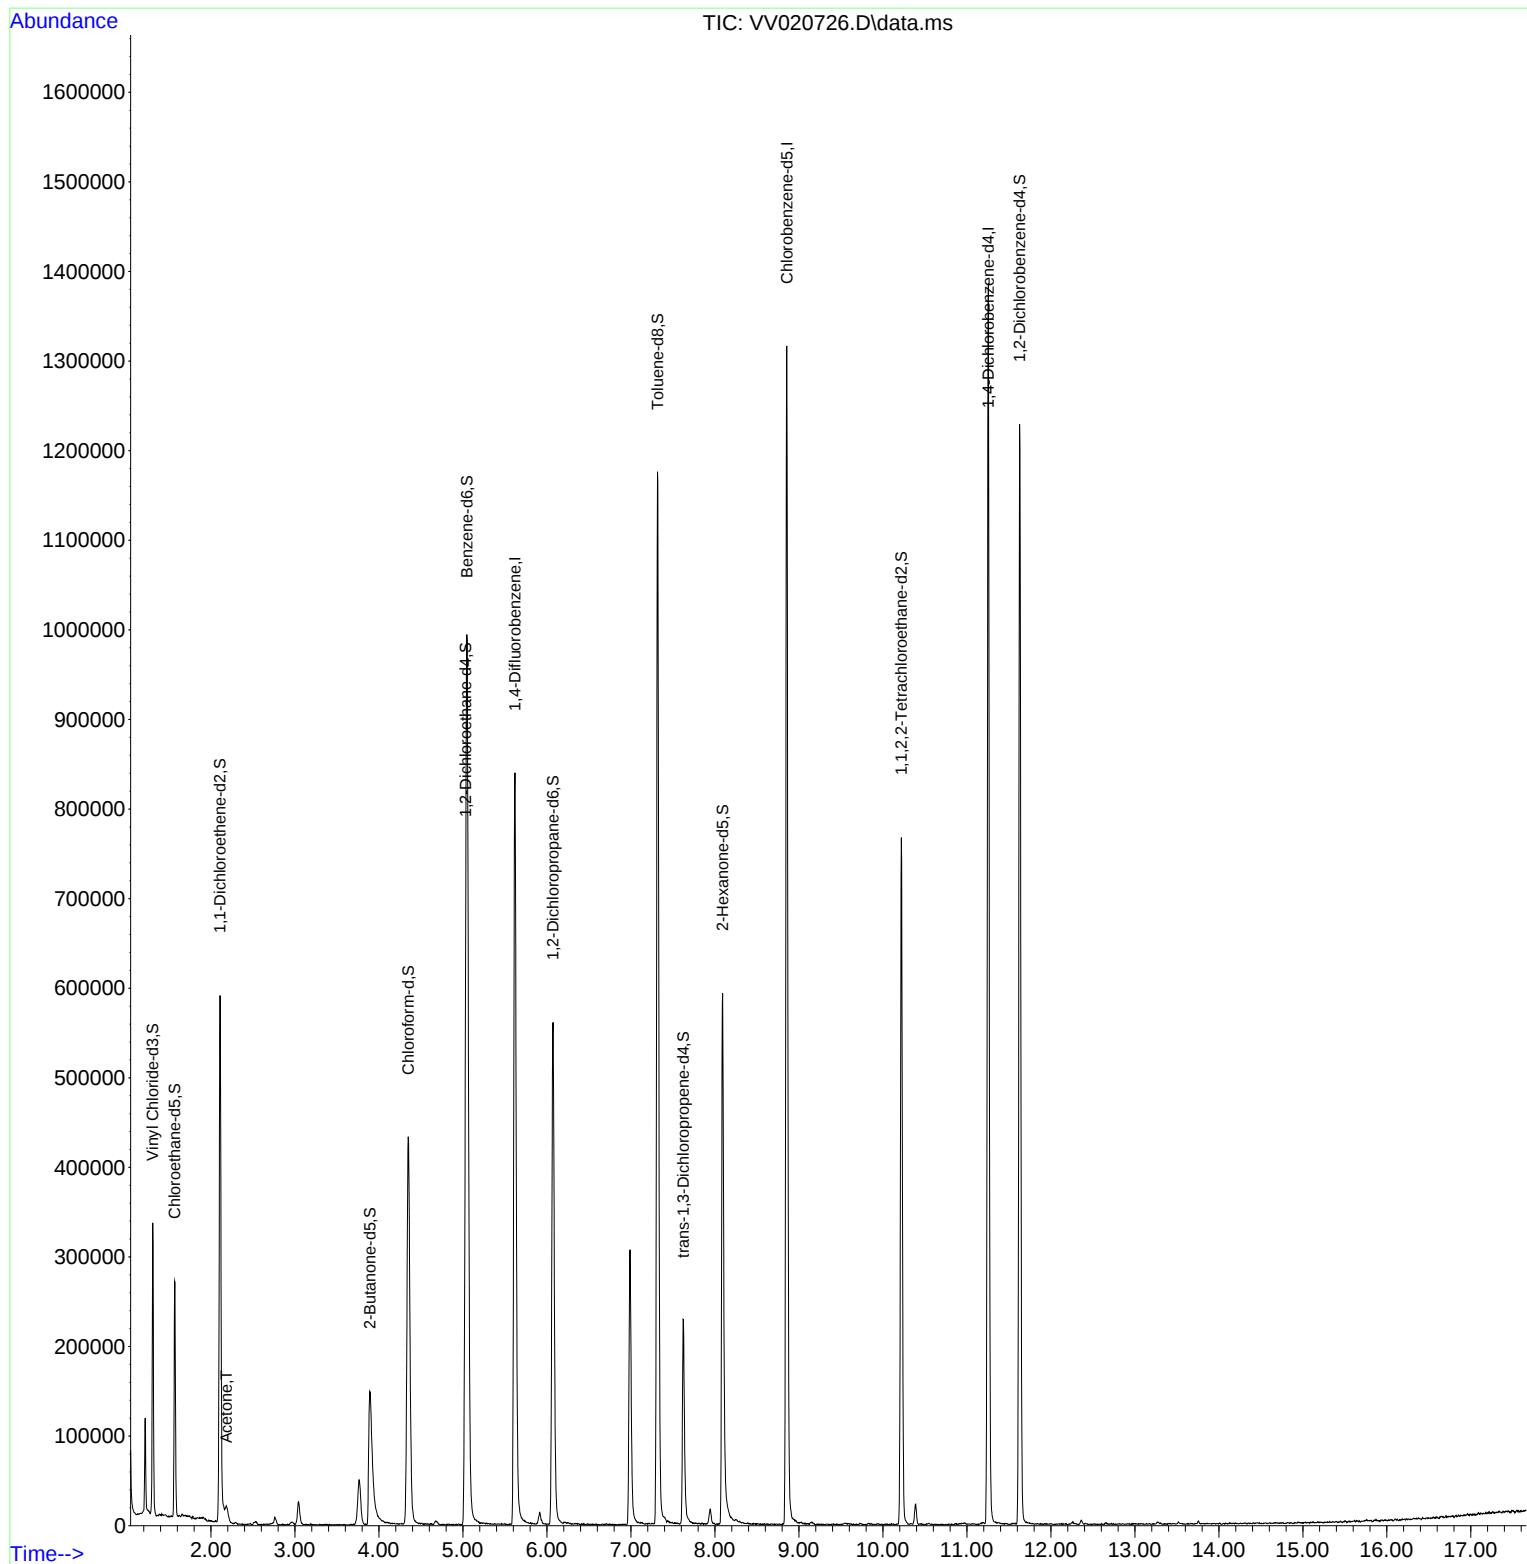

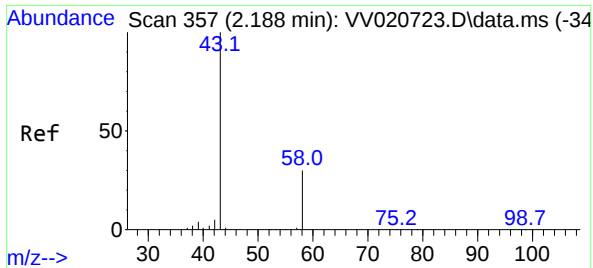

#13
 Acetone
 Concen: 12.23 ug/L
 RT: 2.182 min Scan# 355
 Delta R.T. -0.006 min
 Lab File: VV020726.D
 Acq: 24 Mar 2021 10:59

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3F9

Tgt Ion:	43	Resp:	29072
Ion	Ratio	Lower	Upper
43	100		
58	10.0	0.0	60.8

