

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020738.D
 Acq On : 24 Mar 2021 15:41
 Operator : SY/MD
 Sample : M1781-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3G0

Quant Time: Mar 25 03:14:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 25 03:10:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	580050	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	566754	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	277155	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	188788	45.84	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.68%		
7) Chloroethane-d5	1.568	69	155054	49.80	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	99.60%		
11) 1,1-Dichloroethene-d2	2.108	63	297227	38.26	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.52%		
21) 2-Butanone-d5	3.892	46	316640	118.19	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	118.19%		
24) Chloroform-d	4.352	84	446735	54.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	109.16%		
26) 1,2-Dichloroethane-d4	5.037	65	311737	57.82	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	115.64%		
32) Benzene-d6	5.053	84	826872	54.74	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	109.48%		
36) 1,2-Dichloropropane-d6	6.072	67	267340	57.64	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	115.28%		
41) Toluene-d8	7.320	98	732606	52.10	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.20%		
43) trans-1,3-Dichloroprop...	7.625	79	130975	53.08	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	106.16%		
47) 2-Hexanone-d5	8.092	63	237787	122.29	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	122.29%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	376833	55.78	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	111.56%		
64) 1,2-Dichlorobenzene-d4	11.632	152	319294	59.36	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	118.72%		
Target Compounds					Qvalue	
13) Acetone	2.185	43	26216	13.72	ug/L	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020738.D
Acq On : 24 Mar 2021 15:41
Operator : SY/MD
Sample : M1781-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3G0

Quant Time: Mar 25 03:14:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 25 03:10:36 2021
Response via : Initial Calibration

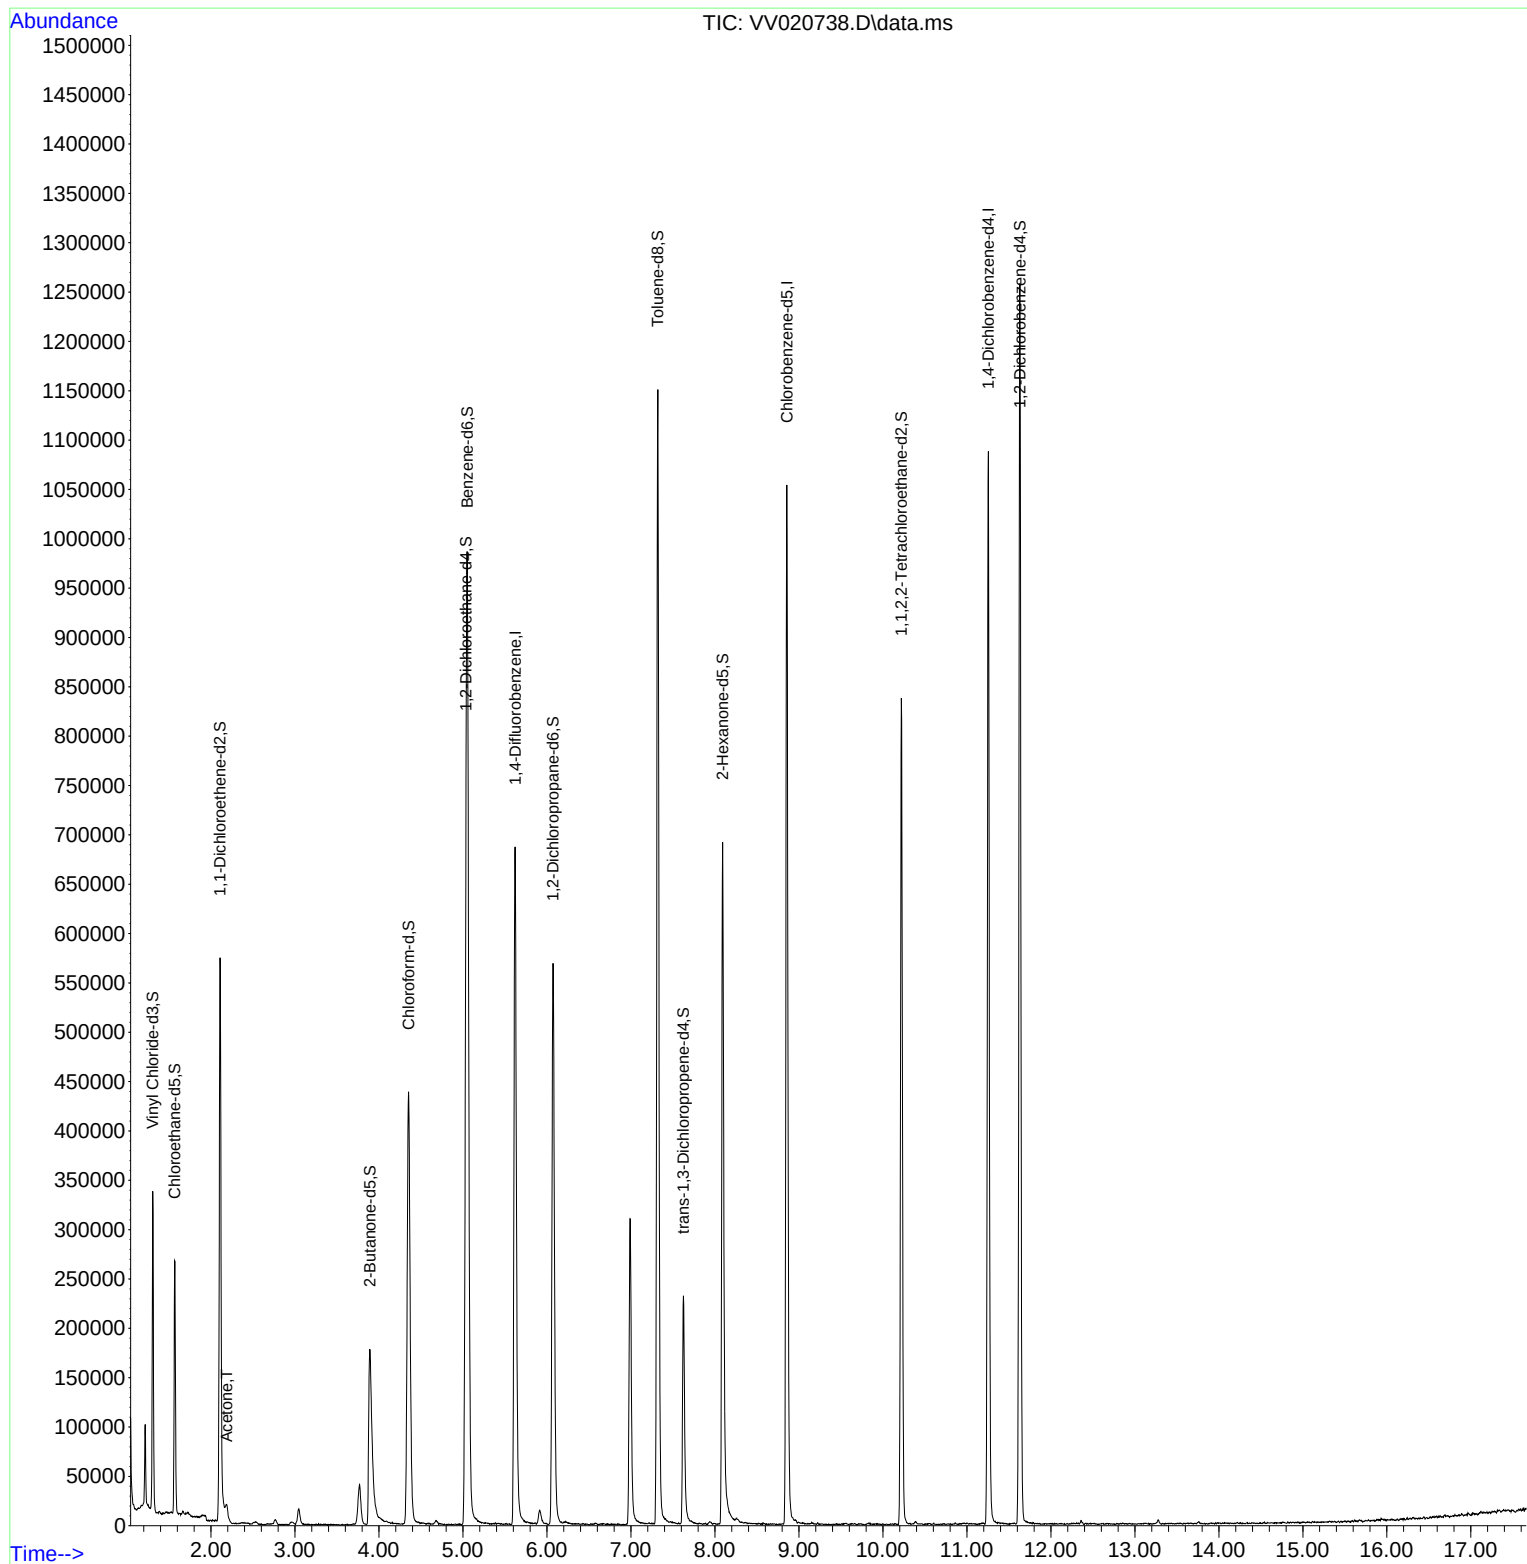

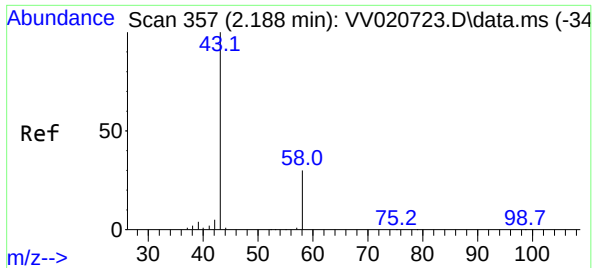

#13
 Acetone
 Concen: 13.72 ug/L
 RT: 2.185 min Scan# 356
 Delta R.T. -0.003 min
 Lab File: VV020738.D
 Acq: 24 Mar 2021 15:41

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3G0

Tgt Ion: 43	Resp: 26216
Ion Ratio	Lower Upper
43	100
58	12.3 0.0 60.8

