

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020724.D
 Acq On : 24 Mar 2021 10:06
 Operator : SY/MD
 Sample : VV0324MBL01
 Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	420113	414087	14.36%	1.865%
2	1.568	157	164	174	rBV	314725	352443	12.22%	1.587%
3	2.108	322	332	360	rVB	707407	1057839	36.69%	4.764%
4	2.442	433	436	442	rBV6	1101	955	0.03%	0.004%
5	2.510	452	457	463	rBV6	2620	3290	0.11%	0.015%
6	2.626	487	493	495	rBV4	1024	975	0.03%	0.004%
7	2.928	582	587	589	rBV4	640	538	0.02%	0.002%
8	2.979	599	603	605	rVB2	553	443	0.02%	0.002%
9	3.005	609	611	616	rVB3	800	649	0.02%	0.003%
10	3.031	616	619	620	rBV2	500	222	0.01%	0.001%
11	3.076	629	633	635	rBV4	774	571	0.02%	0.003%
12	3.101	639	641	643	rBV3	669	386	0.01%	0.002%
13	3.143	650	654	655	rBV2	971	531	0.02%	0.002%
14	3.179	663	665	668	rBV	513	277	0.01%	0.001%
15	3.236	680	683	689	rBV3	722	517	0.02%	0.002%
16	3.269	691	693	696	rVV2	630	375	0.01%	0.002%
17	3.301	699	703	705	rVV4	809	453	0.02%	0.002%
18	3.336	711	714	715	rBV	463	277	0.01%	0.001%
19	3.372	721	725	726	rBV2	630	369	0.01%	0.002%
20	3.388	726	730	735	rVB6	918	827	0.03%	0.004%
21	3.471	752	756	758	rBV2	559	441	0.02%	0.002%
22	3.519	769	771	775	rBV3	519	377	0.01%	0.002%
23	3.555	780	782	785	rBV3	597	434	0.02%	0.002%
24	3.587	789	792	794	rBV	521	259	0.01%	0.001%
25	3.706	825	829	831	rBV4	1123	765	0.03%	0.003%
26	3.754	841	844	846	rBV2	745	414	0.01%	0.002%
27	3.892	876	887	930	rBV	172259	571285	19.81%	2.573%
28	4.349	1013	1029	1056	rBV	484401	1187088	41.17%	5.346%
29	4.580	1098	1101	1102	rBV2	876	530	0.02%	0.002%
30	4.751	1152	1154	1155	rBV2	553	278	0.01%	0.001%
31	4.783	1162	1164	1166	rBV2	649	288	0.01%	0.001%
32	4.851	1183	1185	1189	rVB3	542	197	0.01%	0.001%
33	4.912	1201	1204	1207	rBV3	1150	820	0.03%	0.004%
34	5.047	1229	1246	1289	rBV2	1128440	2883277	100.00%	12.984%
35	5.461	1373	1375	1378	rBV3	545	292	0.01%	0.001%
36	5.481	1378	1381	1384	rBV4	1640	841	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020724.D
 Acq On : 24 Mar 2021 10:06
 Operator : SY/MD
 Sample : VV0324MBL01
 Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.619	1411	1424	1447	rBV	883223	1771892	61.45%	7.979%
38	6.072	1551	1565	1593	rBV	614908	1260199	43.71%	5.675%
39	6.378	1658	1660	1661	rVB	603	227	0.01%	0.001%
40	6.400	1661	1667	1669	rBV3	1152	1219	0.04%	0.005%
41	6.468	1686	1688	1692	rVB2	620	394	0.01%	0.002%
42	6.532	1706	1708	1711	rVB2	865	421	0.01%	0.002%
43	6.555	1711	1715	1717	rVB2	900	451	0.02%	0.002%
44	6.571	1717	1720	1721	rBV2	448	207	0.01%	0.001%
45	6.596	1726	1728	1731	rBV	474	232	0.01%	0.001%
46	6.651	1743	1745	1748	rBV3	568	264	0.01%	0.001%
47	6.670	1748	1751	1754	rBV4	930	643	0.02%	0.003%
48	6.719	1764	1766	1770	rVB4	685	332	0.01%	0.001%
49	6.741	1770	1773	1779	rVB4	976	898	0.03%	0.004%
50	6.767	1779	1781	1784	rBV3	997	538	0.02%	0.002%
51	6.783	1784	1786	1789	rBV2	643	308	0.01%	0.001%
52	6.831	1796	1801	1805	rBV5	1185	994	0.03%	0.004%
53	6.886	1816	1818	1819	rBV	407	213	0.01%	0.001%
54	6.918	1826	1828	1830	rBV2	431	210	0.01%	0.001%
55	6.989	1834	1850	1870	rBV	359680	656564	22.77%	2.957%
56	7.317	1940	1952	1975	rBV	1352808	2310970	80.15%	10.406%
57	7.622	2037	2047	2067	rBV	256042	449766	15.60%	2.025%
58	8.047	2176	2179	2180	rBV3	964	464	0.02%	0.002%
59	8.092	2183	2193	2222	rBV	711993	1251541	43.41%	5.636%
60	8.365	2272	2278	2284	rBV9	1655	2367	0.08%	0.011%
61	8.403	2288	2290	2292	rBV3	1155	566	0.02%	0.003%
62	8.526	2326	2328	2333	rBV4	1283	990	0.03%	0.004%
63	8.670	2370	2373	2375	rBV4	679	364	0.01%	0.002%
64	8.805	2414	2415	2417	rBV2	473	212	0.01%	0.001%
65	8.854	2417	2430	2457	rBV	1351250	2208706	76.60%	9.946%
66	9.210	2537	2541	2546	rBV6	1046	1138	0.04%	0.005%
67	9.391	2595	2597	2599	rBV2	601	209	0.01%	0.001%
68	9.436	2609	2611	2612	rBV2	669	262	0.01%	0.001%
69	9.484	2623	2626	2631	rBV4	1319	833	0.03%	0.004%
70	9.551	2644	2647	2648	rBV2	1221	654	0.02%	0.003%
71	9.735	2702	2704	2705	rVB2	707	211	0.01%	0.001%
72	9.831	2730	2734	2738	rBV3	706	757	0.03%	0.003%
73	9.860	2740	2743	2744	rBV2	733	297	0.01%	0.001%
74	9.889	2750	2752	2755	rBV3	692	412	0.01%	0.002%
75	9.905	2755	2757	2761	rVB3	1254	852	0.03%	0.004%
76	9.928	2761	2764	2765	rBV	832	534	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020724.D
 Acq On : 24 Mar 2021 10:06
 Operator : SY/MD
 Sample : VV0324MBL01
 Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	9.969	2775	2777	2779	rVB2	642	242	0.01%	0.001%
78	10.037	2796	2798	2801	rBV3	557	334	0.01%	0.002%
79	10.082	2810	2812	2813	rBV	579	211	0.01%	0.001%
80	10.108	2818	2820	2825	rVB5	1076	784	0.03%	0.004%
81	10.149	2831	2833	2835	rVB	739	288	0.01%	0.001%
82	10.162	2835	2837	2841	rBV3	457	304	0.01%	0.001%
83	10.220	2842	2855	2879	rVV	903718	1387366	48.12%	6.247%
84	10.384	2904	2906	2907	rBV2	952	349	0.01%	0.002%
85	10.432	2919	2921	2924	rBV4	504	229	0.01%	0.001%
86	10.542	2951	2955	2963	rBV7	1583	2300	0.08%	0.010%
87	10.628	2977	2982	2985	rBV4	705	668	0.02%	0.003%
88	10.696	3001	3003	3008	rVB3	937	513	0.02%	0.002%
89	10.818	3039	3041	3042	rBV2	867	359	0.01%	0.002%
90	10.921	3070	3073	3085	rVB9	2442	3333	0.12%	0.015%
91	10.966	3085	3087	3089	rBV2	542	348	0.01%	0.002%
92	11.255	3165	3177	3202	rBV	1420063	2196735	76.19%	9.892%
93	11.628	3279	3293	3316	rBV	1392972	2184193	75.75%	9.836%
94	11.937	3386	3389	3392	rBV	835	625	0.02%	0.003%
95	12.136	3449	3451	3454	rBV3	766	571	0.02%	0.003%
96	12.191	3465	3468	3472	rBV4	953	818	0.03%	0.004%
97	12.387	3527	3529	3532	rBV2	791	330	0.01%	0.001%
98	12.651	3607	3611	3612	rBV4	4434	2939	0.10%	0.013%
99	13.519	3875	3881	3888	rBV3	7405	10210	0.35%	0.046%
100	13.844	3976	3982	3983	rBV3	1227	1164	0.04%	0.005%




Sum of corrected areas: 22207134

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020724.D
Acq On : 24 Mar 2021 10:06
Operator : SY/MD
Sample : VV0324MBL01
Misc : 5.00g/5.0ml/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

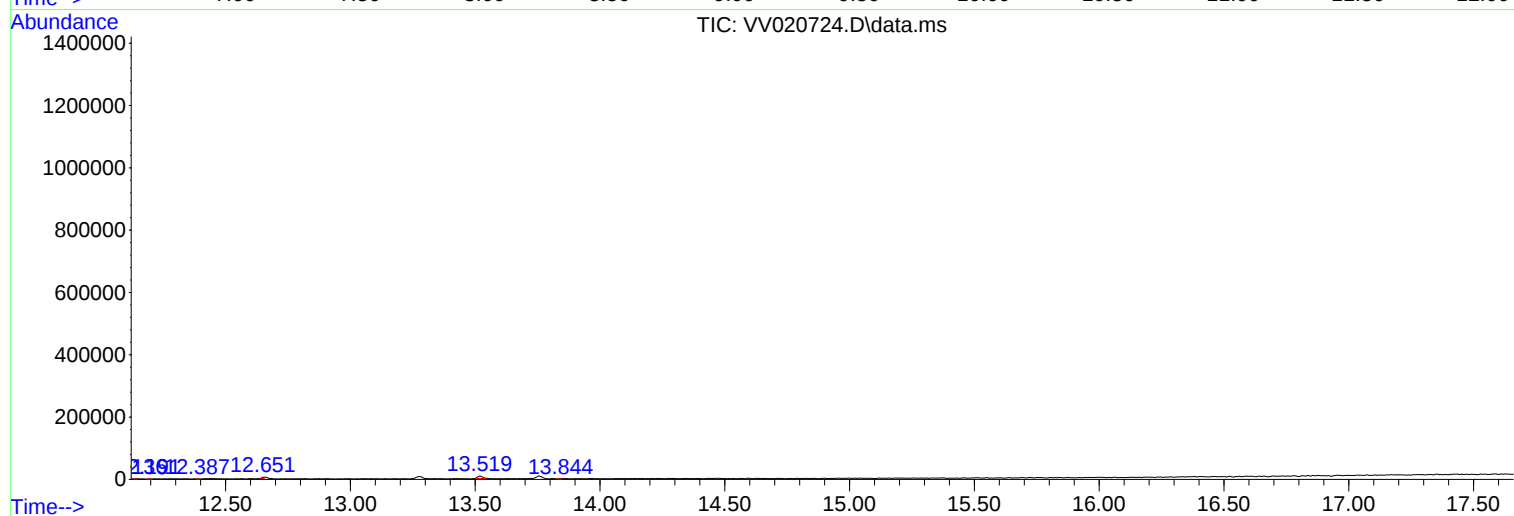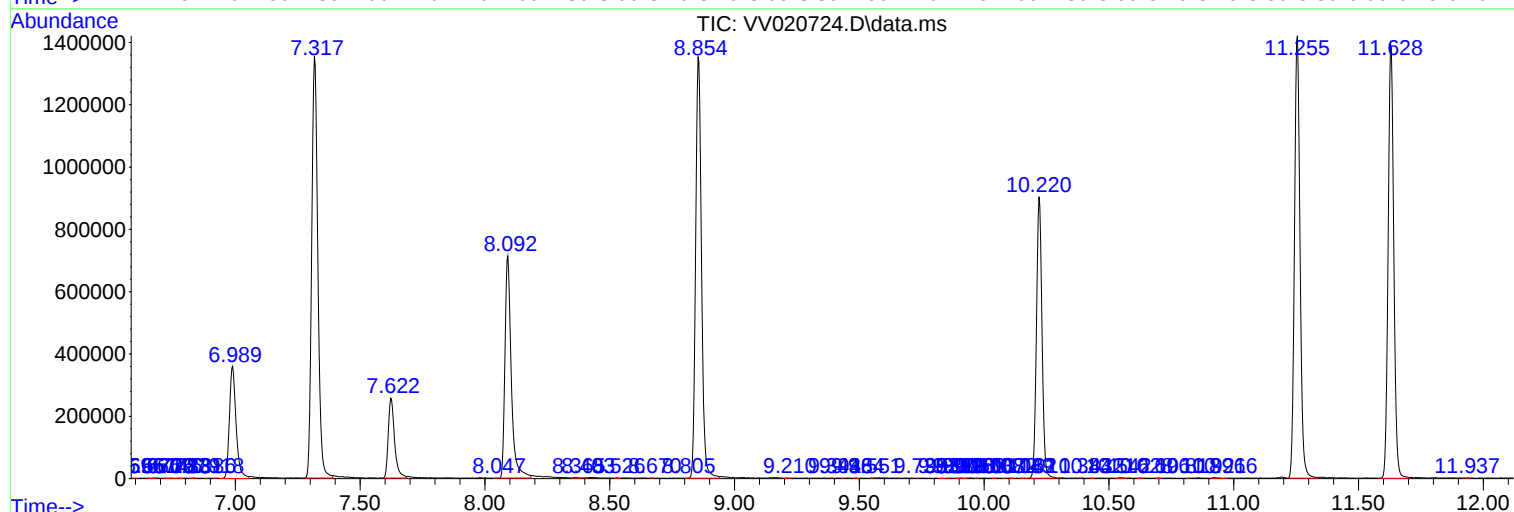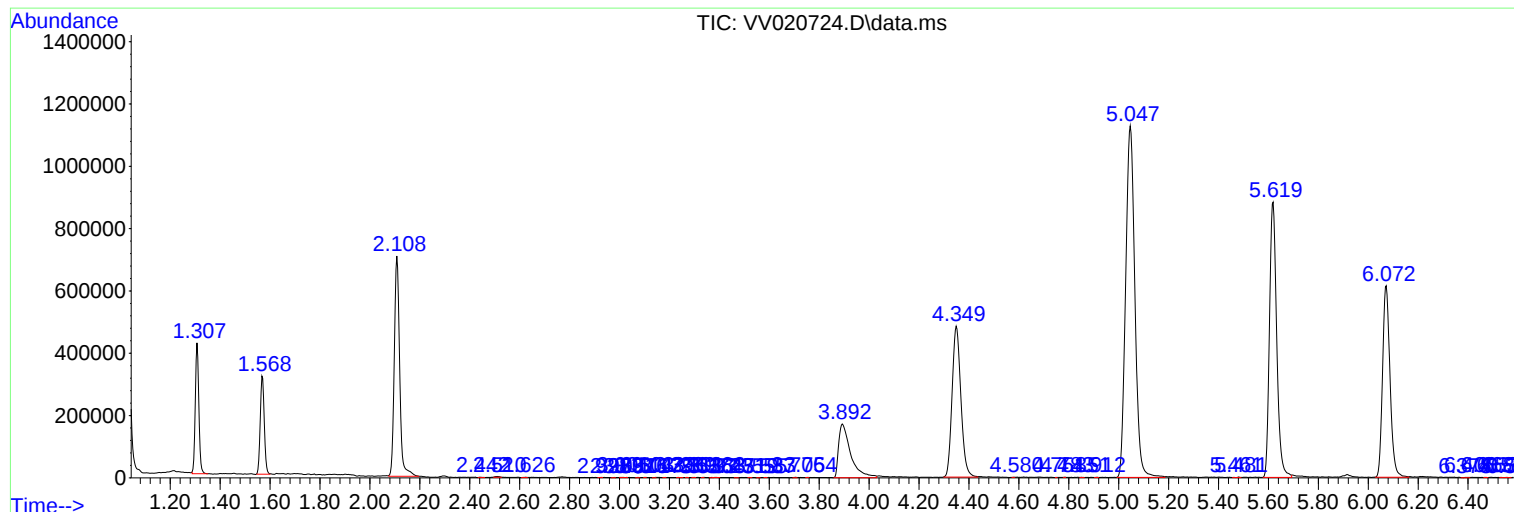

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020724.D
Acq On : 24 Mar 2021 10:06
Operator : SY/MD
Sample : VV0324MBL01
Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020724.D
Acq On : 24 Mar 2021 10:06
Operator : SY/MD
Sample : VV0324MBL01
Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
