

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020725.D
 Acq On : 24 Mar 2021 10:30
 Operator : SY/MD
 Sample : VV0324WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	399375	399363	14.08%	1.840%
2	1.571	158	165	175	rVB	303604	337996	11.91%	1.557%
3	2.108	323	332	365	rVB	688058	1044201	36.80%	4.811%
4	2.272	380	383	384	rBV2	1325	648	0.02%	0.003%
5	2.455	437	440	444	rBV2	892	764	0.03%	0.004%
6	2.497	449	453	454	rBV2	2055	1289	0.05%	0.006%
7	2.751	530	532	534	rBV2	506	266	0.01%	0.001%
8	2.773	535	539	542	rVV4	1242	1084	0.04%	0.005%
9	2.802	545	548	550	rBV2	581	369	0.01%	0.002%
10	2.815	550	552	554	rVV2	554	207	0.01%	0.001%
11	2.876	568	571	575	rBV3	616	351	0.01%	0.002%
12	2.912	578	582	585	rBV2	937	792	0.03%	0.004%
13	2.941	588	591	592	rBV	564	255	0.01%	0.001%
14	2.986	602	605	610	rBV3	633	519	0.02%	0.002%
15	3.037	619	621	623	rBV3	536	271	0.01%	0.001%
16	3.159	655	659	662	rVB3	647	491	0.02%	0.002%
17	3.175	662	664	667	rVB	532	254	0.01%	0.001%
18	3.198	670	671	673	rBV	478	182	0.01%	0.001%
19	3.275	691	695	696	rBV2	517	273	0.01%	0.001%
20	3.336	713	714	716	rBV2	419	177	0.01%	0.001%
21	3.349	716	718	721	rVV2	637	314	0.01%	0.001%
22	3.368	721	724	728	rVV3	985	824	0.03%	0.004%
23	3.397	729	733	737	rVB4	910	699	0.02%	0.003%
24	3.465	753	754	756	rVB	480	150	0.01%	0.001%
25	3.478	756	758	761	rVB3	630	306	0.01%	0.001%
26	3.506	764	767	768	rBV	679	307	0.01%	0.001%
27	3.597	793	795	798	rVB3	544	228	0.01%	0.001%
28	3.632	803	806	814	rVB4	848	890	0.03%	0.004%
29	3.664	814	816	817	rBV	547	212	0.01%	0.001%
30	3.674	817	819	823	rVB2	736	445	0.02%	0.002%
31	3.706	823	829	832	rBV3	996	882	0.03%	0.004%
32	3.754	840	844	848	rBV2	636	533	0.02%	0.002%
33	3.831	866	868	871	rVB2	366	175	0.01%	0.001%
34	3.851	871	874	876	rBV2	450	279	0.01%	0.001%
35	3.896	877	888	918	rBV	177887	536367	18.90%	2.471%
36	4.352	1012	1030	1056	rBV	479801	1170867	41.27%	5.395%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020725.D
 Acq On : 24 Mar 2021 10:30
 Operator : SY/MD
 Sample : VV0324WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.715	1140	1143	1144	rVB2	1019	439	0.02%	0.002%
38	4.725	1144	1146	1148	rBV2	862	540	0.02%	0.002%
39	4.757	1152	1156	1159	rBV5	631	550	0.02%	0.003%
40	4.802	1164	1170	1173	rBV5	1271	1233	0.04%	0.006%
41	4.892	1196	1198	1200	rBV2	752	300	0.01%	0.001%
42	4.928	1207	1209	1210	rBV2	557	234	0.01%	0.001%
43	4.979	1223	1225	1228	rBV3	675	331	0.01%	0.002%
44	5.050	1228	1247	1284	rBV2	1105551	2837290	100.00%	13.073%
45	5.333	1333	1335	1336	rBV2	1287	556	0.02%	0.003%
46	5.477	1378	1380	1384	rBV4	690	630	0.02%	0.003%
47	5.619	1412	1424	1453	rBV	850459	1726233	60.84%	7.954%
48	6.072	1550	1565	1592	rBV	613614	1252393	44.14%	5.771%
49	6.294	1631	1634	1637	rVB2	1232	754	0.03%	0.003%
50	6.313	1637	1640	1641	rBV3	589	356	0.01%	0.002%
51	6.400	1664	1667	1669	rBV3	1074	583	0.02%	0.003%
52	6.452	1682	1683	1686	rBV	349	215	0.01%	0.001%
53	6.484	1691	1693	1697	rBV3	573	514	0.02%	0.002%
54	6.500	1697	1698	1700	rBV	576	212	0.01%	0.001%
55	6.555	1713	1715	1716	rVB	581	148	0.01%	0.001%
56	6.606	1729	1731	1734	rVB3	819	469	0.02%	0.002%
57	6.635	1738	1740	1742	rVB3	792	380	0.01%	0.002%
58	6.648	1742	1744	1746	rBV	622	340	0.01%	0.002%
59	6.699	1758	1760	1763	rVB2	660	374	0.01%	0.002%
60	6.715	1763	1765	1766	rBV2	415	163	0.01%	0.001%
61	6.751	1774	1776	1778	rBV2	547	251	0.01%	0.001%
62	6.764	1778	1780	1784	rVB3	1136	569	0.02%	0.003%
63	6.786	1784	1787	1789	rBV2	630	295	0.01%	0.001%
64	6.796	1789	1790	1791	rBV2	521	184	0.01%	0.001%
65	6.854	1806	1808	1811	rBV3	1190	774	0.03%	0.004%
66	6.931	1830	1832	1835	rBV	510	332	0.01%	0.002%
67	6.989	1838	1850	1876	rBV	348340	640563	22.58%	2.951%
68	7.320	1940	1953	1979	rBV	1306508	2265770	79.86%	10.440%
69	7.625	2038	2048	2076	rBV	249787	442368	15.59%	2.038%
70	8.092	2181	2193	2225	rBV	724871	1265320	44.60%	5.830%
71	8.587	2344	2347	2349	rBV3	1068	619	0.02%	0.003%
72	8.693	2377	2380	2385	rBV4	913	660	0.02%	0.003%
73	8.857	2419	2431	2453	rBV	1331540	2152655	75.87%	9.919%
74	9.233	2544	2548	2551	rBV5	1006	917	0.03%	0.004%
75	9.452	2612	2616	2618	rBV4	979	728	0.03%	0.003%
76	9.493	2626	2629	2632	rBV3	845	472	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020725.D
 Acq On : 24 Mar 2021 10:30
 Operator : SY/MD
 Sample : VV0324WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	9.625	2668	2670	2672	rBV2	867	550	0.02%	0.003%
78	9.661	2678	2681	2684	rBV3	751	656	0.02%	0.003%
79	9.741	2704	2706	2707	rBV2	561	227	0.01%	0.001%
80	9.773	2712	2716	2718	rBV3	717	558	0.02%	0.003%
81	9.899	2750	2755	2758	rBV5	880	965	0.03%	0.004%
82	9.998	2784	2786	2789	rBV2	828	485	0.02%	0.002%
83	10.053	2800	2803	2808	rVB6	828	648	0.02%	0.003%
84	10.117	2821	2823	2828	rBV3	760	412	0.01%	0.002%
85	10.220	2840	2855	2883	rBV	865176	1363070	48.04%	6.281%
86	10.487	2936	2938	2940	rBV2	502	290	0.01%	0.001%
87	10.857	3049	3053	3055	rBV2	1812	1170	0.04%	0.005%
88	10.898	3061	3066	3068	rBV2	964	711	0.03%	0.003%
89	10.972	3086	3089	3092	rVB4	703	442	0.02%	0.002%
90	11.050	3111	3113	3115	rVB2	666	235	0.01%	0.001%
91	11.095	3126	3127	3129	rBV2	533	228	0.01%	0.001%
92	11.162	3145	3148	3150	rBV3	661	441	0.02%	0.002%
93	11.175	3150	3152	3154	rBV2	1115	612	0.02%	0.003%
94	11.255	3165	3177	3197	rBV	1362429	2112818	74.47%	9.735%
95	11.519	3257	3259	3263	rVB4	1265	706	0.02%	0.003%
96	11.632	3281	3294	3312	rBV	1343910	2113481	74.49%	9.738%
97	11.940	3387	3390	3392	rBV2	1124	722	0.03%	0.003%
98	12.242	3482	3484	3488	rBV4	845	493	0.02%	0.002%
99	12.844	3669	3671	3672	rBV2	800	422	0.01%	0.002%
100	15.438	4476	4478	4482	rBV3	2502	1779	0.06%	0.008%




Sum of corrected areas: 21703065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020725.D
Acq On : 24 Mar 2021 10:30
Operator : SY/MD
Sample : VV0324WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

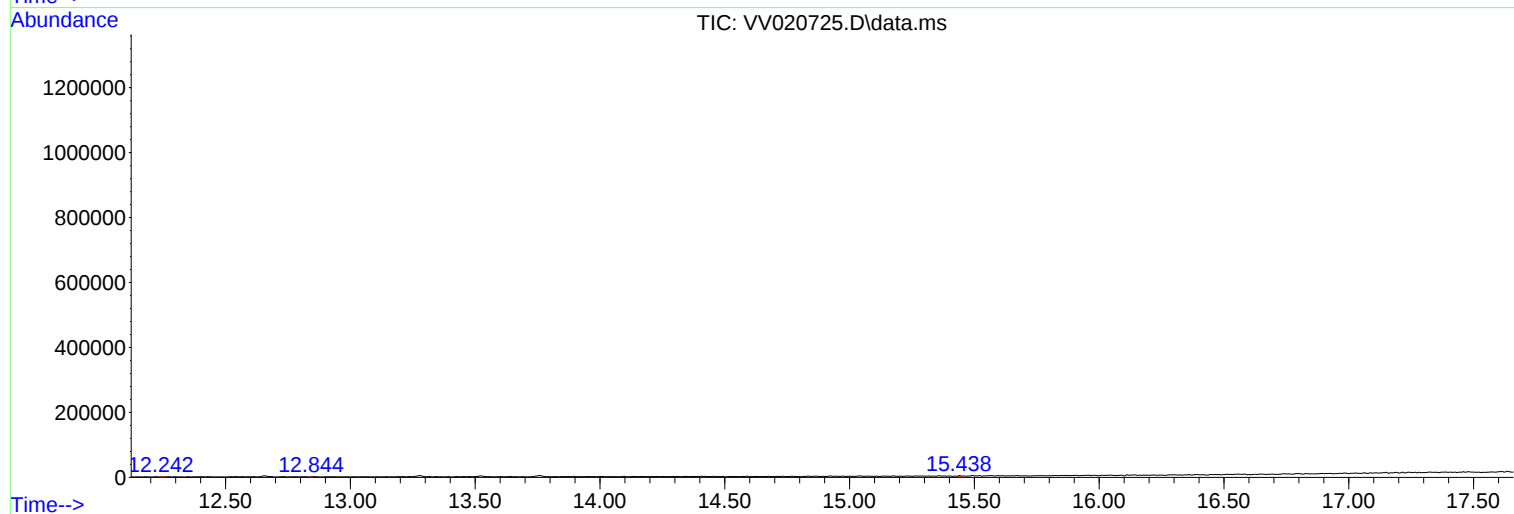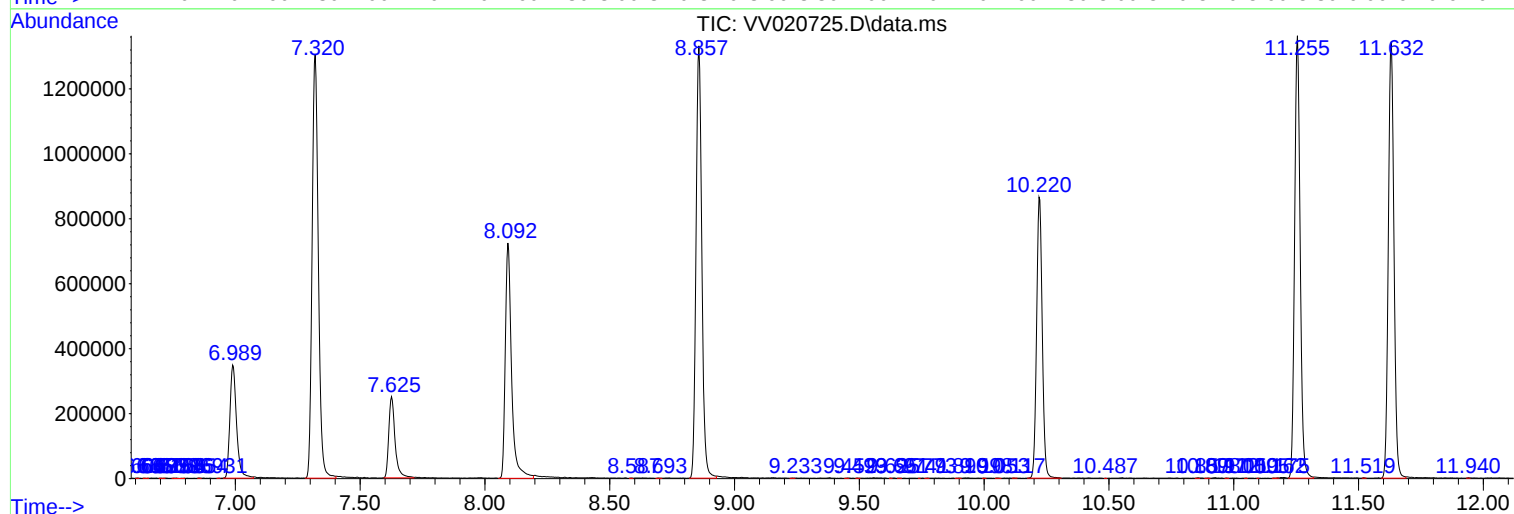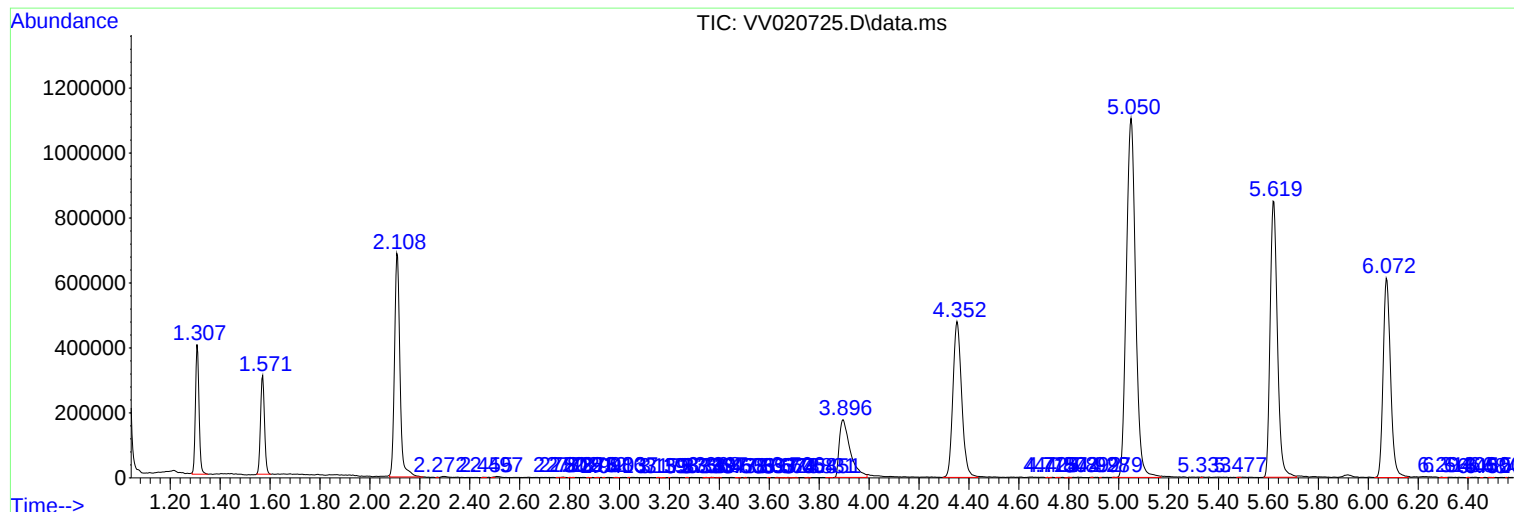

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020725.D
Acq On : 24 Mar 2021 10:30
Operator : SY/MD
Sample : VV0324WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020725.D
Acq On : 24 Mar 2021 10:30
Operator : SY/MD
Sample : VV0324WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
