

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020728.D
 Acq On : 24 Mar 2021 11:46
 Operator : SY/MD
 Sample : M1783-04DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G10DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020728.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	94	rVB	386266	381705	12.02%	1.613%
2	1.568	158	164	174	rBV	292206	321796	10.14%	1.360%
3	2.108	322	332	359	rVB	663209	1005491	31.68%	4.250%
4	2.487	447	450	451	rBV3	968	498	0.02%	0.002%
5	2.548	467	469	471	rVB	521	203	0.01%	0.001%
6	2.561	471	473	477	rVV3	712	451	0.01%	0.002%
7	2.584	477	480	482	rVB3	1162	503	0.02%	0.002%
8	2.600	482	485	489	rVB4	731	483	0.02%	0.002%
9	2.641	496	498	501	rBV3	519	309	0.01%	0.001%
10	2.658	501	503	504	rBV	406	131	0.00%	0.001%
11	2.725	522	524	528	rVB4	933	588	0.02%	0.002%
12	2.741	528	529	531	rVB	709	188	0.01%	0.001%
13	2.751	531	532	533	rBV	671	248	0.01%	0.001%
14	2.760	533	535	538	rBV2	676	394	0.01%	0.002%
15	2.976	599	602	605	rVB3	907	506	0.02%	0.002%
16	2.998	606	609	613	rVV4	658	464	0.01%	0.002%
17	3.014	613	614	616	rVB2	603	219	0.01%	0.001%
18	3.047	622	624	630	rBV4	773	651	0.02%	0.003%
19	3.117	643	646	650	rBV2	863	520	0.02%	0.002%
20	3.137	650	652	654	rBV2	608	287	0.01%	0.001%
21	3.182	664	666	670	rVB3	677	383	0.01%	0.002%
22	3.207	670	674	676	rBV3	817	643	0.02%	0.003%
23	3.294	699	701	702	rBV	345	150	0.00%	0.001%
24	3.307	702	705	707	rVB2	688	341	0.01%	0.001%
25	3.384	725	729	730	rBV	448	251	0.01%	0.001%
26	3.394	730	732	735	rBV2	521	433	0.01%	0.002%
27	3.442	745	747	751	rVB3	802	499	0.02%	0.002%
28	3.471	754	756	758	rBV	460	198	0.01%	0.001%
29	3.500	763	765	767	rBV	607	258	0.01%	0.001%
30	3.539	774	777	781	rBV2	355	382	0.01%	0.002%
31	3.561	781	784	785	rVV	494	256	0.01%	0.001%
32	3.596	794	795	798	rVB	739	251	0.01%	0.001%
33	3.619	798	802	803	rBV	434	278	0.01%	0.001%
34	3.641	806	809	811	rVV2	597	307	0.01%	0.001%
35	3.654	811	813	815	rBV	491	218	0.01%	0.001%
36	3.699	824	827	828	rVB2	203	115	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020728.D
 Acq On : 24 Mar 2021 11:46
 Operator : SY/MD
 Sample : M1783-04DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G10DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

37	3.709	828	830	834	rBV3	635	495	0.02%	0.002%
38	3.725	834	835	838	rBV	511	228	0.01%	0.001%
39	3.770	842	849	850	rBV3	1104	1114	0.04%	0.005%
40	3.825	864	866	868	rVB	571	230	0.01%	0.001%
41	3.889	876	886	927	rBV	176003	521061	16.41%	2.202%
42	4.256	998	1000	1004	rBV5	955	786	0.02%	0.003%
43	4.352	1013	1030	1053	rBV	466085	1136504	35.80%	4.804%
44	4.757	1154	1156	1159	rVB3	715	373	0.01%	0.002%
45	4.818	1172	1175	1178	rBV3	1284	1011	0.03%	0.004%
46	4.895	1197	1199	1202	rBV2	572	339	0.01%	0.001%
47	4.928	1206	1209	1210	rBV	425	217	0.01%	0.001%
48	5.050	1229	1247	1262	rBV2	1074337	2773462	87.37%	11.723%
49	5.487	1378	1383	1385	rBV6	1283	1309	0.04%	0.006%
50	5.558	1404	1405	1409	rBV4	641	262	0.01%	0.001%
51	5.619	1412	1424	1450	rBV	861690	1723418	54.29%	7.285%
52	5.918	1508	1517	1525	rBV7	6598	12334	0.39%	0.052%
53	6.072	1550	1565	1593	rBV	589776	1211307	38.16%	5.120%
54	6.407	1667	1669	1670	rBV2	915	401	0.01%	0.002%
55	6.616	1731	1734	1736	rBV3	602	446	0.01%	0.002%
56	6.645	1740	1743	1745	rBV3	977	526	0.02%	0.002%
57	6.715	1761	1765	1767	rBV4	955	611	0.02%	0.003%
58	6.751	1773	1776	1778	rBV2	380	202	0.01%	0.001%
59	6.763	1778	1780	1782	rBV2	755	477	0.02%	0.002%
60	6.792	1786	1789	1790	rBV	761	404	0.01%	0.002%
61	6.825	1797	1799	1801	rBV2	639	254	0.01%	0.001%
62	6.882	1816	1817	1821	rVB	719	319	0.01%	0.001%
63	6.989	1839	1850	1875	rBV2	336578	615927	19.40%	2.603%
64	7.249	1928	1931	1934	rVB2	1832	1171	0.04%	0.005%
65	7.320	1941	1953	1977	rBV	1277186	2190183	69.00%	9.258%
66	7.625	2036	2048	2073	rBV	245435	433392	13.65%	1.832%
67	8.091	2183	2193	2227	rBV	682204	1191025	37.52%	5.034%
68	8.635	2360	2362	2364	rBV2	912	510	0.02%	0.002%
69	8.763	2400	2402	2404	rVB2	564	204	0.01%	0.001%
70	8.857	2418	2431	2436	rBV	1377961	2269242	71.49%	9.592%
71	9.239	2548	2550	2552	rBV	776	474	0.01%	0.002%
72	9.294	2565	2567	2569	rBV3	926	468	0.01%	0.002%
73	9.316	2572	2574	2576	rVB2	549	210	0.01%	0.001%
74	9.410	2600	2603	2607	rBV5	883	898	0.03%	0.004%
75	9.722	2695	2700	2701	rBV3	756	623	0.02%	0.003%
76	9.796	2720	2723	2725	rBV2	762	467	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020728.D
 Acq On : 24 Mar 2021 11:46
 Operator : SY/MD
 Sample : M1783-04DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G10DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	9.969	2773	2777	2783	rVB4	1273	1082	0.03%	0.005%
78	10.050	2798	2802	2805	rBV5	710	552	0.02%	0.002%
79	10.220	2843	2855	2873	rBV	839552	1320469	41.60%	5.582%
80	10.516	2944	2947	2950	rBV4	1158	690	0.02%	0.003%
81	10.641	2982	2986	2988	rBV2	603	364	0.01%	0.002%
82	10.664	2992	2993	2998	rVB	473	224	0.01%	0.001%
83	10.693	2998	3002	3006	rBV5	457	365	0.01%	0.002%
84	10.712	3006	3008	3010	rBV3	553	254	0.01%	0.001%
85	10.776	3025	3028	3033	rBV4	854	906	0.03%	0.004%
86	10.815	3036	3040	3043	rBV3	632	454	0.01%	0.002%
87	10.831	3043	3045	3048	rBV3	744	383	0.01%	0.002%
88	10.998	3094	3097	3098	rBV2	682	415	0.01%	0.002%
89	11.188	3147	3156	3166	rBV2	67606	108346	3.41%	0.458%
90	11.255	3166	3177	3208	rVB2	1454111	2989341	94.17%	12.636%
91	11.631	3281	3294	3321	rBV3	1501666	3174301	100.00%	13.418%
92	12.143	3452	3453	3459	rVB4	1052	860	0.03%	0.004%
93	12.172	3459	3462	3464	rBV2	918	646	0.02%	0.003%
94	12.291	3496	3499	3503	rBV3	974	645	0.02%	0.003%
95	12.506	3564	3566	3569	rBV3	614	332	0.01%	0.001%
96	12.892	3684	3686	3687	rBV	1111	462	0.01%	0.002%
97	13.056	3735	3737	3739	rBV2	808	406	0.01%	0.002%
98	13.136	3760	3762	3765	rBV2	976	591	0.02%	0.002%
99	13.268	3794	3803	3823	rBV2	122054	196997	6.21%	0.833%
100	13.754	3947	3954	3964	rVB2	30583	45168	1.42%	0.191%


Sum of corrected areas: 23657735

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020728.D
Acq On : 24 Mar 2021 11:46
Operator : SY/MD
Sample : M1783-04DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G10DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

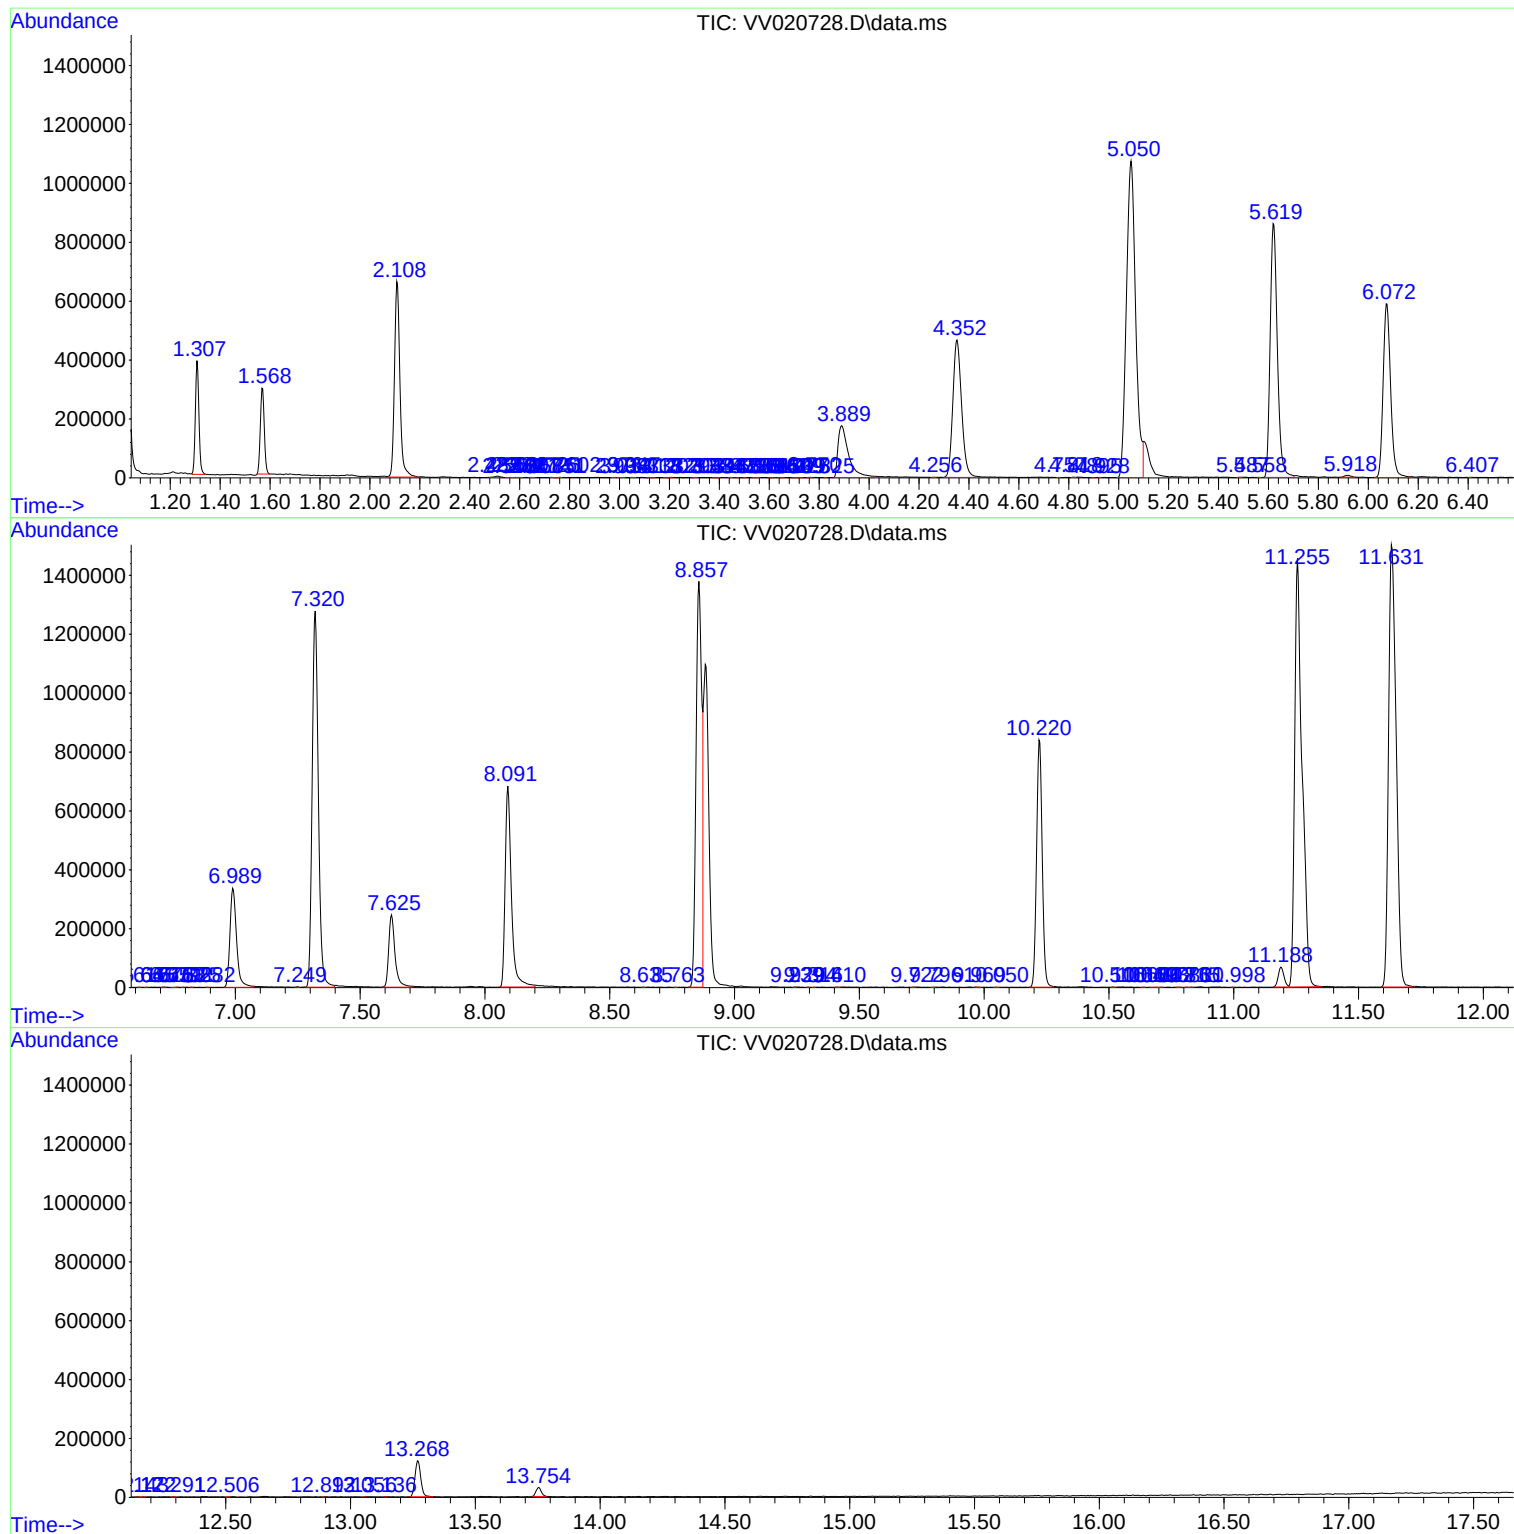

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020728.D
Acq On : 24 Mar 2021 11:46
Operator : SY/MD
Sample : M1783-04DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G10DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020728.D
Acq On : 24 Mar 2021 11:46
Operator : SY/MD
Sample : M1783-04DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G10DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
