

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020729.D
 Acq On : 24 Mar 2021 12:09
 Operator : SY/MD
 Sample : M1783-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	94	rVB	375585	371036	13.88%	1.792%
2	1.568	157	164	177	rBV	291987	321316	12.02%	1.552%
3	2.108	322	332	362	rVB	648574	970873	36.31%	4.690%
4	2.738	524	528	531	rBV3	999	843	0.03%	0.004%
5	2.847	559	562	566	rBV3	633	519	0.02%	0.003%
6	2.896	576	577	578	rVB	534	103	0.00%	0.000%
7	2.979	601	603	605	rVB	535	193	0.01%	0.001%
8	2.995	605	608	612	rVB4	662	470	0.02%	0.002%
9	3.027	612	618	620	rBV3	1029	910	0.03%	0.004%
10	3.191	667	669	671	rBV2	382	168	0.01%	0.001%
11	3.220	676	678	679	rBV	469	212	0.01%	0.001%
12	3.253	686	688	690	rBV2	446	272	0.01%	0.001%
13	3.288	696	699	701	rBV2	769	464	0.02%	0.002%
14	3.333	711	713	716	rBV2	553	354	0.01%	0.002%
15	3.378	722	727	731	rVB4	777	617	0.02%	0.003%
16	3.413	737	738	741	rVB2	655	338	0.01%	0.002%
17	3.439	741	746	752	rBV5	820	985	0.04%	0.005%
18	3.465	752	754	761	rVB4	668	461	0.02%	0.002%
19	3.500	761	765	766	rBV2	476	361	0.01%	0.002%
20	3.526	771	773	778	rVB2	671	415	0.02%	0.002%
21	3.548	778	780	781	rBV	570	241	0.01%	0.001%
22	3.590	790	793	796	rBV2	512	380	0.01%	0.002%
23	3.635	805	807	812	rBV4	724	452	0.02%	0.002%
24	3.677	819	820	821	rVB	340	66	0.00%	0.000%
25	3.693	821	825	828	rBV3	1059	942	0.04%	0.005%
26	3.719	831	833	835	rVV2	307	136	0.01%	0.001%
27	3.761	845	846	848	rBV2	407	215	0.01%	0.001%
28	3.802	852	859	861	rBV3	789	926	0.03%	0.004%
29	3.828	865	867	869	rBV2	571	297	0.01%	0.001%
30	3.847	871	873	874	rBV	860	320	0.01%	0.002%
31	3.892	875	887	932	rBV3	209252	696751	26.06%	3.366%
32	4.352	1015	1030	1059	rBV	470125	1234128	46.16%	5.962%
33	4.786	1163	1165	1166	rBV2	677	225	0.01%	0.001%
34	4.831	1175	1179	1183	rBV5	1185	1000	0.04%	0.005%
35	4.953	1212	1217	1221	rBV5	1120	887	0.03%	0.004%
36	4.973	1221	1223	1225	rBV3	645	263	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020729.D
 Acq On : 24 Mar 2021 12:09
 Operator : SY/MD
 Sample : M1783-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.050	1229	1247	1291	rBV2	1036253	2673628	100.00%	12.915%
38	5.423	1361	1363	1370	rVB5	1147	994	0.04%	0.005%
39	5.619	1411	1424	1451	rBV	813358	1622007	60.67%	7.835%
40	6.072	1552	1565	1591	rBV	577845	1167305	43.66%	5.639%
41	6.487	1692	1694	1697	rBV4	604	484	0.02%	0.002%
42	6.571	1716	1720	1722	rBV	814	528	0.02%	0.003%
43	6.654	1744	1746	1747	rBV	696	275	0.01%	0.001%
44	6.687	1754	1756	1759	rBV2	680	295	0.01%	0.001%
45	6.738	1770	1772	1773	rBV2	558	216	0.01%	0.001%
46	6.777	1782	1784	1787	rBV3	718	324	0.01%	0.002%
47	6.818	1794	1797	1801	rVB4	886	786	0.03%	0.004%
48	6.838	1801	1803	1805	rBV3	815	440	0.02%	0.002%
49	6.895	1819	1821	1823	rBV2	808	332	0.01%	0.002%
50	6.989	1838	1850	1874	rBV	324011	596081	22.29%	2.879%
51	7.320	1941	1953	1973	rBV	1217826	2107942	78.84%	10.183%
52	7.625	2038	2048	2070	rBV	236649	407641	15.25%	1.969%
53	7.844	2114	2116	2121	rBV5	1228	943	0.04%	0.005%
54	7.915	2134	2138	2140	rBV4	1359	1172	0.04%	0.006%
55	8.034	2172	2175	2177	rBV2	1141	599	0.02%	0.003%
56	8.092	2183	2193	2228	rBV	657566	1173711	43.90%	5.670%
57	8.532	2328	2330	2333	rBV5	875	489	0.02%	0.002%
58	8.593	2346	2349	2352	rBV2	901	664	0.02%	0.003%
59	8.686	2375	2378	2381	rBV4	797	752	0.03%	0.004%
60	8.757	2398	2400	2403	rBV3	826	475	0.02%	0.002%
61	8.793	2408	2411	2416	rVB4	944	905	0.03%	0.004%
62	8.857	2416	2431	2459	rBV	1248729	2034771	76.11%	9.829%
63	9.346	2580	2583	2584	rBV3	598	366	0.01%	0.002%
64	9.371	2588	2591	2593	rBV2	740	444	0.02%	0.002%
65	9.542	2642	2644	2645	rBV	537	255	0.01%	0.001%
66	9.683	2684	2688	2691	rBV3	1070	752	0.03%	0.004%
67	9.728	2697	2702	2705	rBV4	800	816	0.03%	0.004%
68	9.764	2711	2713	2717	rVB4	1047	678	0.03%	0.003%
69	9.860	2741	2743	2744	rBV	416	124	0.00%	0.001%
70	9.940	2764	2768	2771	rBV3	1473	1288	0.05%	0.006%
71	9.995	2782	2785	2787	rBV3	929	532	0.02%	0.003%
72	10.066	2804	2807	2808	rBV	632	430	0.02%	0.002%
73	10.153	2832	2834	2837	rBV2	429	308	0.01%	0.001%
74	10.220	2843	2855	2883	rBV	804691	1265307	47.33%	6.112%
75	10.645	2981	2987	2988	rBV3	872	800	0.03%	0.004%
76	10.747	3017	3019	3022	rBV3	794	533	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020729.D
 Acq On : 24 Mar 2021 12:09
 Operator : SY/MD
 Sample : M1783-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G07

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.921	3069	3073	3075	rBV	1009	730	0.03%	0.004%
78	10.998	3094	3097	3099	rVB	1061	493	0.02%	0.002%
79	11.095	3124	3127	3128	rBV	820	393	0.01%	0.002%
80	11.255	3165	3177	3203	rBV	1286188	1990781	74.46%	9.617%
81	11.632	3281	3294	3316	rBV	1286967	2022989	75.66%	9.772%
82	11.963	3392	3397	3400	rBV4	1266	1225	0.05%	0.006%
83	12.188	3464	3467	3471	rVB3	1298	765	0.03%	0.004%
84	12.587	3584	3591	3593	rBV4	958	1177	0.04%	0.006%
85	13.278	3797	3806	3815	rVB4	4721	7716	0.29%	0.037%
86	14.332	4132	4134	4136	rBV3	1300	616	0.02%	0.003%




Sum of corrected areas: 20701416

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020729.D
Acq On : 24 Mar 2021 12:09
Operator : SY/MD
Sample : M1783-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

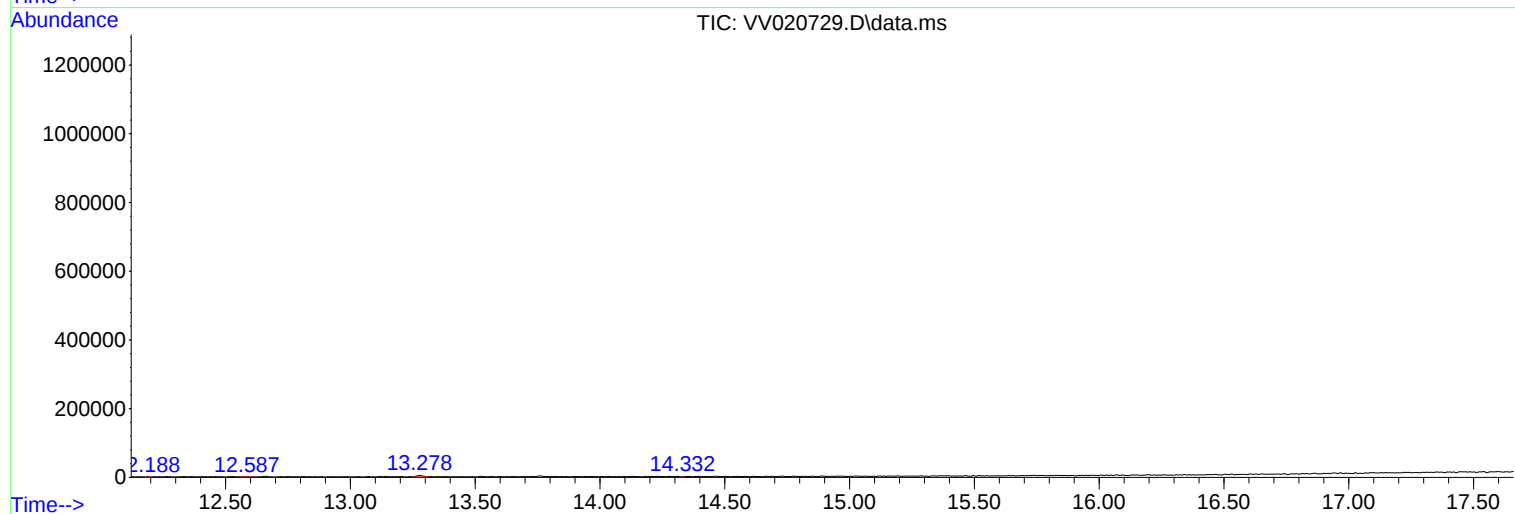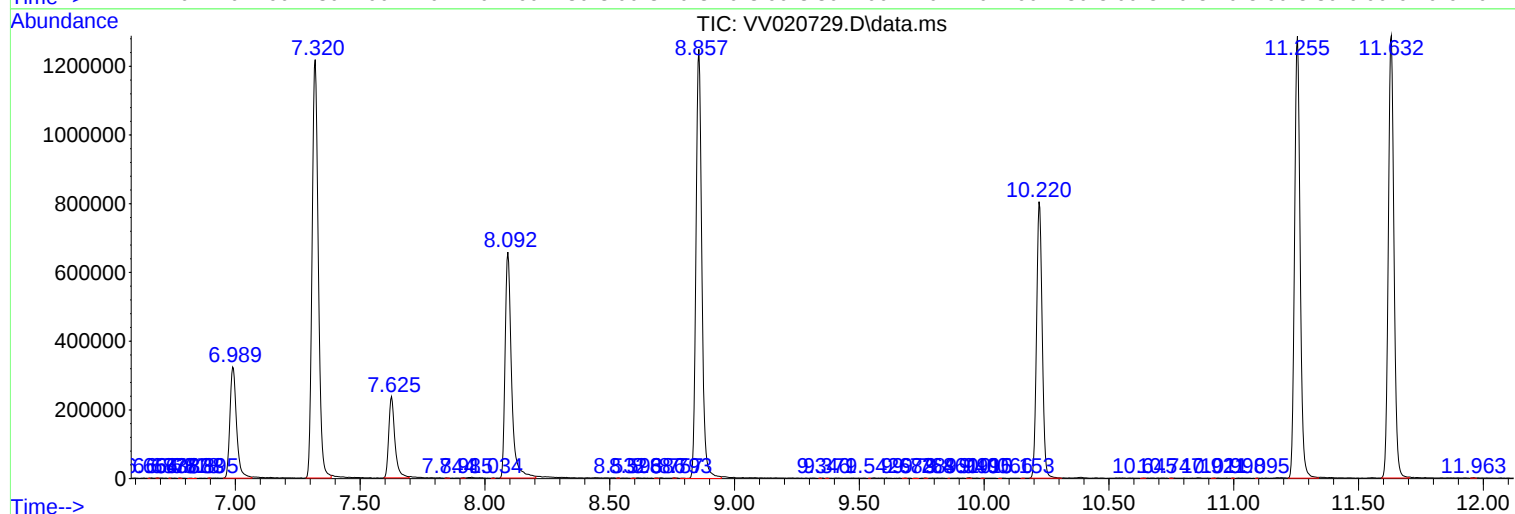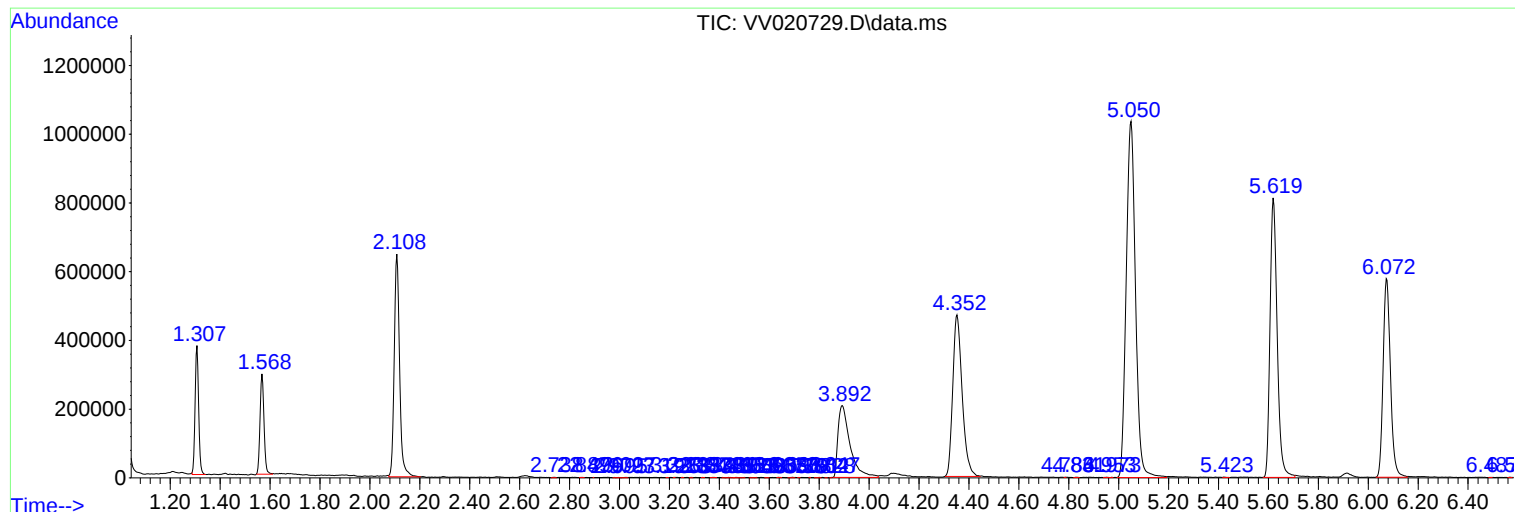

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020729.D
Acq On : 24 Mar 2021 12:09
Operator : SY/MD
Sample : M1783-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020729.D
Acq On : 24 Mar 2021 12:09
Operator : SY/MD
Sample : M1783-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------