

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020732.D
 Acq On : 24 Mar 2021 13:19
 Operator : SY/MD
 Sample : M1783-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	341649	343046	2.23%	0.767%
2	1.571	158	165	174	rBV	262682	288056	1.87%	0.644%
3	2.111	323	333	347	rBV	583080	869955	5.66%	1.945%
4	2.278	383	385	387	rBV2	1086	648	0.00%	0.001%
5	2.455	437	440	443	rBV2	1061	669	0.00%	0.001%
6	2.507	451	456	457	rBV5	1569	1346	0.01%	0.003%
7	2.584	477	480	483	rBV3	893	650	0.00%	0.001%
8	2.677	505	509	512	rVB3	891	681	0.00%	0.002%
9	2.706	513	518	521	rVB5	940	759	0.00%	0.002%
10	2.735	524	527	530	rBV3	639	387	0.00%	0.001%
11	2.770	534	538	540	rBV4	904	555	0.00%	0.001%
12	2.854	560	564	568	rBV2	822	830	0.01%	0.002%
13	2.957	594	596	600	rVB3	797	529	0.00%	0.001%
14	2.999	606	609	611	rBV3	833	589	0.00%	0.001%
15	3.056	624	627	630	rBV3	830	546	0.00%	0.001%
16	3.069	630	631	634	rVB2	586	278	0.00%	0.001%
17	3.092	636	638	642	rBV3	1014	513	0.00%	0.001%
18	3.130	648	650	653	rBV	914	545	0.00%	0.001%
19	3.236	681	683	686	rVB2	762	346	0.00%	0.001%
20	3.262	686	691	693	rBV3	862	639	0.00%	0.001%
21	3.285	696	698	703	rVB3	715	569	0.00%	0.001%
22	3.314	703	707	708	rBV	595	334	0.00%	0.001%
23	3.423	739	741	743	rVB2	1012	408	0.00%	0.001%
24	3.439	743	746	751	rBV3	481	421	0.00%	0.001%
25	3.462	751	753	756	rBV3	789	399	0.00%	0.001%
26	3.532	771	775	776	rBV2	701	447	0.00%	0.001%
27	3.564	782	785	788	rBV3	758	366	0.00%	0.001%
28	3.590	788	793	797	rBV4	639	613	0.00%	0.001%
29	3.632	801	806	809	rBV5	933	769	0.01%	0.002%
30	3.661	812	815	816	rBV3	727	296	0.00%	0.001%
31	3.735	832	838	841	rBV3	928	814	0.01%	0.002%
32	3.835	866	869	871	rBV	608	387	0.00%	0.001%
33	3.892	874	887	922	rBV2	197591	646163	4.20%	1.445%
34	4.352	1016	1030	1060	rVB	412889	1015069	6.60%	2.269%
35	4.767	1157	1159	1161	rVB2	1414	585	0.00%	0.001%
36	4.786	1161	1165	1167	rBV3	839	642	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020732.D
 Acq On : 24 Mar 2021 13:19
 Operator : SY/MD
 Sample : M1783-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.870	1188	1191	1193	rBV2	590	351	0.00%	0.001%
38	4.889	1196	1197	1199	rVB	779	277	0.00%	0.001%
39	4.902	1199	1201	1205	rBV5	791	574	0.00%	0.001%
40	4.921	1205	1207	1209	rBV	801	439	0.00%	0.001%
41	5.050	1229	1247	1286	rBV2	958308	2592521	16.86%	5.796%
42	5.381	1347	1350	1355	rBV6	1387	1166	0.01%	0.003%
43	5.619	1412	1424	1450	rBV	785249	1578855	10.27%	3.530%
44	5.915	1508	1516	1523	rBV7	10957	19900	0.13%	0.044%
45	6.021	1545	1549	1552	rBV5	1209	1108	0.01%	0.002%
46	6.076	1552	1566	1595	rVV	526363	1082273	7.04%	2.420%
47	6.317	1637	1641	1647	rVV7	1025	1178	0.01%	0.003%
48	6.349	1648	1651	1655	rVB3	867	606	0.00%	0.001%
49	6.529	1705	1707	1709	rVB	823	285	0.00%	0.001%
50	6.577	1717	1722	1725	rBV2	757	764	0.00%	0.002%
51	6.632	1736	1739	1740	rBV3	456	282	0.00%	0.001%
52	6.677	1750	1753	1755	rBV2	1120	632	0.00%	0.001%
53	6.741	1770	1773	1774	rBV	581	292	0.00%	0.001%
54	6.751	1774	1776	1777	rBV2	808	303	0.00%	0.001%
55	6.841	1802	1804	1809	rVB3	981	795	0.01%	0.002%
56	6.873	1812	1814	1818	rBV	582	328	0.00%	0.001%
57	6.892	1818	1820	1824	rVB4	878	558	0.00%	0.001%
58	6.912	1824	1826	1828	rBV	714	425	0.00%	0.001%
59	6.934	1831	1833	1836	rBV2	915	581	0.00%	0.001%
60	6.989	1839	1850	1872	rBV	296981	549599	3.57%	1.229%
61	7.320	1941	1953	1975	rBV	1114474	1935750	12.59%	4.328%
62	7.625	2038	2048	2071	rBV	213785	381108	2.48%	0.852%
63	7.873	2122	2125	2127	rBV4	961	607	0.00%	0.001%
64	8.043	2176	2178	2181	rBV4	696	430	0.00%	0.001%
65	8.092	2183	2193	2225	rBV	612215	1067997	6.95%	2.388%
66	8.638	2360	2363	2367	rBV3	780	709	0.00%	0.002%
67	8.741	2393	2395	2398	rBV4	963	632	0.00%	0.001%
68	8.757	2398	2400	2403	rVB3	1331	706	0.00%	0.002%
69	8.857	2419	2431	2434	rBV	1307445	1831401	11.91%	4.095%
70	9.426	2605	2608	2610	rBV3	887	650	0.00%	0.001%
71	9.455	2614	2617	2622	rVB4	1603	1250	0.01%	0.003%
72	9.551	2643	2647	2652	rBV4	1062	1254	0.01%	0.003%
73	9.625	2668	2670	2677	rBV5	1036	1225	0.01%	0.003%
74	9.789	2718	2721	2725	rBV2	1053	697	0.00%	0.002%
75	9.812	2725	2728	2732	rVB4	858	727	0.00%	0.002%
76	9.931	2763	2765	2766	rBV	869	345	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020732.D
 Acq On : 24 Mar 2021 13:19
 Operator : SY/MD
 Sample : M1783-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.117	2821	2823	2827	rBV4	556	338	0.00%	0.001%
78	10.153	2831	2834	2837	rVB4	621	441	0.00%	0.001%
79	10.220	2841	2855	2874	rBV	746127	1183648	7.70%	2.646%
80	10.381	2902	2905	2916	rBV8	1518	2085	0.01%	0.005%
81	10.487	2935	2938	2940	rBV4	1016	652	0.00%	0.001%
82	10.532	2950	2952	2955	rBV3	867	674	0.00%	0.002%
83	10.834	3044	3046	3048	rBV	650	422	0.00%	0.001%
84	10.931	3072	3076	3078	rBV3	846	685	0.00%	0.002%
85	10.992	3092	3095	3098	rBV3	643	418	0.00%	0.001%
86	11.030	3102	3107	3110	rBV4	913	923	0.01%	0.002%
87	11.085	3120	3124	3126	rBV3	801	565	0.00%	0.001%
88	11.114	3131	3133	3136	rVB2	603	390	0.00%	0.001%
89	11.188	3145	3156	3166	rBV	331560	511946	3.33%	1.145%
90	11.278	3167	3184	3204	rVB2	3183169	6729941	43.77%	15.047%
91	11.500	3250	3253	3257	rBV5	1692	1648	0.01%	0.004%
92	11.648	3281	3299	3324	rBV2	9161204	15377278	100.00%	34.380%
93	12.175	3460	3463	3467	rVB4	1171	738	0.00%	0.002%
94	12.407	3527	3535	3547	rVB3	15182	24743	0.16%	0.055%
95	12.644	3599	3609	3628	rBV2	74489	128636	0.84%	0.288%
96	13.165	3769	3771	3772	rBV	1219	525	0.00%	0.001%
97	13.268	3790	3803	3825	rBV	2774606	4151633	27.00%	9.282%
98	13.751	3942	3953	3974	rVB	1348065	2031896	13.21%	4.543%
99	14.159	4074	4080	4091	rVB2	22057	32099	0.21%	0.072%
100	15.406	4458	4468	4481	rVB2	197203	305696	1.99%	0.683%




Sum of corrected areas: 44727449

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020732.D
Acq On : 24 Mar 2021 13:19
Operator : SY/MD
Sample : M1783-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

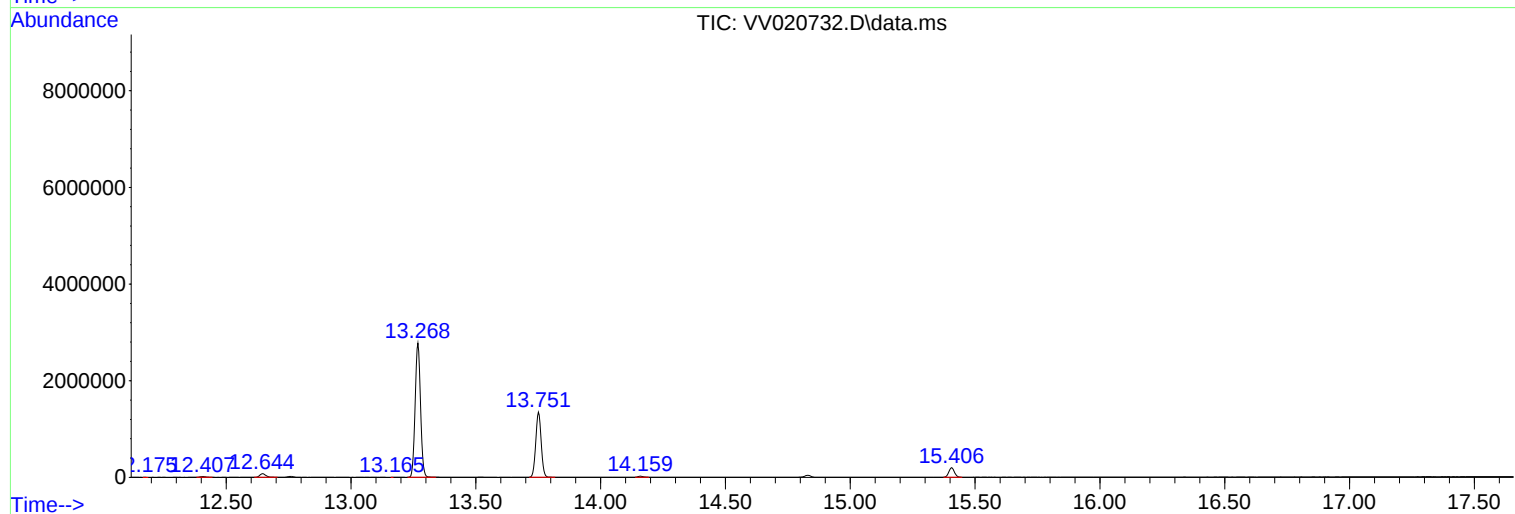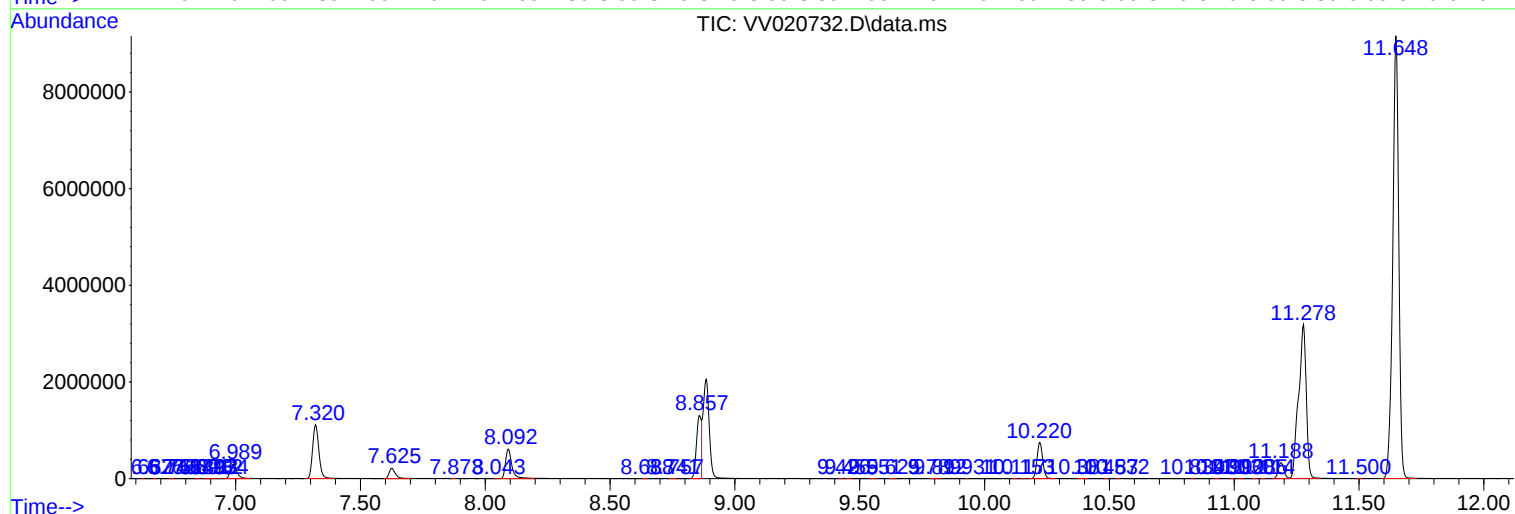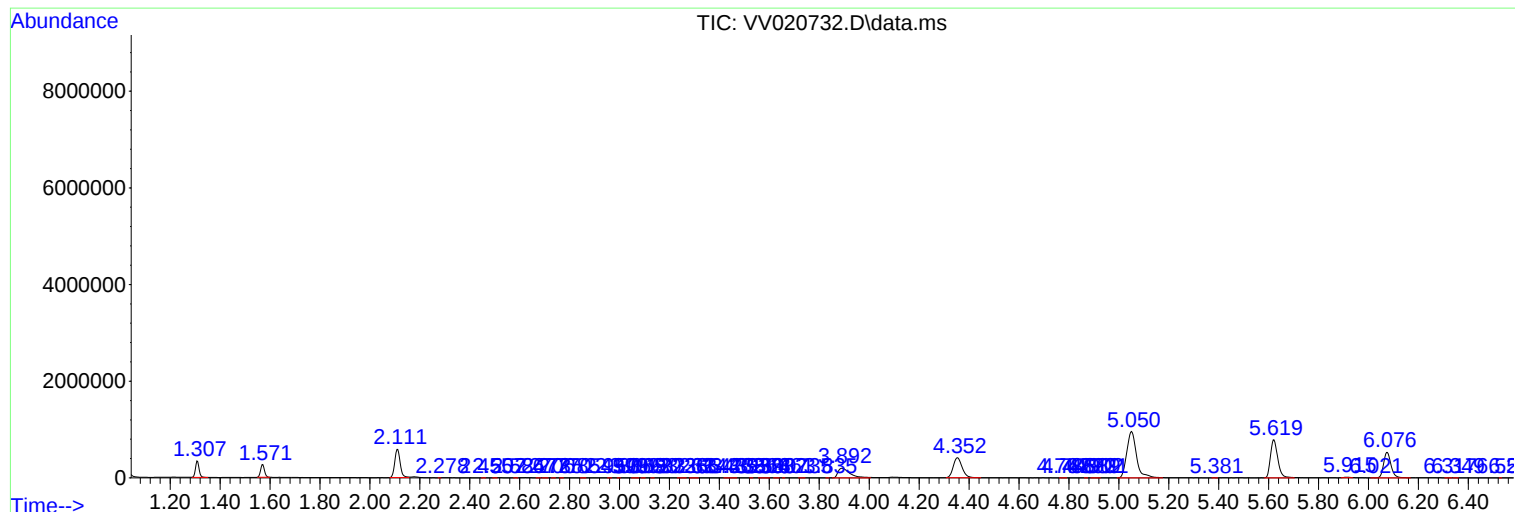

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020732.D
Acq On : 24 Mar 2021 13:19
Operator : SY/MD
Sample : M1783-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020732.D
Acq On : 24 Mar 2021 13:19
Operator : SY/MD
Sample : M1783-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
