

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020733.D
 Acq On : 24 Mar 2021 13:43
 Operator : SY/MD
 Sample : M1783-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	368474	374812	14.28%	1.908%
2	1.568	158	164	175	rVB	280603	310229	11.82%	1.580%
3	2.108	322	332	352	rBV	624799	940046	35.83%	4.787%
4	2.735	525	527	530	rBV2	535	212	0.01%	0.001%
5	2.764	534	536	538	rBV3	636	309	0.01%	0.002%
6	2.973	599	601	603	rVB2	501	183	0.01%	0.001%
7	3.034	619	620	624	rVB4	503	284	0.01%	0.001%
8	3.130	647	650	653	rBV3	666	459	0.02%	0.002%
9	3.150	653	656	661	rVV3	764	528	0.02%	0.003%
10	3.198	669	671	676	rVB3	593	375	0.01%	0.002%
11	3.262	689	691	693	rBV2	520	249	0.01%	0.001%
12	3.387	728	730	731	rBV	388	190	0.01%	0.001%
13	3.397	731	733	736	rVB	574	261	0.01%	0.001%
14	3.445	745	748	751	rBV3	884	559	0.02%	0.003%
15	3.535	772	776	783	rVB5	951	1012	0.04%	0.005%
16	3.571	783	787	788	rBV	869	576	0.02%	0.003%
17	3.613	794	800	802	rBV4	824	719	0.03%	0.004%
18	3.622	802	803	811	rVB3	830	672	0.03%	0.003%
19	3.654	811	813	817	rBV2	667	615	0.02%	0.003%
20	3.696	822	826	828	rBV2	814	631	0.02%	0.003%
21	3.751	841	843	844	rBV	352	129	0.00%	0.001%
22	3.764	845	847	850	rVV4	611	366	0.01%	0.002%
23	3.812	860	862	864	rBV4	155	83	0.00%	0.000%
24	3.847	871	873	874	rBV2	481	146	0.01%	0.001%
25	3.889	875	886	932	rVV	179988	544182	20.74%	2.771%
26	4.352	1016	1030	1055	rBV	440907	1071867	40.85%	5.458%
27	4.815	1172	1174	1177	rBV3	792	462	0.02%	0.002%
28	4.860	1185	1188	1190	rVB3	763	380	0.01%	0.002%
29	4.873	1190	1192	1194	rBV2	1091	581	0.02%	0.003%
30	4.950	1215	1216	1219	rVB2	534	144	0.01%	0.001%
31	5.050	1229	1247	1282	rBV2	1019152	2623911	100.00%	13.361%
32	5.358	1341	1343	1347	rBV3	788	476	0.02%	0.002%
33	5.477	1377	1380	1383	rBV3	757	537	0.02%	0.003%
34	5.622	1412	1425	1455	rBV	707043	1431809	54.57%	7.291%
35	5.866	1499	1501	1503	rBV3	1336	669	0.03%	0.003%
36	5.911	1508	1515	1530	rVB3	14969	28972	1.10%	0.148%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020733.D
 Acq On : 24 Mar 2021 13:43
 Operator : SY/MD
 Sample : M1783-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.072	1552	1565	1593	rBV	563715	1157551	44.12%	5.894%
38	6.429	1674	1676	1681	rBV4	1307	872	0.03%	0.004%
39	6.500	1695	1698	1700	rBV3	734	413	0.02%	0.002%
40	6.519	1700	1704	1706	rBV4	967	864	0.03%	0.004%
41	6.670	1749	1751	1754	rBV2	979	731	0.03%	0.004%
42	6.712	1763	1764	1770	rVB4	936	593	0.02%	0.003%
43	6.744	1770	1774	1776	rBV3	1013	780	0.03%	0.004%
44	6.844	1803	1805	1813	rVB4	1401	1067	0.04%	0.005%
45	6.876	1813	1815	1818	rBV2	629	385	0.01%	0.002%
46	6.899	1818	1822	1826	rVB4	873	635	0.02%	0.003%
47	6.924	1826	1830	1832	rBV2	698	614	0.02%	0.003%
48	6.989	1839	1850	1872	rBV	322941	591348	22.54%	3.011%
49	7.320	1941	1953	1979	rBV	1223873	2070957	78.93%	10.545%
50	7.625	2038	2048	2072	rBV	236205	409658	15.61%	2.086%
51	8.091	2183	2193	2222	rBV	660267	1163983	44.36%	5.927%
52	8.622	2356	2358	2360	rBV3	801	393	0.01%	0.002%
53	8.677	2373	2375	2376	rBV	900	374	0.01%	0.002%
54	8.857	2419	2431	2460	rBV	1103354	1788216	68.15%	9.105%
55	9.111	2509	2510	2511	rBV	749	232	0.01%	0.001%
56	9.165	2519	2527	2530	rBV7	1721	2115	0.08%	0.011%
57	9.265	2556	2558	2560	rBV2	727	340	0.01%	0.002%
58	9.403	2598	2601	2602	rBV2	811	445	0.02%	0.002%
59	9.641	2672	2675	2678	rBV3	634	411	0.02%	0.002%
60	9.699	2691	2693	2696	rVB2	493	204	0.01%	0.001%
61	9.802	2723	2725	2727	rBV	522	260	0.01%	0.001%
62	9.815	2727	2729	2731	rBV2	851	507	0.02%	0.003%
63	9.953	2770	2772	2776	rVB4	923	527	0.02%	0.003%
64	9.988	2781	2783	2786	rBV3	667	491	0.02%	0.003%
65	10.114	2818	2822	2823	rBV2	503	327	0.01%	0.002%
66	10.220	2844	2855	2874	rBV	803682	1250121	47.64%	6.365%
67	10.429	2919	2920	2923	rBV	660	322	0.01%	0.002%
68	10.474	2930	2934	2937	rBV4	1223	1076	0.04%	0.005%
69	10.841	3046	3048	3050	rBV	597	361	0.01%	0.002%
70	10.905	3065	3068	3069	rBV	763	374	0.01%	0.002%
71	11.001	3096	3098	3100	rBV	558	254	0.01%	0.001%
72	11.059	3114	3116	3119	rBV3	664	319	0.01%	0.002%
73	11.165	3144	3149	3152	rBV5	2168	2150	0.08%	0.011%
74	11.255	3166	3177	3195	rBV	1145409	1767392	67.36%	8.999%
75	11.545	3259	3267	3279	rBV2	7980	15248	0.58%	0.078%
76	11.632	3282	3294	3314	rBV	1264910	2010000	76.60%	10.235%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020733.D
Acq On : 24 Mar 2021 13:43
Operator : SY/MD
Sample : M1783-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G12

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Title : VOC Analysis

77	12.014	3411	3413	3417	rBV3	1073	587	0.02%	0.003%
78	12.812	3659	3661	3663	rBV	701	331	0.01%	0.002%
79	12.844	3667	3671	3672	rBV3	1208	833	0.03%	0.004%
80	13.271	3796	3804	3818	rVB3	22887	37217	1.42%	0.190%
81	13.754	3950	3954	3968	rVB3	14431	19783	0.75%	0.101%


Sum of corrected areas: 19639296

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020733.D
Acq On : 24 Mar 2021 13:43
Operator : SY/MD
Sample : M1783-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

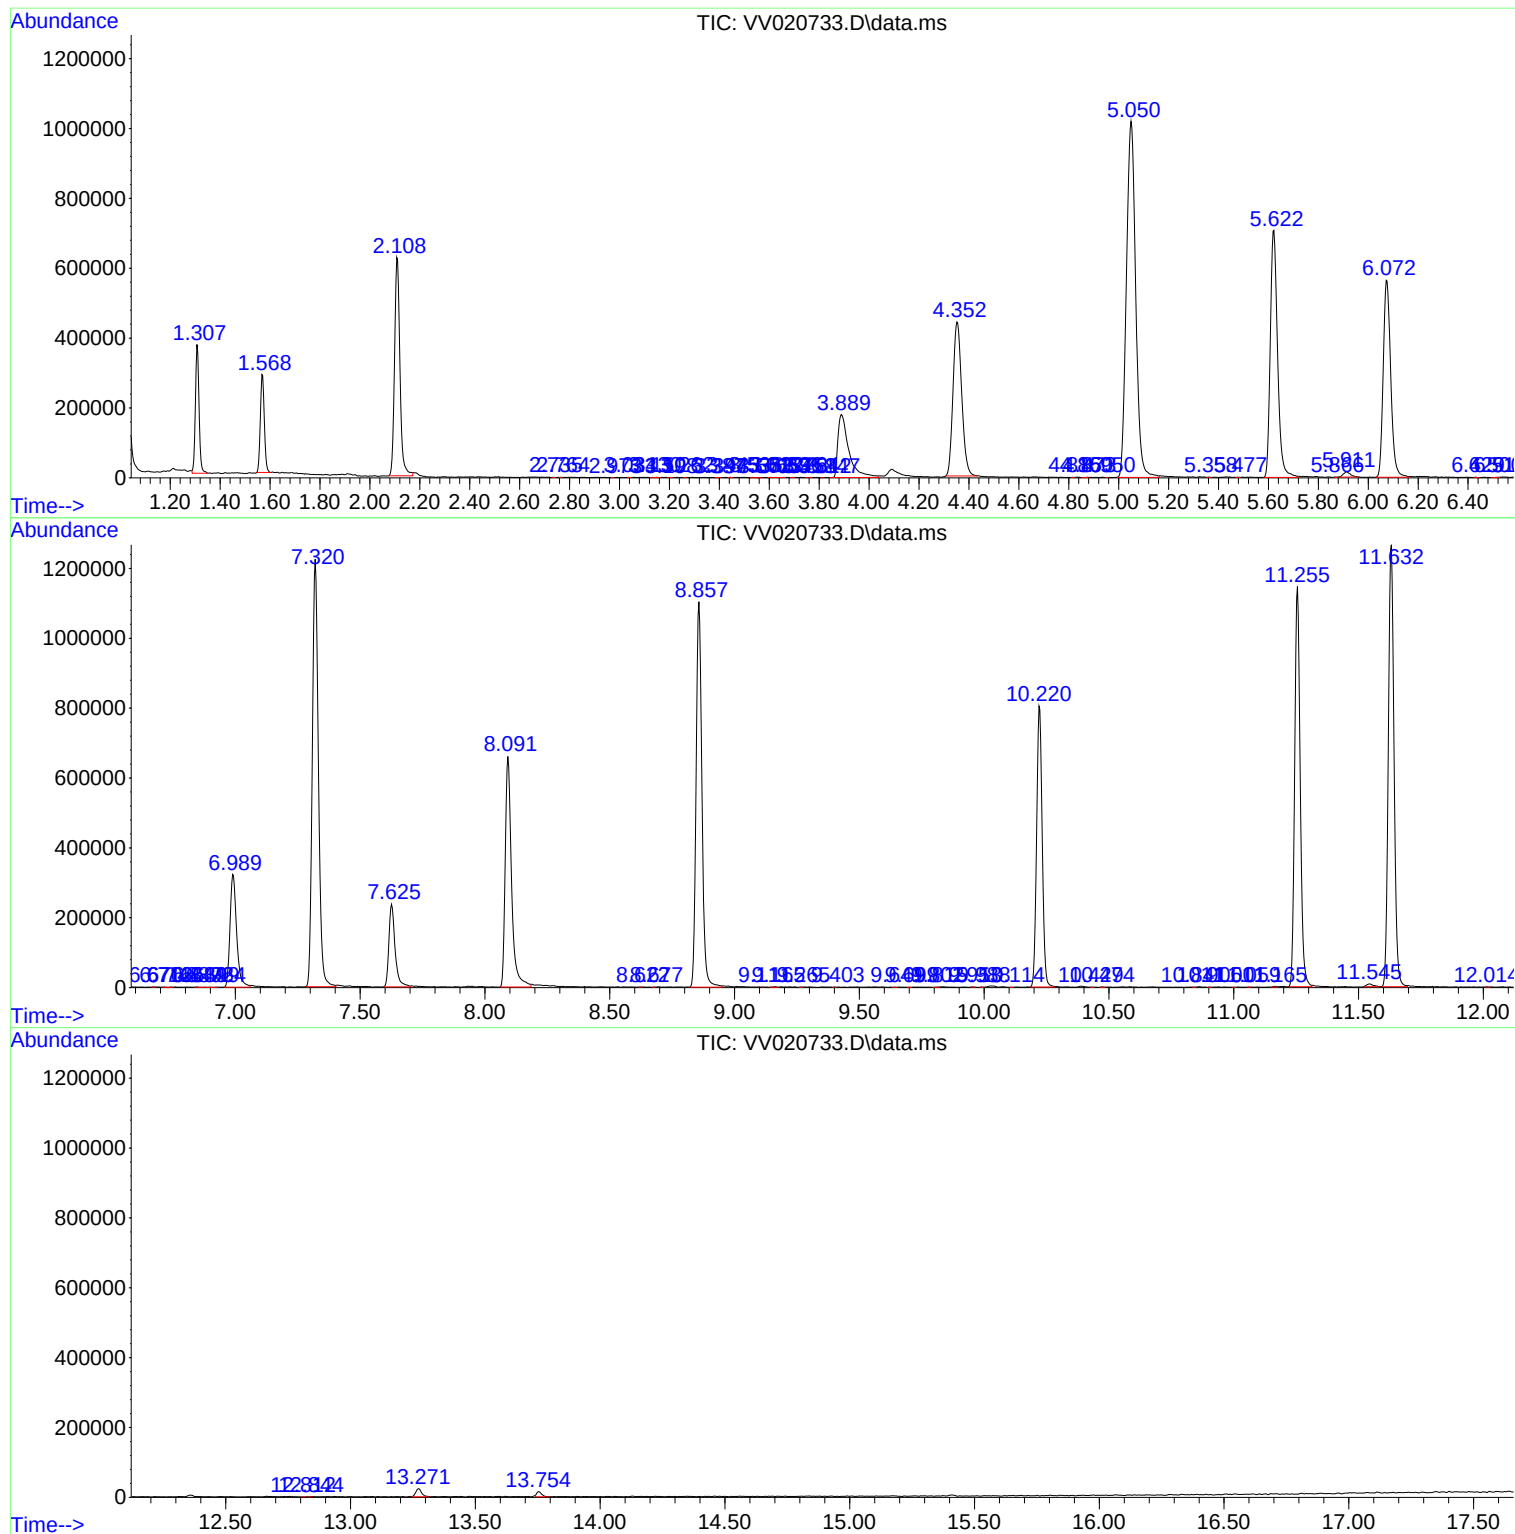

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020733.D
Acq On : 24 Mar 2021 13:43
Operator : SY/MD
Sample : M1783-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020733.D
Acq On : 24 Mar 2021 13:43
Operator : SY/MD
Sample : M1783-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
