

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020735.D
 Acq On : 24 Mar 2021 14:30
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	78	83	97	rVB	378764	386402	13.89%	1.811%
2	1.571	158	165	181	rVB	302365	338461	12.16%	1.586%
3	2.111	323	333	358	rVB	655026	994958	35.76%	4.662%
4	2.259	376	379	384	rBV5	987	947	0.03%	0.004%
5	2.654	499	502	506	rBV3	520	410	0.01%	0.002%
6	2.712	517	520	527	rBV5	577	512	0.02%	0.002%
7	2.748	529	531	535	rBV4	631	366	0.01%	0.002%
8	2.770	535	538	542	rBV3	1042	810	0.03%	0.004%
9	2.805	547	549	551	rBV	632	311	0.01%	0.001%
10	2.818	551	553	557	rVB2	666	405	0.01%	0.002%
11	2.838	557	559	563	rBV2	582	375	0.01%	0.002%
12	2.870	563	569	571	rBV3	868	863	0.03%	0.004%
13	2.895	575	577	579	rBV2	302	147	0.01%	0.001%
14	2.982	601	604	607	rBV2	564	435	0.02%	0.002%
15	3.037	619	621	623	rBV2	863	301	0.01%	0.001%
16	3.063	628	629	632	rBV	658	371	0.01%	0.002%
17	3.114	643	645	649	rVB	539	283	0.01%	0.001%
18	3.130	649	650	653	rVB2	631	305	0.01%	0.001%
19	3.159	653	659	663	rBV3	756	788	0.03%	0.004%
20	3.178	663	665	669	rBV2	662	460	0.02%	0.002%
21	3.268	687	693	696	rVB3	764	748	0.03%	0.004%
22	3.288	696	699	701	rBV2	553	409	0.01%	0.002%
23	3.313	706	707	709	rBV	446	209	0.01%	0.001%
24	3.358	720	721	723	rBV	467	216	0.01%	0.001%
25	3.397	726	733	738	rVV5	853	1305	0.05%	0.006%
26	3.461	751	753	757	rBV4	690	432	0.02%	0.002%
27	3.494	761	763	764	rBV	508	189	0.01%	0.001%
28	3.532	772	775	776	rBV	371	215	0.01%	0.001%
29	3.587	786	792	795	rVB3	783	819	0.03%	0.004%
30	3.612	795	800	803	rBV3	699	714	0.03%	0.003%
31	3.641	807	809	812	rBV3	392	254	0.01%	0.001%
32	3.661	812	815	817	rVB2	933	548	0.02%	0.003%
33	3.719	831	833	837	rVB4	595	344	0.01%	0.002%
34	3.738	837	839	841	rBV3	660	244	0.01%	0.001%
35	3.757	843	845	846	rBV	475	205	0.01%	0.001%
36	3.786	853	854	857	rBV2	328	95	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020735.D
 Acq On : 24 Mar 2021 14:30
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	3.799	857	858	862	rBV2	467	295	0.01%	0.001%
38	3.889	876	886	928	rBV	187000	547046	19.66%	2.563%
39	4.352	1016	1030	1066	rVB	472445	1154959	41.51%	5.412%
40	4.651	1119	1123	1127	rBV6	1066	1156	0.04%	0.005%
41	4.854	1184	1186	1188	rVB3	676	295	0.01%	0.001%
42	4.879	1192	1194	1196	rVV2	819	441	0.02%	0.002%
43	4.902	1199	1201	1204	rVV2	633	343	0.01%	0.002%
44	4.982	1224	1226	1229	rVB3	546	226	0.01%	0.001%
45	5.050	1229	1247	1281	rBV2	1071730	2782367	100.00%	13.038%
46	5.461	1372	1375	1380	rBV5	990	1062	0.04%	0.005%
47	5.622	1412	1425	1456	rBV	836425	1688447	60.68%	7.912%
48	6.075	1552	1566	1592	rBV	606330	1228982	44.17%	5.759%
49	6.349	1650	1651	1655	rVB4	957	558	0.02%	0.003%
50	6.371	1655	1658	1662	rBV3	1287	1237	0.04%	0.006%
51	6.513	1700	1702	1706	rBV3	790	497	0.02%	0.002%
52	6.564	1715	1718	1719	rBV3	707	425	0.02%	0.002%
53	6.606	1729	1731	1734	rVB2	1014	505	0.02%	0.002%
54	6.718	1765	1766	1767	rBV2	412	155	0.01%	0.001%
55	6.828	1798	1800	1805	rVB3	740	594	0.02%	0.003%
56	6.860	1805	1810	1812	rBV3	1011	938	0.03%	0.004%
57	6.908	1822	1825	1827	rBV3	428	306	0.01%	0.001%
58	6.950	1836	1838	1839	rBV	435	129	0.00%	0.001%
59	6.989	1839	1850	1878	rBV	339420	623921	22.42%	2.924%
60	7.320	1941	1953	1977	rBV	1285272	2201462	79.12%	10.316%
61	7.625	2038	2048	2070	rBV	241802	429255	15.43%	2.011%
62	7.918	2137	2139	2141	rBV	831	370	0.01%	0.002%
63	8.011	2166	2168	2170	rBV3	1036	508	0.02%	0.002%
64	8.091	2183	2193	2220	rBV	689137	1208408	43.43%	5.662%
65	8.554	2334	2337	2341	rBV6	1057	946	0.03%	0.004%
66	8.574	2341	2343	2346	rVB2	1061	580	0.02%	0.003%
67	8.590	2346	2348	2350	rBV3	1010	578	0.02%	0.003%
68	8.776	2404	2406	2407	rBV2	466	152	0.01%	0.001%
69	8.802	2413	2414	2415	rBV	516	157	0.01%	0.001%
70	8.857	2418	2431	2462	rBV	1284687	2116467	76.07%	9.917%
71	9.477	2621	2624	2626	rBV2	782	564	0.02%	0.003%
72	9.644	2673	2676	2679	rBV4	671	480	0.02%	0.002%
73	9.660	2679	2681	2682	rBV2	550	190	0.01%	0.001%
74	9.725	2699	2701	2702	rBV2	460	216	0.01%	0.001%
75	9.831	2732	2734	2735	rBV	539	202	0.01%	0.001%
76	9.895	2752	2754	2755	rBV	459	129	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020735.D
 Acq On : 24 Mar 2021 14:30
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.220	2844	2855	2880	rVB	856183	1349470	48.50%	6.323%
78	10.487	2936	2938	2940	rVB3	1058	386	0.01%	0.002%
79	10.500	2940	2942	2944	rBV2	755	325	0.01%	0.002%
80	10.583	2965	2968	2971	rBV4	1253	1060	0.04%	0.005%
81	10.676	2995	2997	2999	rBV2	1145	433	0.02%	0.002%
82	10.718	3008	3010	3012	rBV	636	317	0.01%	0.001%
83	10.853	3050	3052	3057	rBV4	1211	907	0.03%	0.004%
84	10.918	3070	3072	3073	rBV2	662	321	0.01%	0.002%
85	11.255	3165	3177	3201	rBV	1345350	2076752	74.64%	9.731%
86	11.631	3278	3294	3317	rBV	1361859	2149835	77.27%	10.074%
87	11.921	3382	3384	3389	rBV4	1200	1080	0.04%	0.005%
88	12.496	3560	3563	3565	rBV3	729	384	0.01%	0.002%
89	12.635	3602	3606	3609	rBV2	1253	1243	0.04%	0.006%
90	12.930	3696	3698	3701	rBV	728	443	0.02%	0.002%
91	13.274	3797	3805	3819	rVB5	16037	26868	0.97%	0.126%
92	14.326	4129	4132	4134	rBV	1257	840	0.03%	0.004%


Sum of corrected areas: 21341068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020735.D
Acq On : 24 Mar 2021 14:30
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

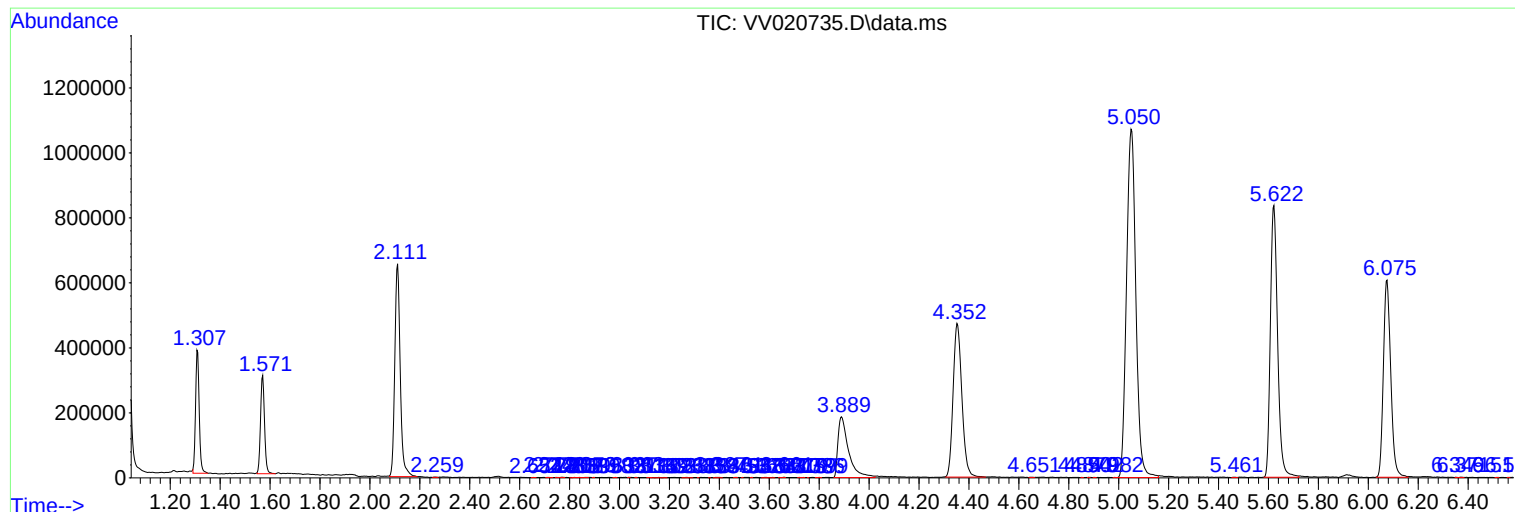

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020735.D
Acq On : 24 Mar 2021 14:30
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020735.D
Acq On : 24 Mar 2021 14:30
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
