

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020736.D
 Acq On : 24 Mar 2021 14:54
 Operator : SY/MD
 Sample : M1783-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G11DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	99	rVB	353430	362903	7.45%	1.459%
2	1.571	158	165	176	rVB	293726	321746	6.60%	1.293%
3	2.111	323	333	367	rVB	640665	985403	20.22%	3.961%
4	2.355	407	409	414	rBV3	697	536	0.01%	0.002%
5	2.513	451	458	468	rVB7	3657	5885	0.12%	0.024%
6	2.571	474	476	480	rVB4	681	313	0.01%	0.001%
7	2.690	511	513	515	rBV	778	293	0.01%	0.001%
8	2.741	526	529	534	rBV3	605	554	0.01%	0.002%
9	2.828	553	556	560	rBV4	1232	884	0.02%	0.004%
10	2.876	569	571	573	rBV	770	426	0.01%	0.002%
11	2.918	582	584	586	rVV	570	266	0.01%	0.001%
12	2.944	590	592	595	rVB3	652	372	0.01%	0.001%
13	3.005	607	611	614	rBV3	613	569	0.01%	0.002%
14	3.072	629	632	635	rBV3	603	381	0.01%	0.002%
15	3.095	635	639	644	rBV4	479	390	0.01%	0.002%
16	3.121	644	647	649	rBV2	646	289	0.01%	0.001%
17	3.207	671	674	679	rVB3	970	759	0.02%	0.003%
18	3.236	679	683	686	rVB3	967	742	0.02%	0.003%
19	3.256	686	689	694	rBV4	805	911	0.02%	0.004%
20	3.336	710	714	715	rBV	548	324	0.01%	0.001%
21	3.442	740	747	749	rBV2	377	427	0.01%	0.002%
22	3.500	762	765	766	rBV3	481	269	0.01%	0.001%
23	3.564	778	785	787	rBV5	1207	1191	0.02%	0.005%
24	3.580	787	790	792	rVV	424	280	0.01%	0.001%
25	3.606	795	798	801	rBV2	804	467	0.01%	0.002%
26	3.677	816	820	824	rBV5	902	744	0.02%	0.003%
27	3.696	824	826	830	rBV3	556	354	0.01%	0.001%
28	3.725	832	835	838	rVB2	837	424	0.01%	0.002%
29	3.757	842	845	846	rBV2	616	339	0.01%	0.001%
30	3.892	872	887	916	rBV	214509	651514	13.37%	2.619%
31	4.352	1014	1030	1069	rVB	501782	1231157	25.26%	4.949%
32	4.725	1144	1146	1149	rBV4	975	480	0.01%	0.002%
33	4.783	1162	1164	1165	rBV2	676	301	0.01%	0.001%
34	4.847	1180	1184	1187	rBV5	819	571	0.01%	0.002%
35	4.863	1187	1189	1190	rBV2	764	349	0.01%	0.001%
36	4.973	1219	1223	1224	rBV3	958	529	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020736.D
 Acq On : 24 Mar 2021 14:54
 Operator : SY/MD
 Sample : M1783-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G11DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

37	5.050	1229	1247	1280	rBV3	1126825	2920697	59.94%	11.741%
38	5.500	1384	1387	1389	rVB3	899	461	0.01%	0.002%
39	5.622	1409	1425	1458	rBV	521722	1056618	21.68%	4.248%
40	6.075	1552	1566	1596	rBV	634170	1291067	26.49%	5.190%
41	6.326	1640	1644	1649	rBV4	1091	1230	0.03%	0.005%
42	6.384	1660	1662	1665	rBV3	852	415	0.01%	0.002%
43	6.445	1679	1681	1686	rVB4	747	571	0.01%	0.002%
44	6.522	1703	1705	1707	rBV2	1010	625	0.01%	0.003%
45	6.558	1713	1716	1719	rBV3	565	440	0.01%	0.002%
46	6.648	1740	1744	1745	rBV3	1282	875	0.02%	0.004%
47	6.670	1748	1751	1754	rBV3	1146	816	0.02%	0.003%
48	6.735	1768	1771	1773	rBV	895	624	0.01%	0.003%
49	6.805	1790	1793	1795	rBV4	935	396	0.01%	0.002%
50	6.870	1811	1813	1816	rVB2	876	441	0.01%	0.002%
51	6.886	1816	1818	1820	rBV	554	335	0.01%	0.001%
52	6.934	1830	1833	1838	rVB4	769	594	0.01%	0.002%
53	6.989	1838	1850	1876	rBV	360700	659563	13.53%	2.651%
54	7.320	1941	1953	1978	rBV	1297469	2235772	45.88%	8.988%
55	7.625	2038	2048	2068	rBV	259150	448709	9.21%	1.804%
56	8.037	2172	2176	2179	rBV3	1173	899	0.02%	0.004%
57	8.091	2182	2193	2225	rBV	821207	1430880	29.36%	5.752%
58	8.664	2368	2371	2372	rBV2	829	508	0.01%	0.002%
59	8.770	2401	2404	2405	rBV	905	423	0.01%	0.002%
60	8.799	2411	2413	2416	rVB2	804	382	0.01%	0.002%
61	8.812	2416	2417	2419	rBV	599	288	0.01%	0.001%
62	8.857	2419	2431	2438	rBV	841371	1457550	29.91%	5.859%
63	9.069	2496	2497	2499	rBV2	864	340	0.01%	0.001%
64	9.252	2551	2554	2556	rBV2	841	482	0.01%	0.002%
65	9.310	2570	2572	2575	rVB3	679	333	0.01%	0.001%
66	9.394	2593	2598	2602	rBV3	920	740	0.02%	0.003%
67	9.413	2602	2604	2605	rBV	895	392	0.01%	0.002%
68	9.480	2623	2625	2627	rBV2	533	273	0.01%	0.001%
69	9.574	2652	2654	2657	rBV3	651	381	0.01%	0.002%
70	9.699	2691	2693	2694	rBV	620	322	0.01%	0.001%
71	9.767	2710	2714	2715	rBV3	725	488	0.01%	0.002%
72	9.802	2722	2725	2729	rBV6	1068	726	0.01%	0.003%
73	9.988	2780	2783	2786	rVB2	691	364	0.01%	0.001%
74	10.053	2801	2803	2807	rBV4	608	447	0.01%	0.002%
75	10.136	2827	2829	2834	rVB2	1241	778	0.02%	0.003%
76	10.220	2843	2855	2879	rBV	952268	1510566	31.00%	6.072%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020736.D
 Acq On : 24 Mar 2021 14:54
 Operator : SY/MD
 Sample : M1783-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G11DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.378	2902	2904	2907	rBV2	926	619	0.01%	0.002%
78	10.503	2941	2943	2949	rVB5	995	587	0.01%	0.002%
79	10.548	2955	2957	2959	rBV2	729	294	0.01%	0.001%
80	10.776	3026	3028	3031	rVB	870	468	0.01%	0.002%
81	10.812	3035	3039	3042	rBV2	765	652	0.01%	0.003%
82	10.863	3051	3055	3062	rVB6	1997	2303	0.05%	0.009%
83	10.911	3068	3070	3073	rBV3	726	615	0.01%	0.002%
84	11.072	3118	3120	3123	rBV2	697	284	0.01%	0.001%
85	11.098	3124	3128	3131	rBV5	749	680	0.01%	0.003%
86	11.191	3145	3157	3166	rBV	63730	100364	2.06%	0.403%
87	11.255	3166	3177	3201	rVV2	906618	2200430	45.15%	8.846%
88	11.448	3235	3237	3239	rBV2	1000	453	0.01%	0.002%
89	11.644	3280	3298	3321	rBV2	2110052	4873087	100.00%	19.589%
90	12.024	3414	3416	3418	rBV3	1127	549	0.01%	0.002%
91	12.159	3456	3458	3462	rVB3	942	578	0.01%	0.002%
92	12.310	3502	3505	3506	rBV2	749	347	0.01%	0.001%
93	12.484	3556	3559	3560	rBV4	655	348	0.01%	0.001%
94	12.541	3573	3577	3580	rBV	662	597	0.01%	0.002%
95	12.654	3605	3612	3623	rBV2	10514	16565	0.34%	0.067%
96	12.757	3634	3644	3646	rBV7	4510	6463	0.13%	0.026%
97	13.149	3764	3766	3768	rBV2	1143	517	0.01%	0.002%
98	13.268	3792	3803	3820	rBV	462876	713866	14.65%	2.870%
99	13.673	3927	3929	3931	rBV	985	549	0.01%	0.002%
100	13.750	3943	3953	3968	rBV	223496	353697	7.26%	1.422%




Sum of corrected areas: 24876065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020736.D
Acq On : 24 Mar 2021 14:54
Operator : SY/MD
Sample : M1783-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G11DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

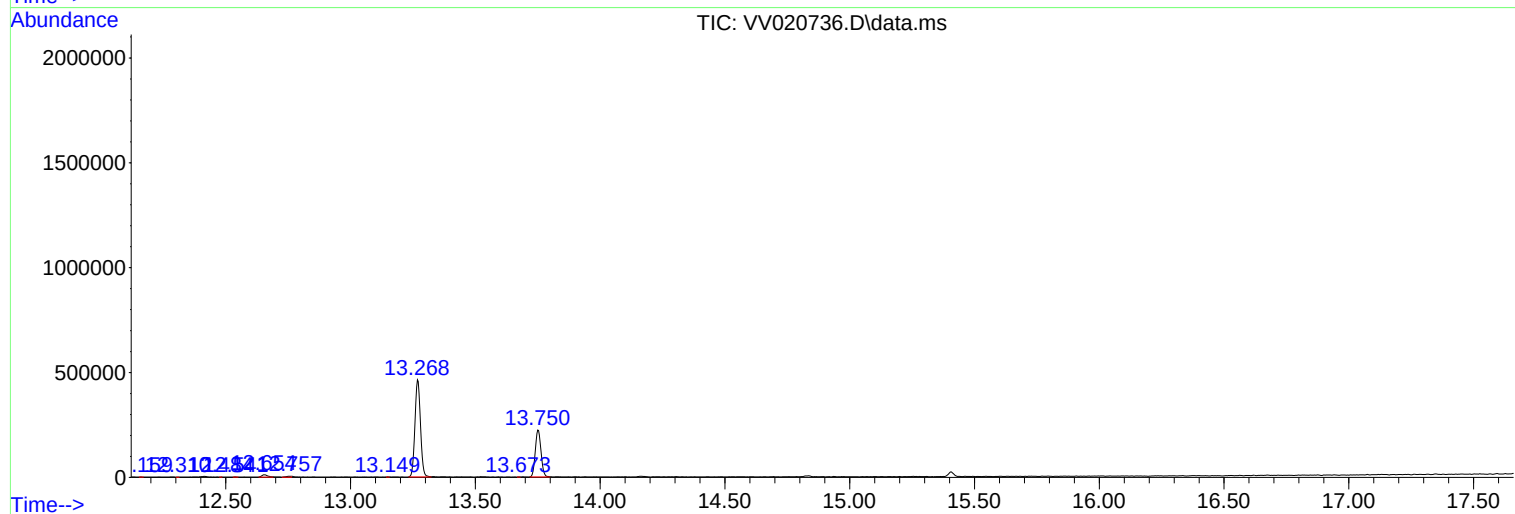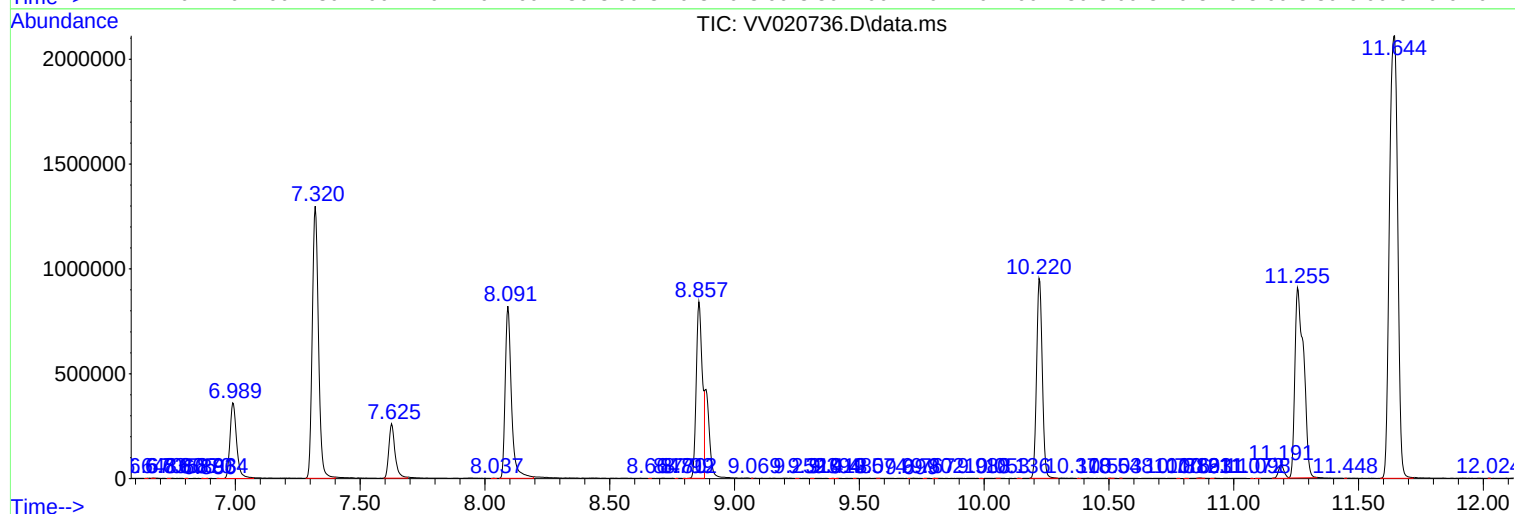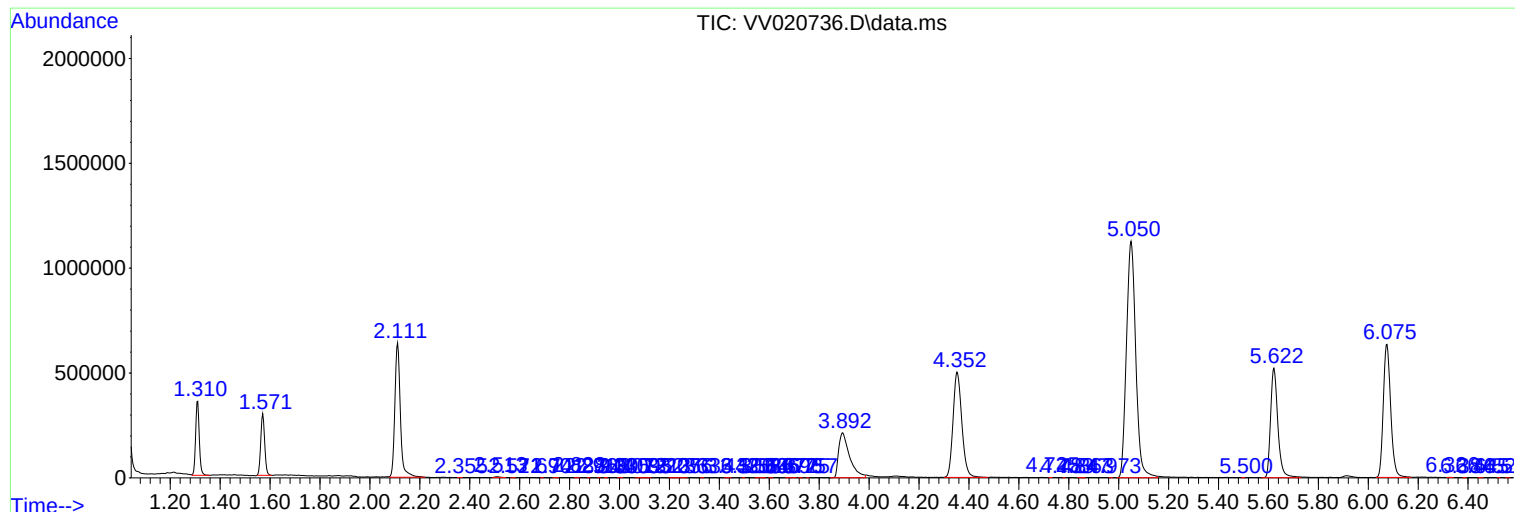

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020736.D
Acq On : 24 Mar 2021 14:54
Operator : SY/MD
Sample : M1783-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G11DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020736.D
Acq On : 24 Mar 2021 14:54
Operator : SY/MD
Sample : M1783-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G11DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
