

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020741.D
 Acq On : 24 Mar 2021 16:51
 Operator : SY/MD
 Sample : M1783-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G11DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	78	83	95	rVB	306008	302635	6.83%	1.218%
2	1.568	158	164	176	rVB	255756	284432	6.42%	1.144%
3	2.111	323	333	363	rVB	537790	833255	18.81%	3.352%
4	2.352	404	408	410	rBV2	892	682	0.02%	0.003%
5	2.429	430	432	434	rBV2	717	331	0.01%	0.001%
6	2.462	440	442	445	rBV3	678	350	0.01%	0.001%
7	2.478	445	447	449	rBV2	999	502	0.01%	0.002%
8	2.610	485	488	490	rBV3	1354	852	0.02%	0.003%
9	2.687	510	512	514	rBV2	643	308	0.01%	0.001%
10	2.728	520	525	527	rBV2	458	312	0.01%	0.001%
11	2.764	532	536	537	rBV2	613	380	0.01%	0.002%
12	2.931	587	588	592	rVB2	754	324	0.01%	0.001%
13	2.970	596	600	602	rVV3	885	477	0.01%	0.002%
14	2.995	606	608	611	rVB2	338	188	0.00%	0.001%
15	3.018	611	615	618	rBV2	746	648	0.01%	0.003%
16	3.040	620	622	625	rBV2	692	375	0.01%	0.002%
17	3.079	632	634	635	rBV	399	105	0.00%	0.000%
18	3.195	664	670	671	rBV4	533	359	0.01%	0.001%
19	3.214	673	676	677	rBV3	905	431	0.01%	0.002%
20	3.243	683	685	688	rBV4	465	284	0.01%	0.001%
21	3.323	707	710	714	rBV4	750	634	0.01%	0.003%
22	3.462	751	753	758	rVB3	857	520	0.01%	0.002%
23	3.503	763	766	771	rBV4	433	436	0.01%	0.002%
24	3.523	771	772	775	rBV2	399	224	0.01%	0.001%
25	3.555	779	782	783	rBV	467	217	0.00%	0.001%
26	3.564	783	785	787	rBV2	499	263	0.01%	0.001%
27	3.606	795	798	799	rBV2	1006	453	0.01%	0.002%
28	3.632	804	806	807	rVB2	644	178	0.00%	0.001%
29	3.728	833	836	837	rBV3	531	243	0.01%	0.001%
30	3.764	846	847	849	rBV	329	99	0.00%	0.000%
31	3.777	849	851	853	rVB2	696	228	0.01%	0.001%
32	3.790	853	855	858	rBV2	637	297	0.01%	0.001%
33	3.818	863	864	868	rBV2	446	168	0.00%	0.001%
34	3.886	875	885	915	rBV2	184874	533778	12.05%	2.148%
35	4.352	1016	1030	1053	rBV	420222	1027340	23.19%	4.133%
36	4.828	1175	1178	1183	rBV5	1005	845	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020741.D
 Acq On : 24 Mar 2021 16:51
 Operator : SY/MD
 Sample : M1783-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G11DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.889	1195	1197	1199	rBV	721	378	0.01%	0.002%
38	5.050	1230	1247	1276	rBV2	940531	2471736	55.79%	9.945%
39	5.352	1339	1341	1343	rBV3	709	371	0.01%	0.001%
40	5.490	1381	1384	1386	rBV	1161	555	0.01%	0.002%
41	5.555	1402	1404	1411	rVB5	735	648	0.01%	0.003%
42	5.622	1412	1425	1451	rBV	842303	1701472	38.41%	6.846%
43	5.915	1508	1516	1527	rBV9	7733	14722	0.33%	0.059%
44	6.072	1551	1565	1597	rBV	546184	1115839	25.19%	4.489%
45	6.307	1635	1638	1643	rBV6	932	659	0.01%	0.003%
46	6.349	1646	1651	1653	rBV5	904	767	0.02%	0.003%
47	6.362	1653	1655	1659	rBV3	681	504	0.01%	0.002%
48	6.429	1672	1676	1677	rBV	808	452	0.01%	0.002%
49	6.439	1677	1679	1681	rBV2	769	334	0.01%	0.001%
50	6.478	1689	1691	1694	rBV3	740	417	0.01%	0.002%
51	6.516	1700	1703	1707	rBV4	958	671	0.02%	0.003%
52	6.558	1714	1716	1719	rBV4	848	517	0.01%	0.002%
53	6.597	1726	1728	1730	rVB3	656	239	0.01%	0.001%
54	6.609	1730	1732	1734	rBV2	512	259	0.01%	0.001%
55	6.738	1770	1772	1777	rBV5	1023	669	0.02%	0.003%
56	6.941	1832	1835	1839	rBV2	1030	669	0.02%	0.003%
57	6.989	1839	1850	1873	rBV	305072	557990	12.60%	2.245%
58	7.262	1933	1935	1938	rBV2	850	510	0.01%	0.002%
59	7.320	1941	1953	1978	rBV	1099344	1889358	42.65%	7.601%
60	7.625	2037	2048	2074	rBV2	218237	386586	8.73%	1.555%
61	8.092	2182	2193	2228	rBV	661043	1157113	26.12%	4.655%
62	8.622	2354	2358	2361	rBV4	1267	1098	0.02%	0.004%
63	8.674	2368	2374	2378	rBV4	1274	1500	0.03%	0.006%
64	8.703	2381	2383	2384	rBV2	574	204	0.00%	0.001%
65	8.757	2398	2400	2401	rBV2	869	364	0.01%	0.001%
66	8.789	2408	2410	2412	rBV	519	308	0.01%	0.001%
67	8.857	2416	2431	2463	rBV2	1350082	2735222	61.74%	11.005%
68	9.320	2572	2575	2581	rVB4	1111	969	0.02%	0.004%
69	9.349	2581	2584	2586	rBV2	725	375	0.01%	0.002%
70	9.674	2678	2685	2688	rBV4	1138	1447	0.03%	0.006%
71	9.725	2697	2701	2702	rBV4	1033	626	0.01%	0.003%
72	9.754	2708	2710	2711	rBV	538	197	0.00%	0.001%
73	9.815	2726	2729	2731	rVB4	940	487	0.01%	0.002%
74	9.860	2741	2743	2744	rBV	476	161	0.00%	0.001%
75	9.902	2754	2756	2758	rBV	503	260	0.01%	0.001%
76	10.027	2792	2795	2797	rBV3	875	515	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020741.D
 Acq On : 24 Mar 2021 16:51
 Operator : SY/MD
 Sample : M1783-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G11DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.088	2811	2814	2815	rBV2	555	356	0.01%	0.001%
78	10.220	2838	2855	2876	rBV	829763	1287206	29.06%	5.179%
79	10.680	2997	2998	3000	rBV	854	277	0.01%	0.001%
80	10.796	3030	3034	3036	rBV3	755	587	0.01%	0.002%
81	10.850	3046	3051	3053	rBV3	1063	830	0.02%	0.003%
82	11.191	3147	3157	3166	rBV2	57856	95198	2.15%	0.383%
83	11.255	3166	3177	3204	rVB2	1437658	2957758	66.77%	11.900%
84	11.645	3279	3298	3320	rBV3	1970484	4430083	100.00%	17.824%
85	12.368	3519	3523	3529	rBV6	1612	2221	0.05%	0.009%
86	12.651	3605	3611	3624	rVB5	7515	13107	0.30%	0.053%
87	12.882	3681	3683	3684	rBV	791	281	0.01%	0.001%
88	13.268	3792	3803	3821	rBV	445197	685794	15.48%	2.759%
89	13.751	3942	3953	3967	rBV	216803	340620	7.69%	1.370%
90	13.866	3987	3989	3992	rBV3	883	537	0.01%	0.002%

Sum of corrected areas: 24855176




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020741.D
Acq On : 24 Mar 2021 16:51
Operator : SY/MD
Sample : M1783-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G11DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L

TIC Integration Parameters: LSCINT.P

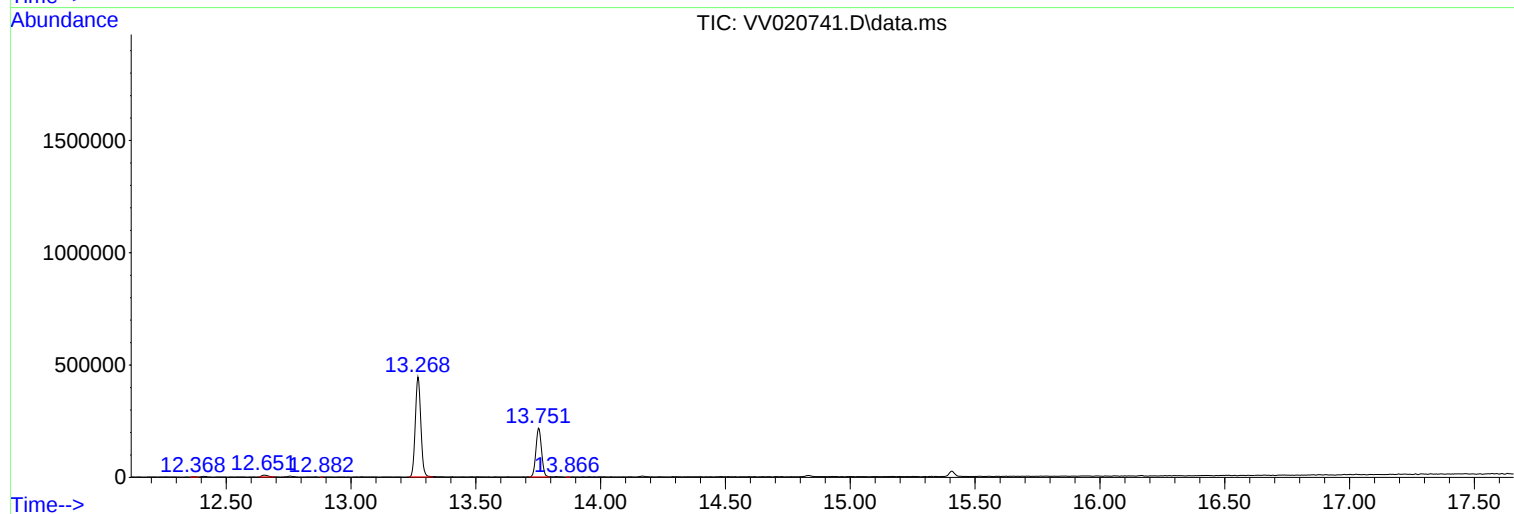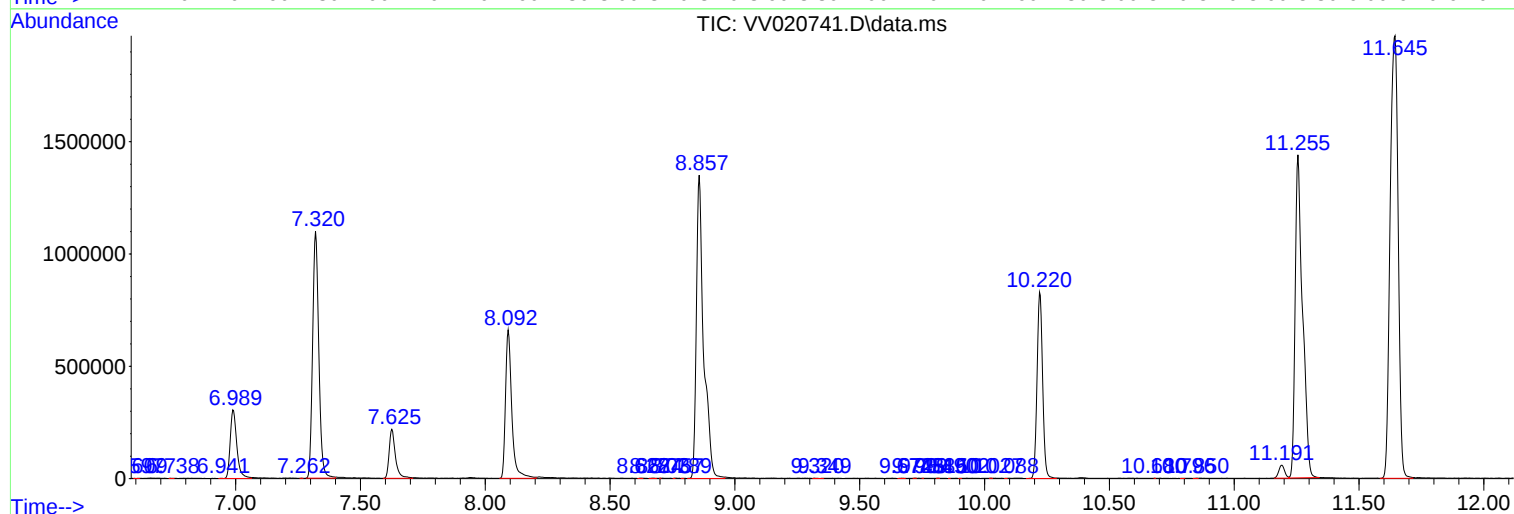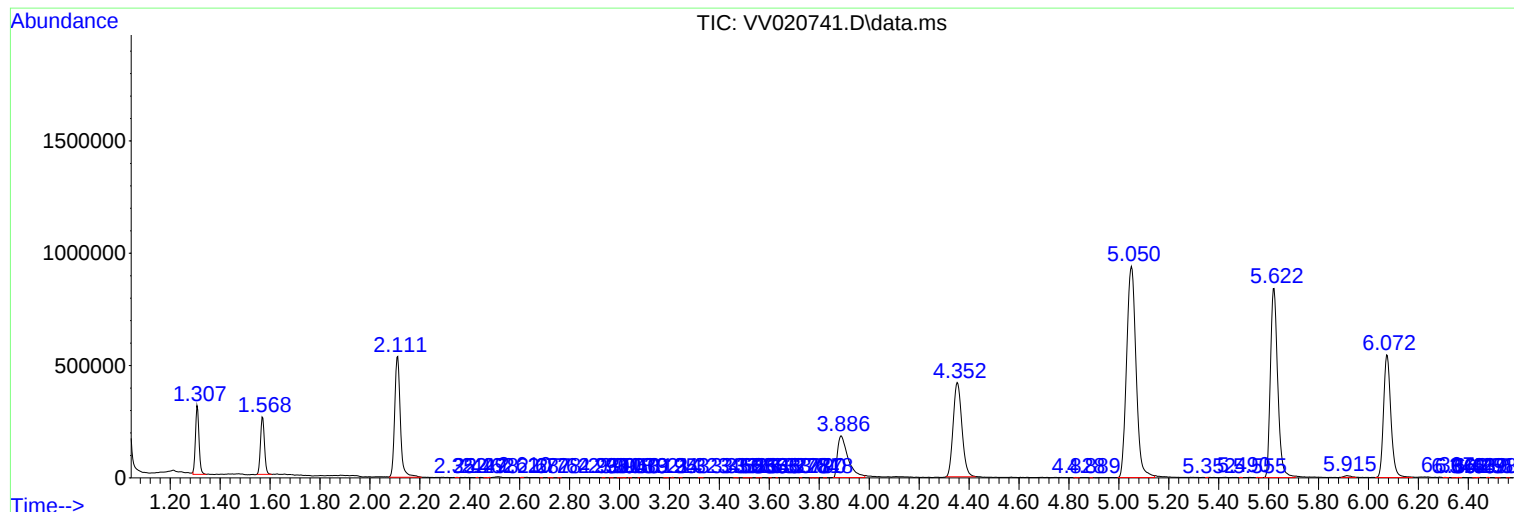

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020741.D
Acq On : 24 Mar 2021 16:51
Operator : SY/MD
Sample : M1783-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G11DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020741.D
Acq On : 24 Mar 2021 16:51
Operator : SY/MD
Sample : M1783-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G11DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------